

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122019\
 Data File : FB023285.D
 Signal(s) : FID2B.CH
 Acq On : 20 Dec 2019 11:06
 Operator : DD/AJ
 Sample : BSF1220S1
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 20 20:25:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	446630	18.834 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.684	920123	29.730 ng/ml
2) t 2,2,4-Trimethylpentane	7.410	1012437	30.307 ng/ml
3) t n-Heptane	7.749	329669	9.994 ng/ml
4) t Benzene	7.885	388514	9.729 ng/ml
6) t Toluene	10.622	1146731	29.782 ng/ml
7) t Ethylbenzene	13.062	367928	10.137 ng/ml
8) t m-Xylene	13.195	700684	20.186 ng/ml
9) t O-Xylene	13.923	681799	20.242 ng/ml
10) t 1,2,4-Trimethylbenzene	16.201	573022	20.423 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122019\
Data File : FB023285.D
Signal(s) : FID2B.CH
Acq On : 20 Dec 2019 11:06
Operator : DD/AJ
Sample : BSF1220S1
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 20 20:25:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

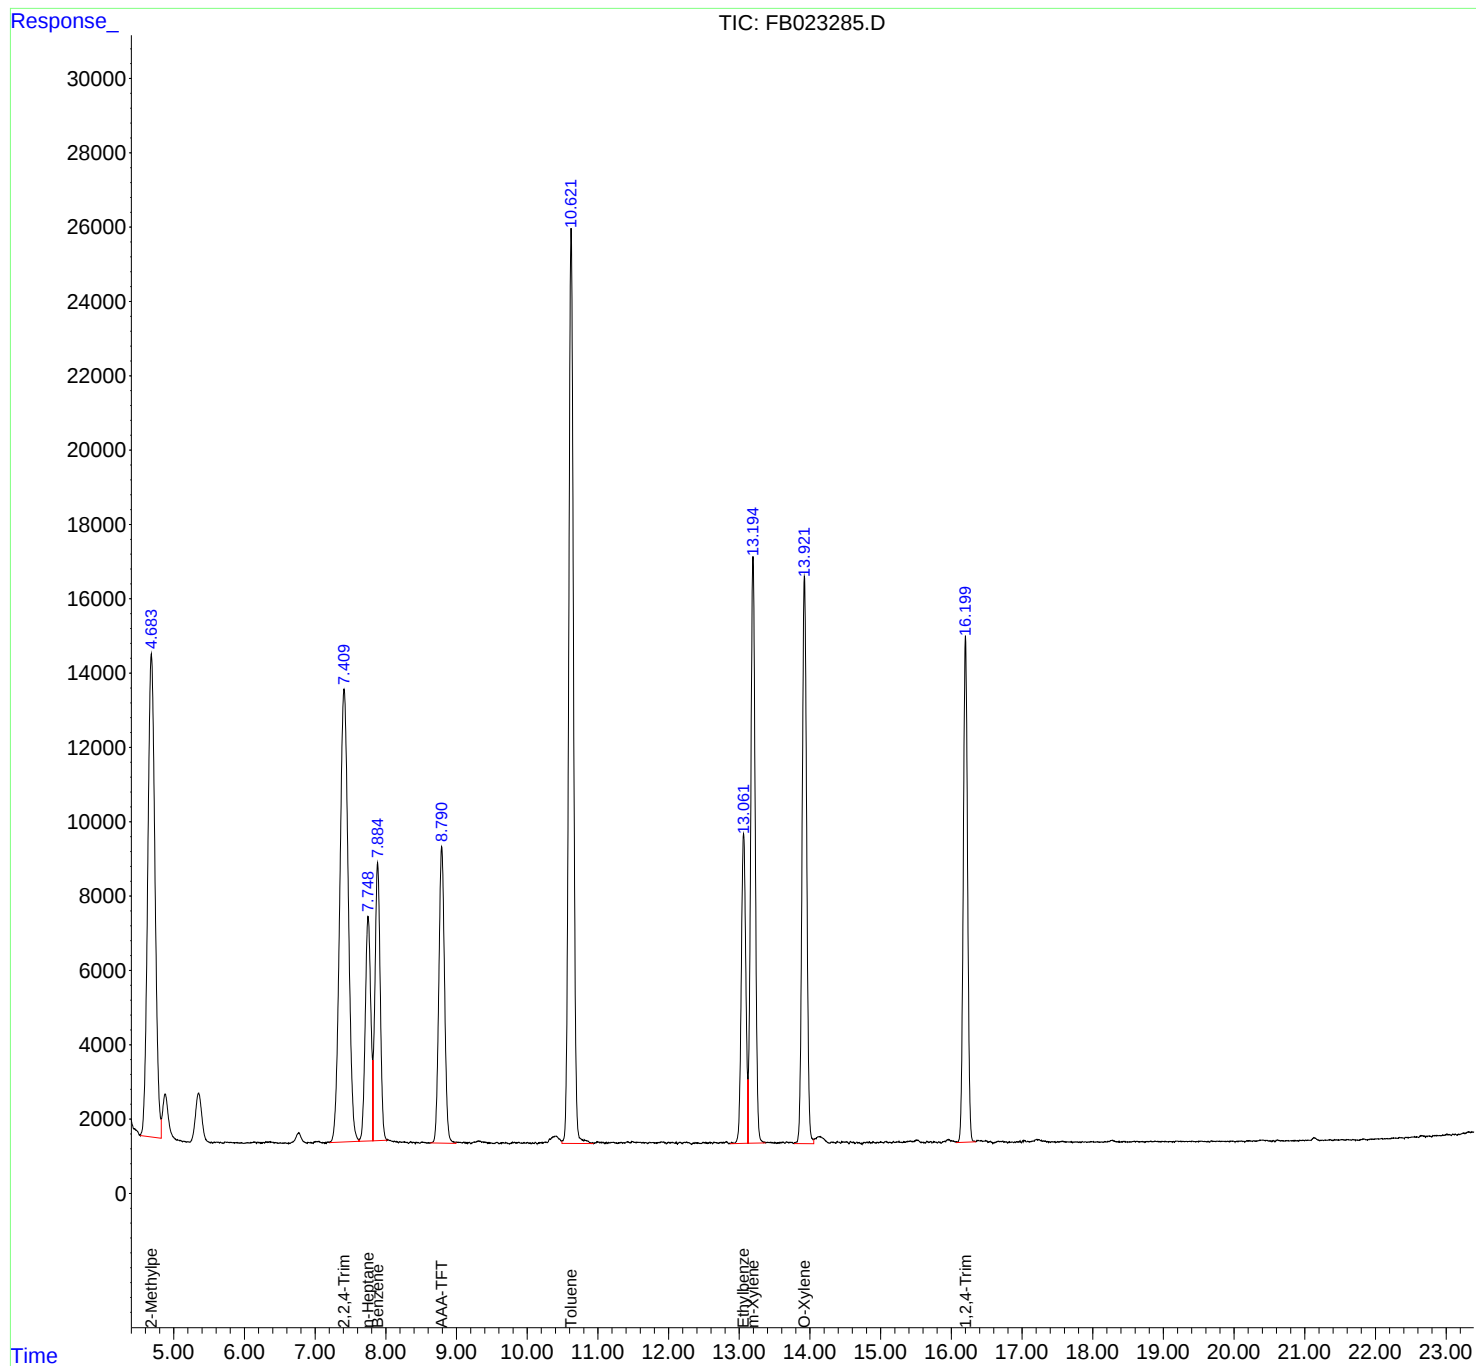

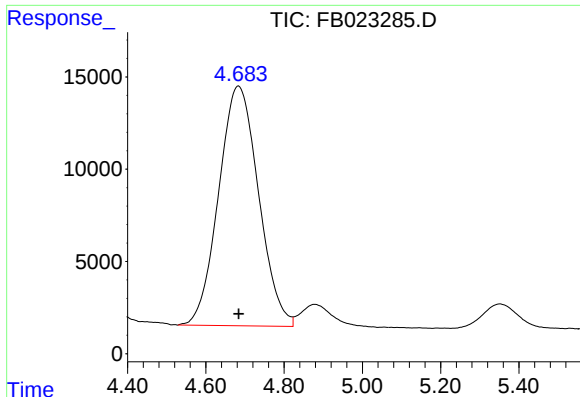


#1 2-Methylpentane

R.T.: 4.684 min
Delta R.T.: 0.000 min
Response: 920123
Conc: 29.73 ng/ml

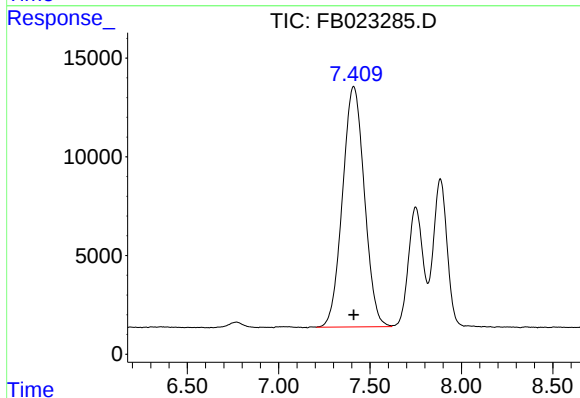


#2 2,2,4-Trimethylpentane

R.T.: 7.410 min
Delta R.T.: -0.001 min
Response: 1012437
Conc: 30.31 ng/ml

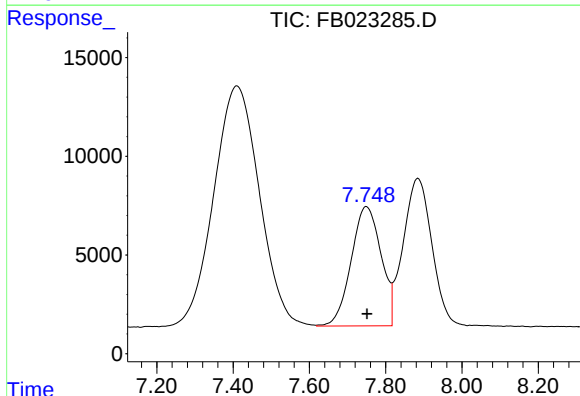


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.002 min
Response: 329669
Conc: 9.99 ng/ml

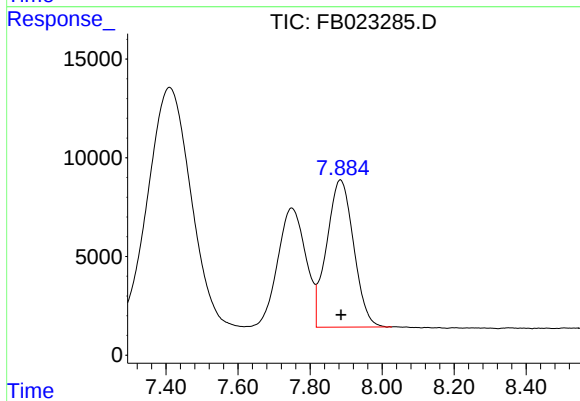


#4 Benzene

R.T.: 7.885 min
Delta R.T.: -0.002 min
Response: 388514
Conc: 9.73 ng/ml

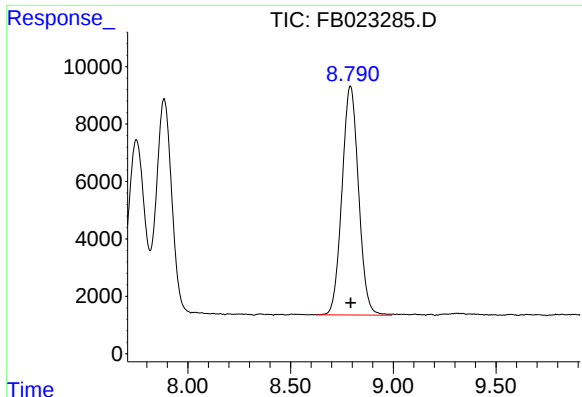


#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: -0.001 min
Response: 446630
Conc: 18.83 ng/ml

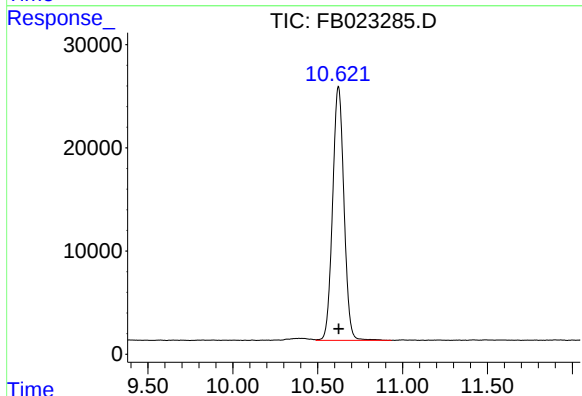


#6 Toluene

R.T.: 10.622 min
Delta R.T.: -0.001 min
Response: 1146731
Conc: 29.78 ng/ml

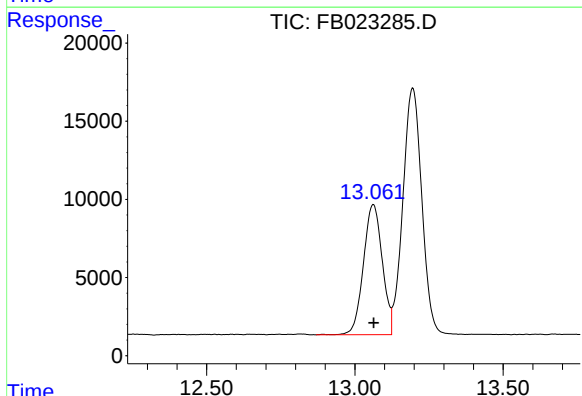


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: -0.002 min
Response: 367928
Conc: 10.14 ng/ml

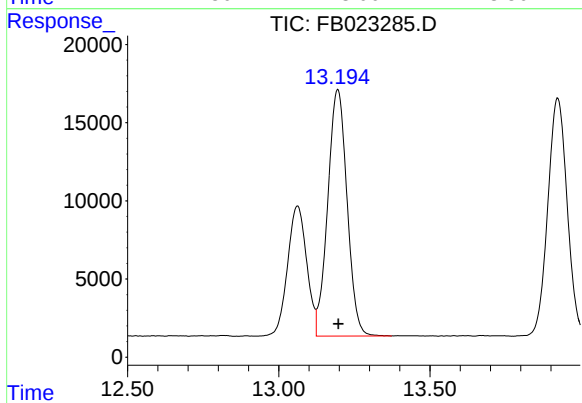


#8 m-Xylene

R.T.: 13.195 min
Delta R.T.: -0.002 min
Response: 700684
Conc: 20.19 ng/ml

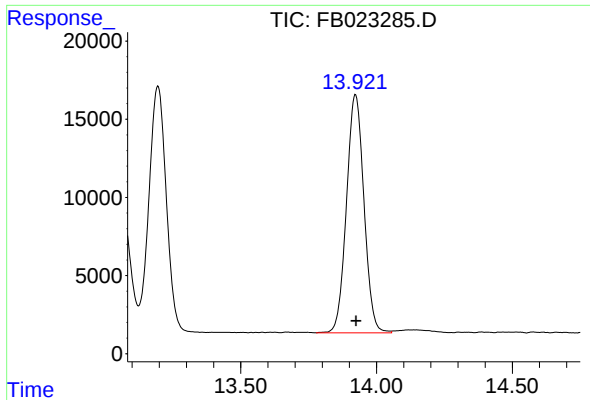

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: -0.002 min
Response: 681799
Conc: 20.24 ng/ml

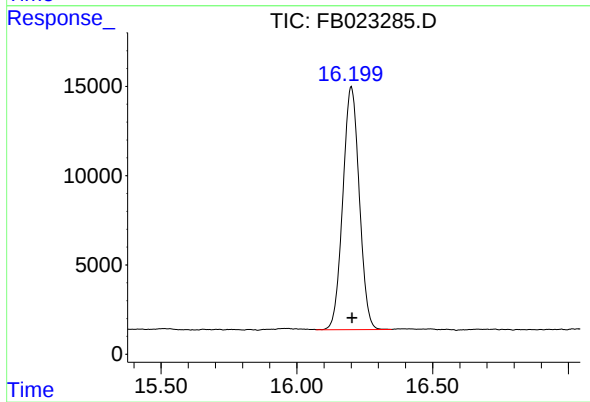

#10 1,2,4-Trimethylbenzene

R.T.: 16.201 min
Delta R.T.: -0.003 min
Response: 573022
Conc: 20.42 ng/ml