

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122019\
 Data File : FB023288.D
 Signal(s) : FID2B.CH
 Acq On : 20 Dec 2019 13:01
 Operator : DD/AJ
 Sample : K6117-08MS
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 20 20:25:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	428205	18.057 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.685	834348	26.958 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	874052	26.165 ng/ml
3) t n-Heptane	7.750	285034	8.641 ng/ml
4) t Benzene	7.885	353495	8.852 ng/ml
6) t Toluene	10.623	1037517	26.946 ng/ml
7) t Ethylbenzene	13.063	318440	8.773 ng/ml
8) t m-Xylene	13.196	603723	17.392 ng/ml
9) t O-Xylene	13.924	588682	17.477 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	489156	17.434 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122019\
Data File : FB023288.D
Signal(s) : FID2B.CH
Acq On : 20 Dec 2019 13:01
Operator : DD/AJ
Sample : K6117-08MS
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 20 20:25:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

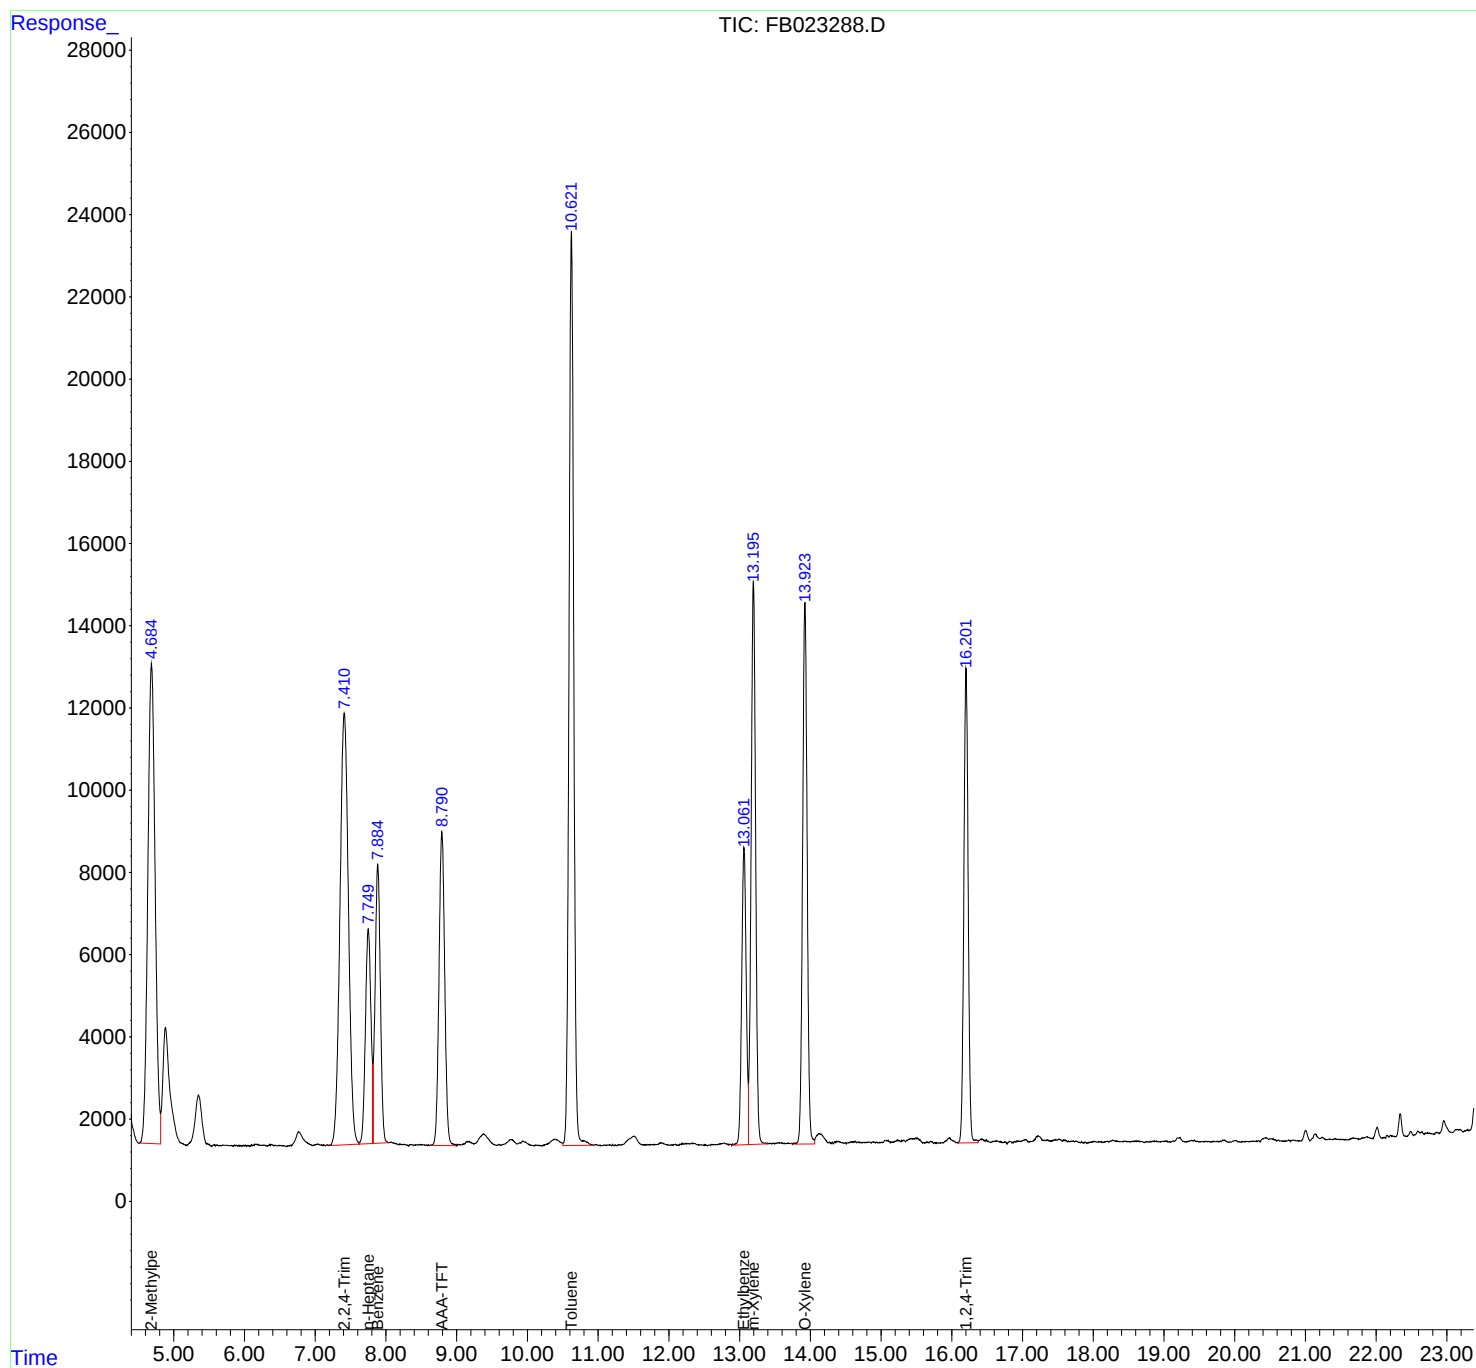

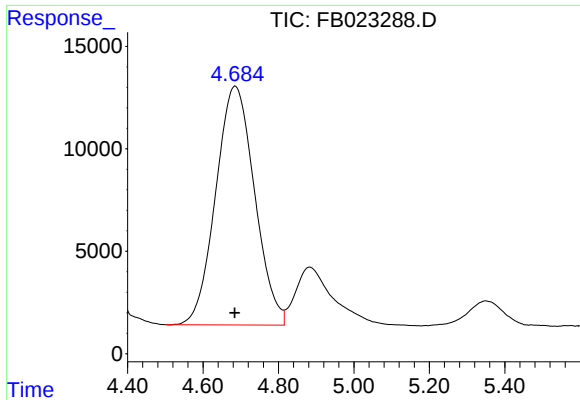


#1 2-Methylpentane

R.T.: 4.685 min
Delta R.T.: 0.001 min
Response: 834348
Conc: 26.96 ng/ml

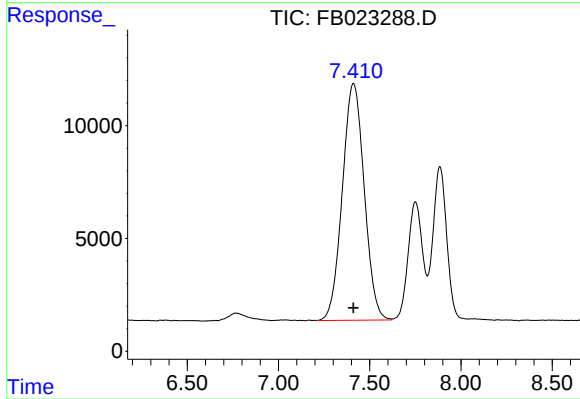


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: 0.000 min
Response: 874052
Conc: 26.16 ng/ml

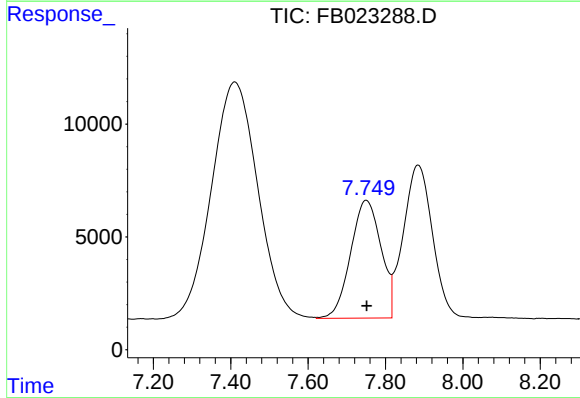


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.001 min
Response: 285034
Conc: 8.64 ng/ml

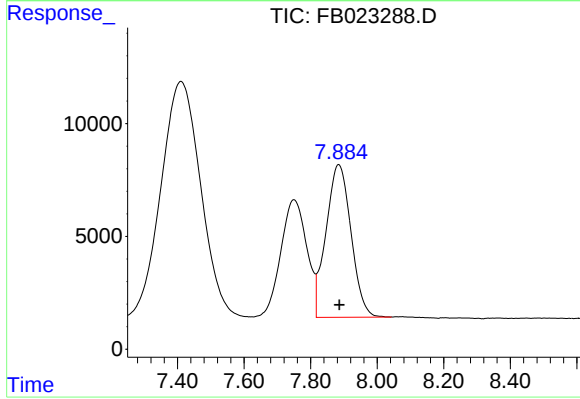


#4 Benzene

R.T.: 7.885 min
Delta R.T.: -0.002 min
Response: 353495
Conc: 8.85 ng/ml

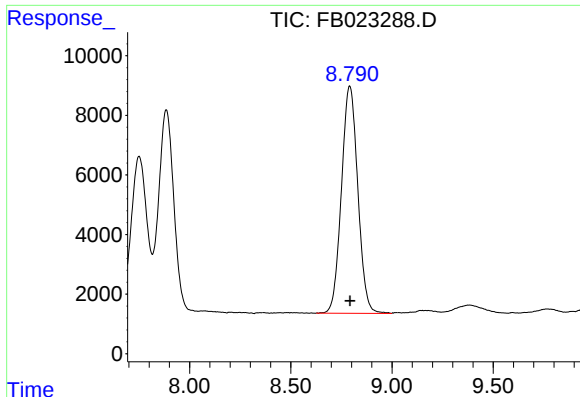


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: -0.002 min
Response: 428205
Conc: 18.06 ng/ml

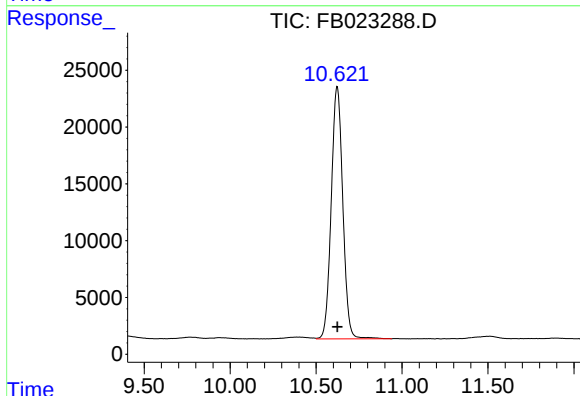


#6 Toluene

R.T.: 10.623 min
Delta R.T.: -0.001 min
Response: 1037517
Conc: 26.95 ng/ml

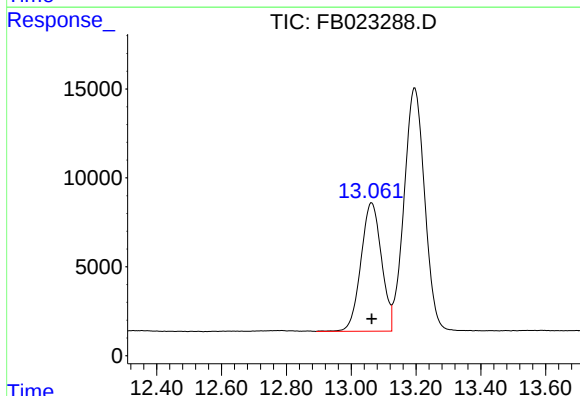


#7 Ethylbenzene

R.T.: 13.063 min
Delta R.T.: 0.000 min
Response: 318440
Conc: 8.77 ng/ml

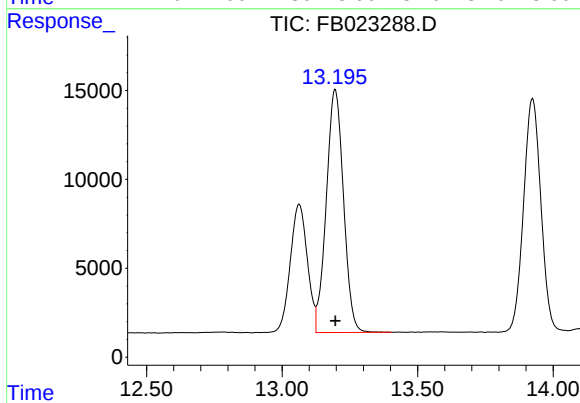

#8 m-Xylene

R.T.: 13.196 min
Delta R.T.: -0.001 min
Response: 603723
Conc: 17.39 ng/ml

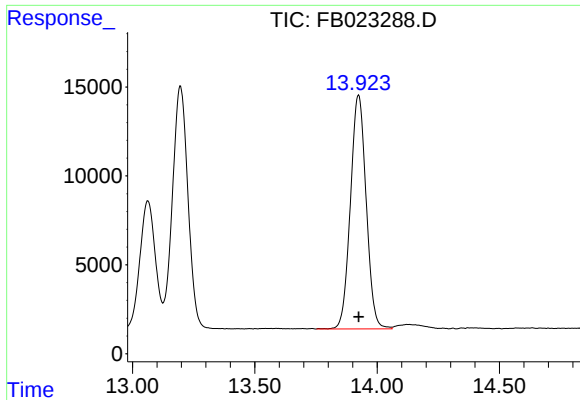


#9 O-Xylene

R.T.: 13.924 min

Delta R.T.: 0.000 min

Response: 588682

Conc: 17.48 ng/ml

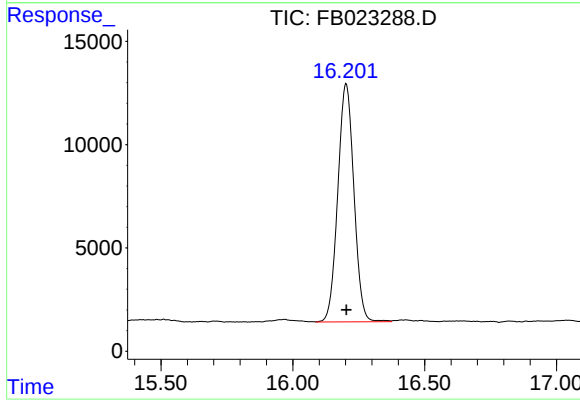

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min

Delta R.T.: 0.000 min

Response: 489156

Conc: 17.43 ng/ml