

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122019\
 Data File : FB023289.D
 Signal(s) : FID2B.CH
 Acq On : 20 Dec 2019 13:31
 Operator : DD/AJ
 Sample : K6117-08MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 20 20:26:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	436557	18.409 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	864609	27.936 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	933240	27.937 ng/ml
3) t n-Heptane	7.753	305654	9.266 ng/ml
4) t Benzene	7.887	364817	9.136 ng/ml
6) t Toluene	10.624	1066351	27.695 ng/ml
7) t Ethylbenzene	13.064	336584	9.273 ng/ml
8) t m-Xylene	13.198	636535	18.338 ng/ml
9) t O-Xylene	13.925	614370	18.240 ng/ml
10) t 1,2,4-Trimethylbenzene	16.203	520192	18.540 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122019\
Data File : FB023289.D
Signal(s) : FID2B.CH
Acq On : 20 Dec 2019 13:31
Operator : DD/AJ
Sample : K6117-08MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 20 20:26:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

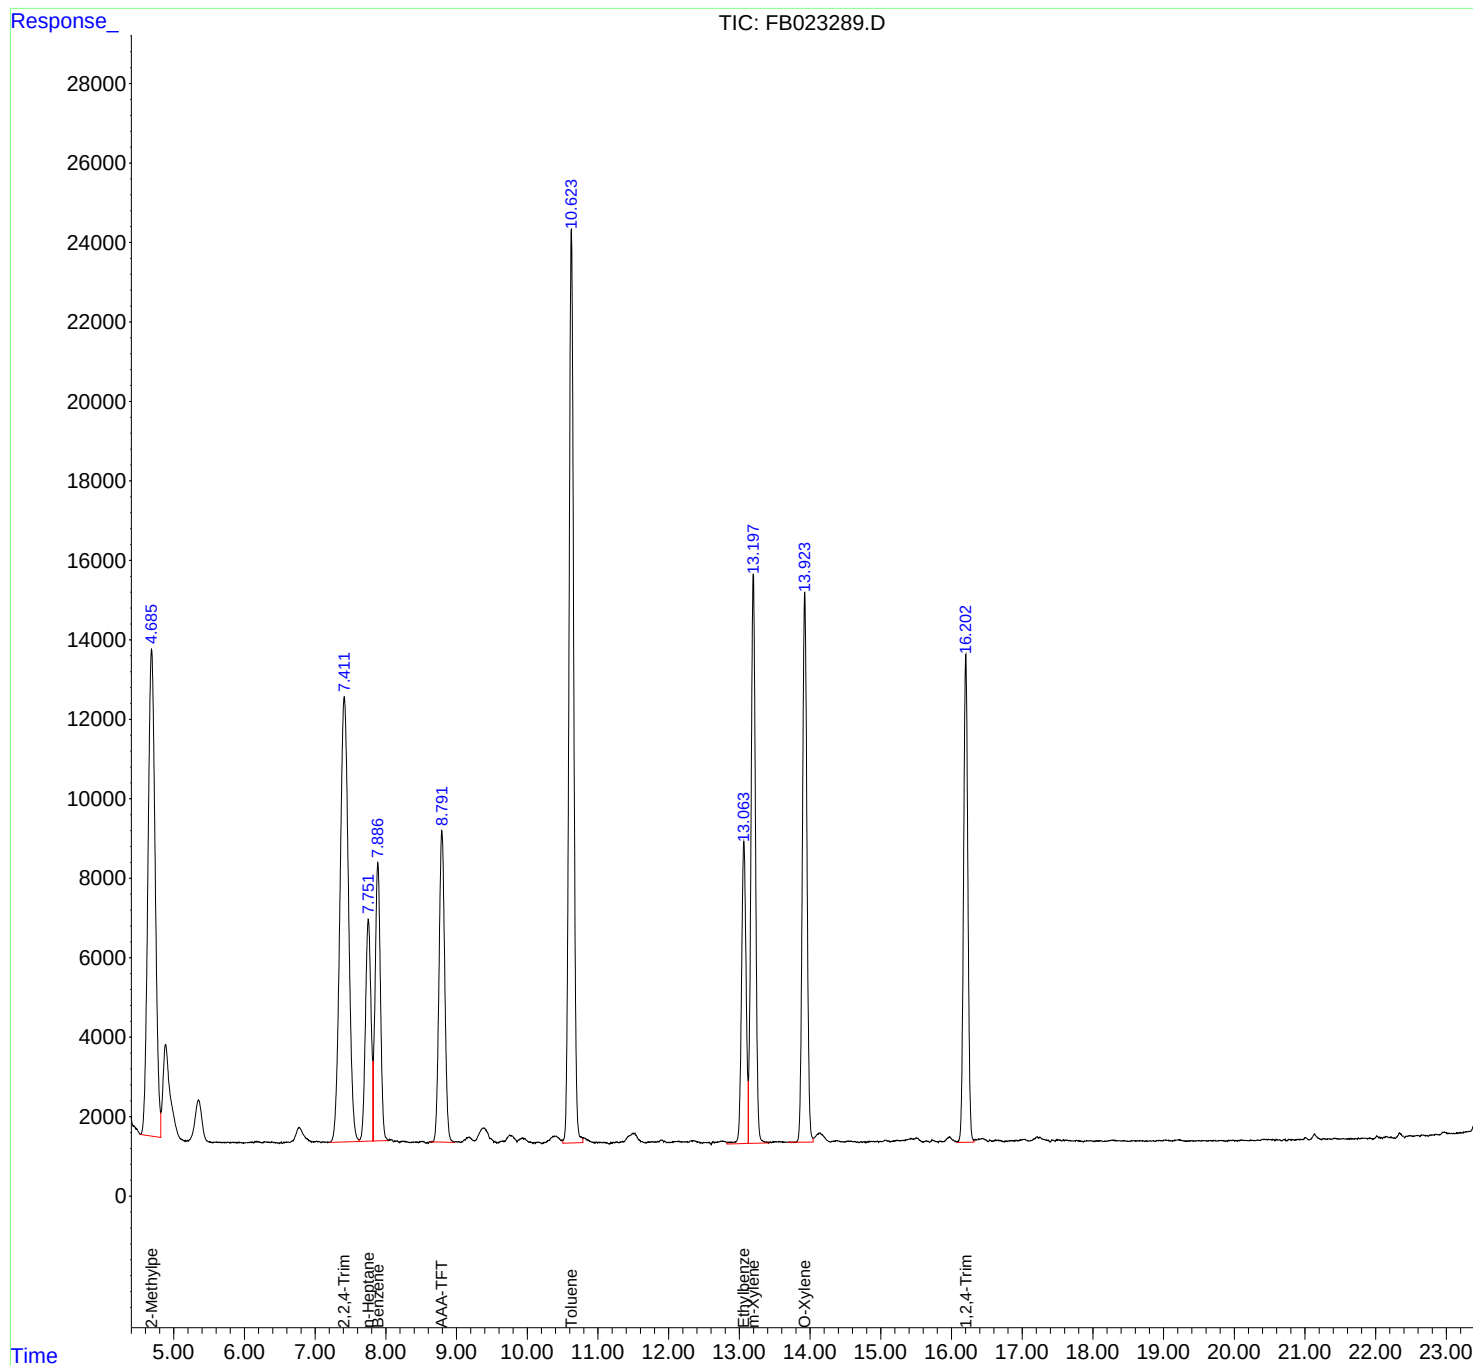

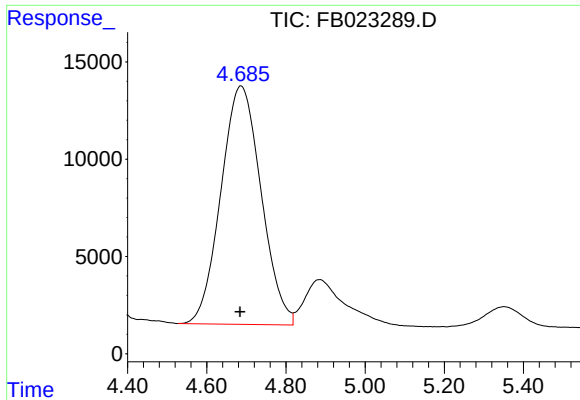


#1 2-Methylpentane

R.T.: 4.687 min
Delta R.T.: 0.003 min
Response: 864609
Conc: 27.94 ng/ml

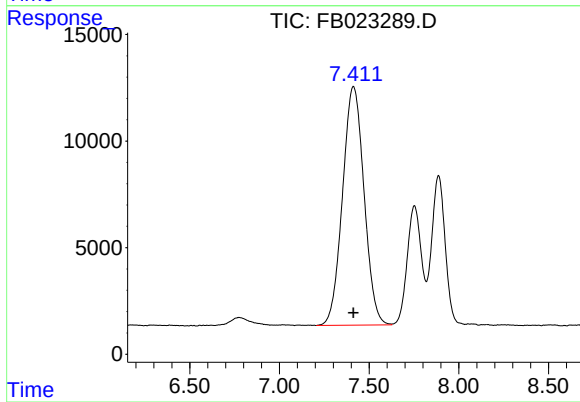


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: 0.001 min
Response: 933240
Conc: 27.94 ng/ml

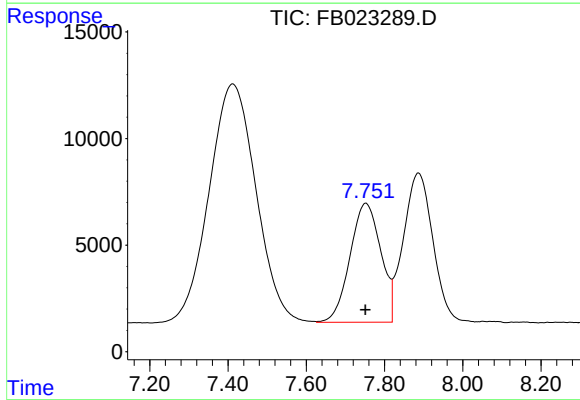


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.000 min
Response: 305654
Conc: 9.27 ng/ml

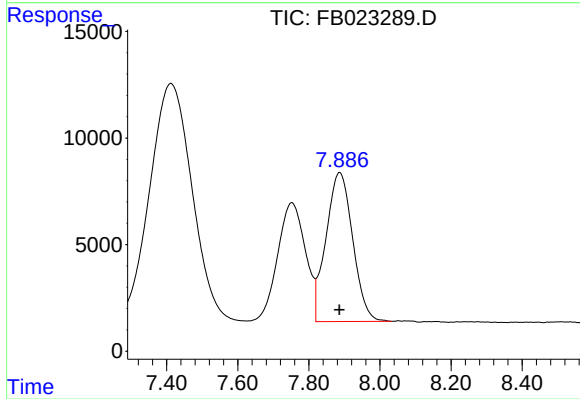


#4 Benzene

R.T.: 7.887 min
Delta R.T.: 0.000 min
Response: 364817
Conc: 9.14 ng/ml

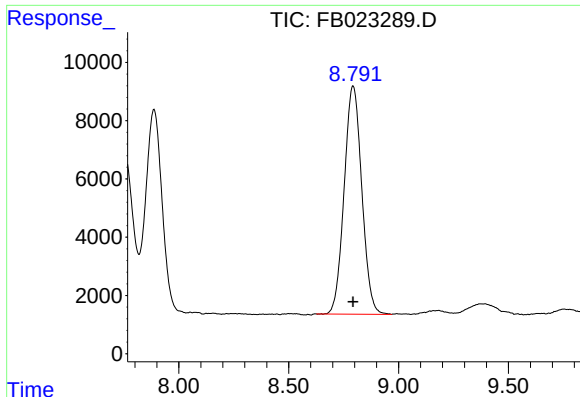


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: 0.000 min
Response: 436557
Conc: 18.41 ng/ml

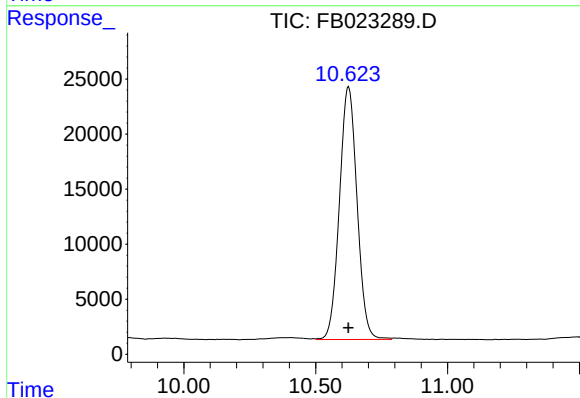


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.000 min
Response: 1066351
Conc: 27.69 ng/ml

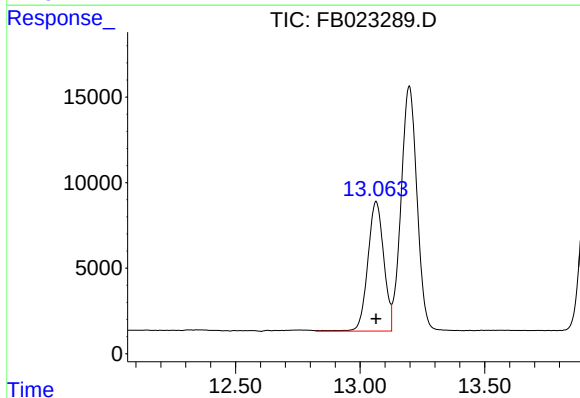


#7 Ethylbenzene

R.T.: 13.064 min
Delta R.T.: 0.000 min
Response: 336584
Conc: 9.27 ng/ml

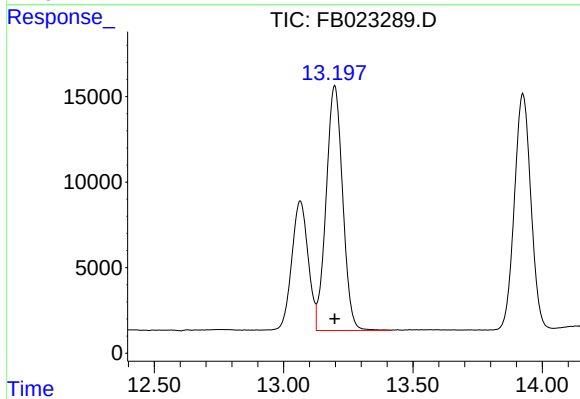


#8 m-Xylene

R.T.: 13.198 min
Delta R.T.: 0.000 min
Response: 636535
Conc: 18.34 ng/ml

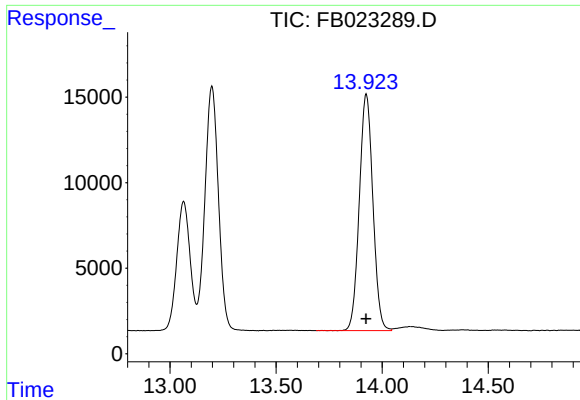

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: 0.000 min
Response: 614370
Conc: 18.24 ng/ml

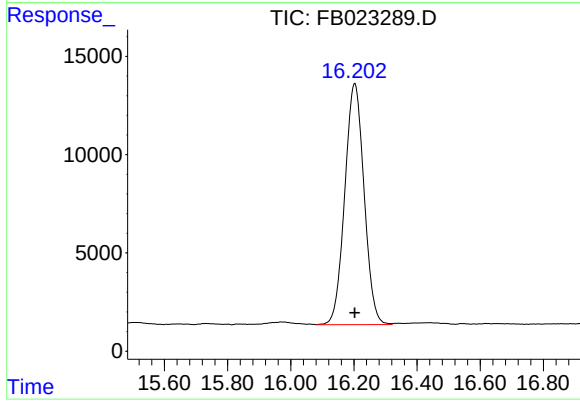

#10 1,2,4-Trimethylbenzene

R.T.: 16.203 min
Delta R.T.: 0.000 min
Response: 520192
Conc: 18.54 ng/ml