

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB122118\  
Data File : FB019180.D  
Signal(s) : FID2B.CH  
Acq On : 21 Dec 2018 18:03  
Operator : MJ/SJ  
Sample : J6511-02  
Misc : 4.61g/5.00ml DI WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Dec 22 01:42:54 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB120718.M  
Quant Title :  
QLast Update : Fri Dec 07 17:57:38 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| 5) s AAA-TFT                | 9.115  | 146902   | 16.807 ng/ml |
| Target Compounds            |        |          |              |
| 4) t Benzene                | 8.213  | 6953     | 0.386 ng/ml  |
| 6) t Toluene                | 10.965 | 15076    | 0.993 ng/ml  |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB122118\  
Data File : FB019180.D  
Signal(s) : FID2B.CH  
Acq On : 21 Dec 2018 18:03  
Operator : MJ/SJ  
Sample : J6511-02  
Misc : 4.61g/5.00ml DI WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Dec 22 01:42:54 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB120718.M  
Quant Title :  
QLast Update : Fri Dec 07 17:57:38 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

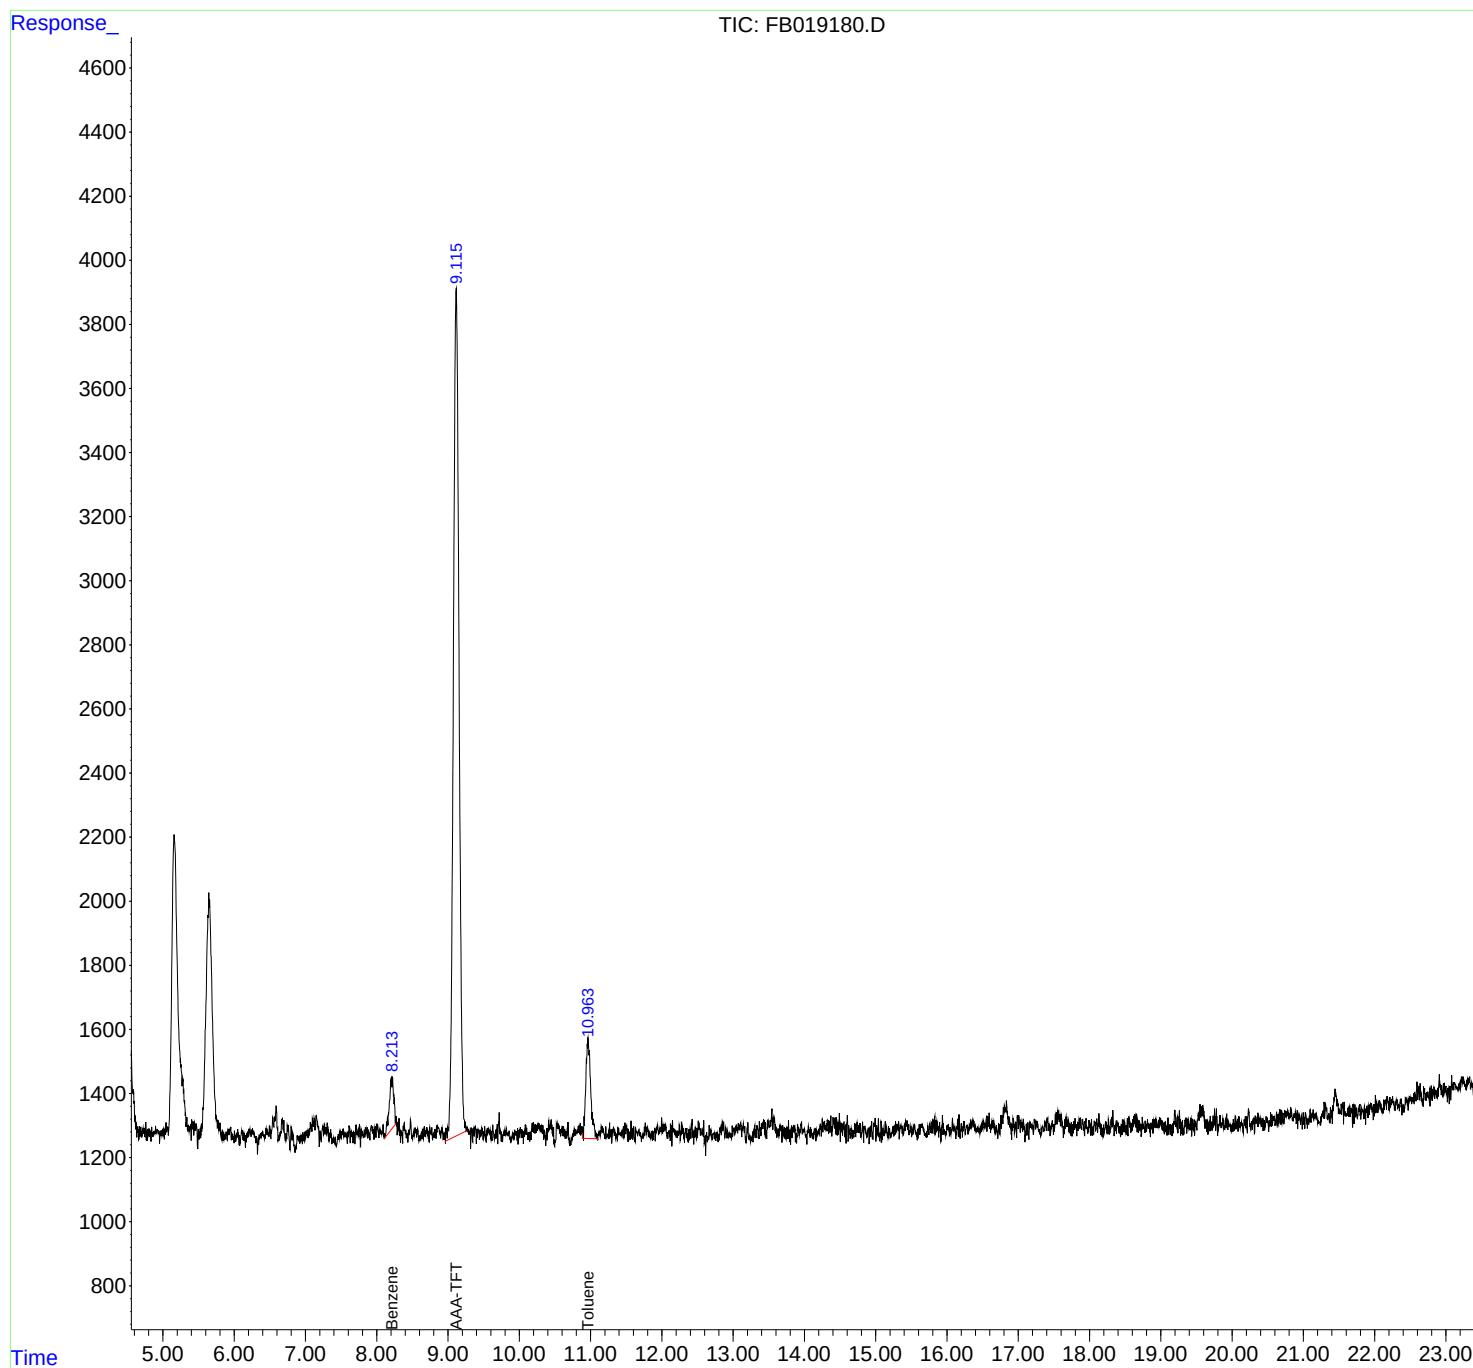


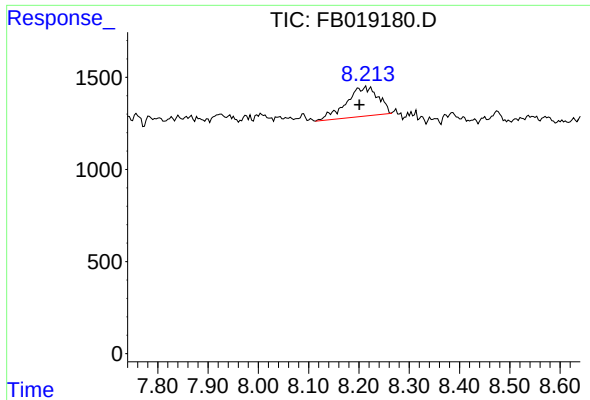

#4 Benzene


R.T.: 8.213 min  
Delta R.T.: 0.012 min  
Response: 6953  
Conc: 0.39 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

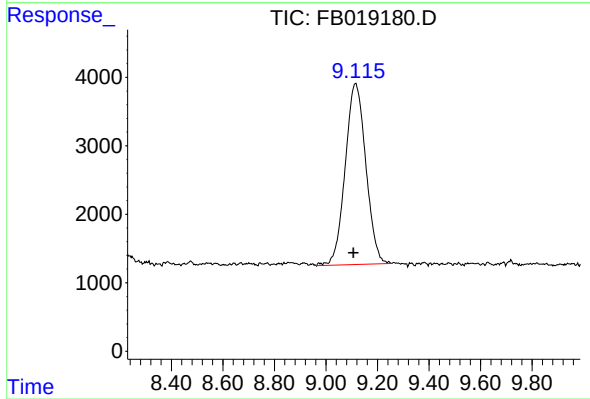

#5 AAA-TFT

R.T.: 9.115 min  
Delta R.T.: 0.009 min  
Response: 146902  
Conc: 16.81 ng/ml

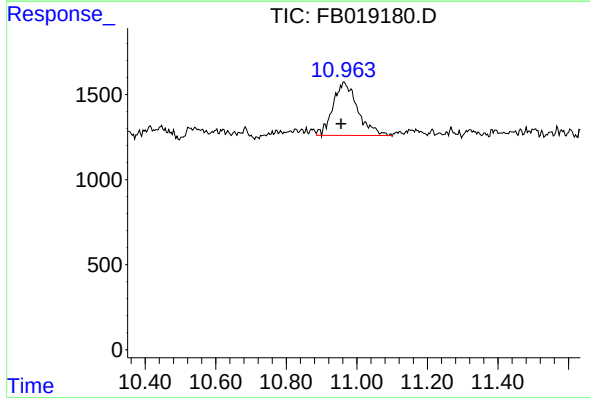

#6 Toluene

R.T.: 10.965 min  
Delta R.T.: 0.009 min  
Response: 15076  
Conc: 0.99 ng/ml