

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122321\
 Data File : FB026541.D
 Signal(s) : FID2B.CH
 Acq On : 23 Dec 2021 11:10
 Operator : AJ/MA
 Sample : BSF1223SS1
 Misc : 4.99G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1223SS1

Integration File: Calibration.e
 Quant Time: Dec 24 21:53:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
 Quant Title :
 QLast Update : Wed Dec 08 14:04:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	242700	21.602 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	492302	28.282 ng/ml
2) t 2,2,4-Trimethylpentane	7.430	570493	28.767 ng/ml
3) t n-Heptane	7.748	182434	9.530 ng/ml
4) t Benzene	7.885	214306	9.639 ng/ml
6) t Toluene	10.618	626580	29.364 ng/ml
7) t Ethylbenzene	13.055	196380	9.948 ng/ml
8) t m-Xylene	13.188	386998	19.629 ng/ml
9) t O-Xylene	13.915	375462	19.661 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	380725	19.598 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122321\
Data File : FB026541.D
Signal(s) : FID2B.CH
Acq On : 23 Dec 2021 11:10
Operator : AJ/MA
Sample : BSF1223SS1
Misc : 4.99G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1223SS1

Integration File: Calibration.e
Quant Time: Dec 24 21:53:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
Quant Title :
QLast Update : Wed Dec 08 14:04:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

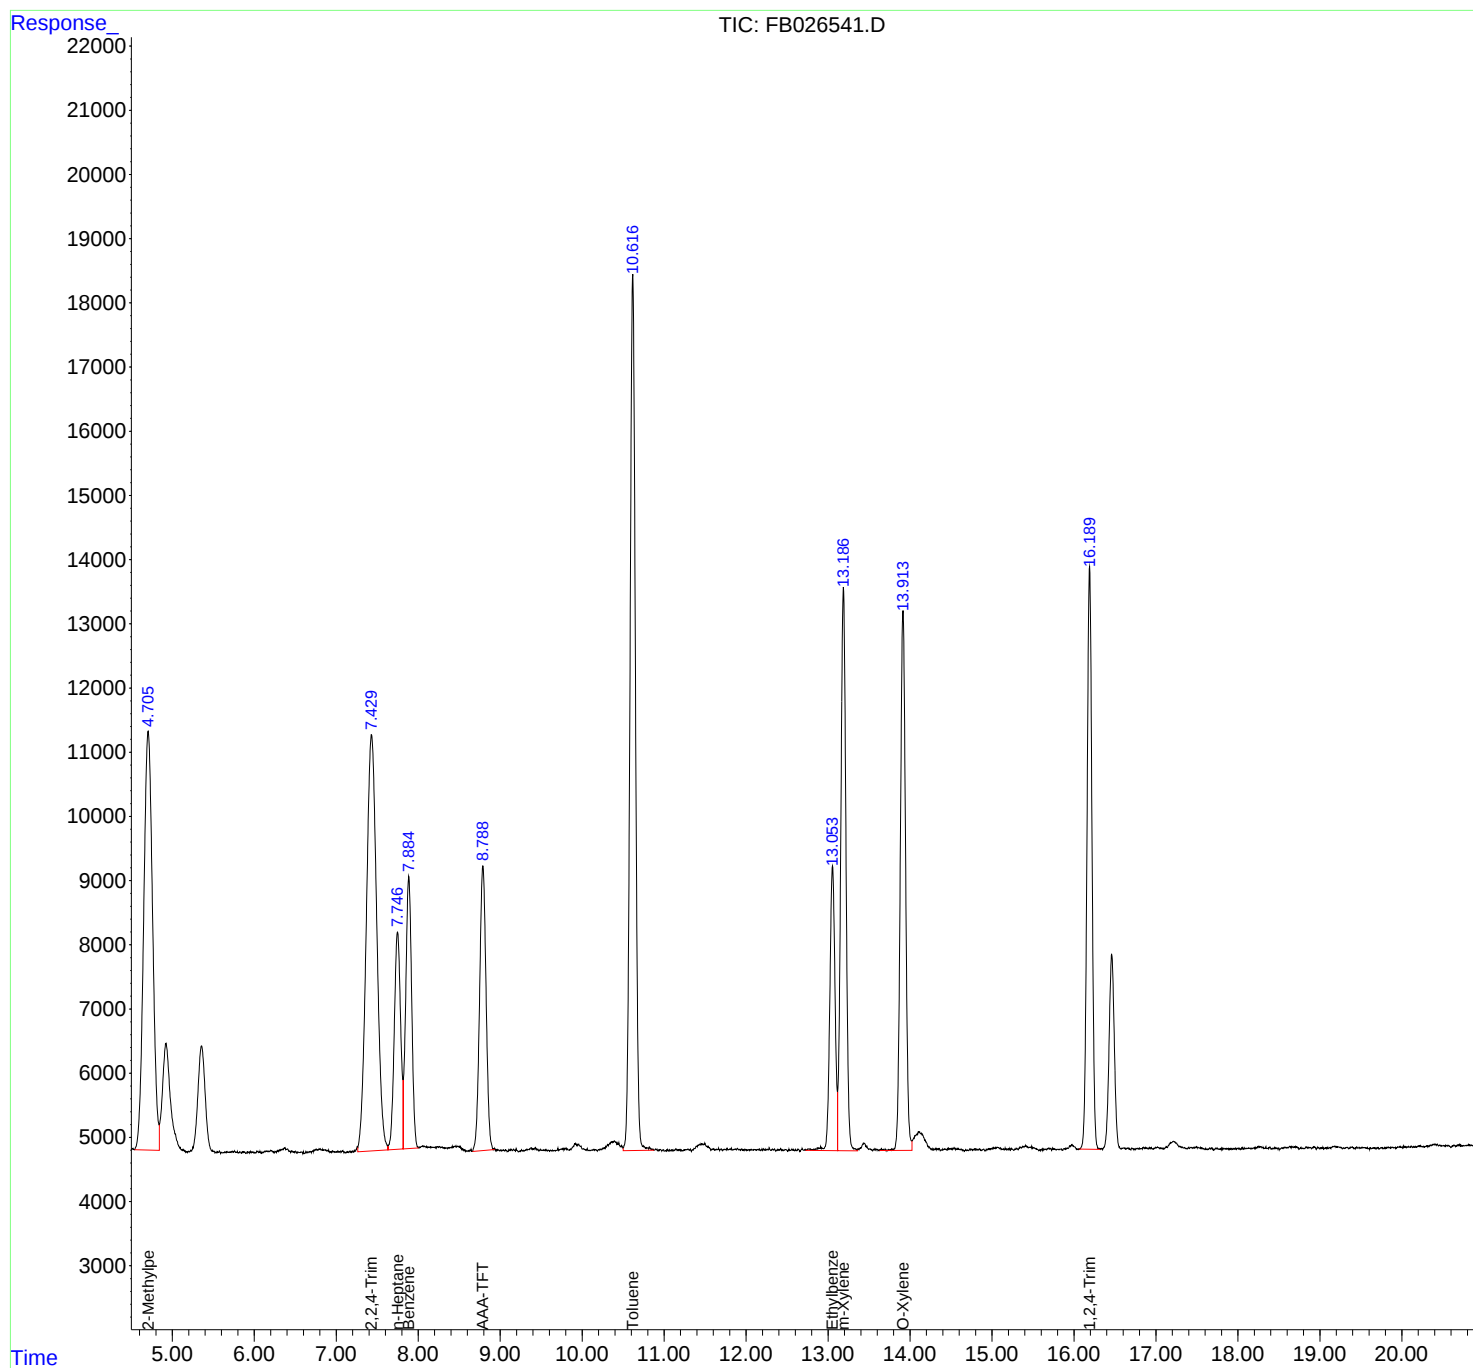


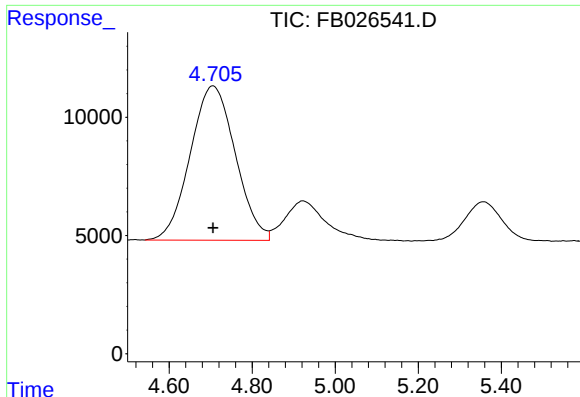

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 492302
Conc: 28.28 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1223SS1

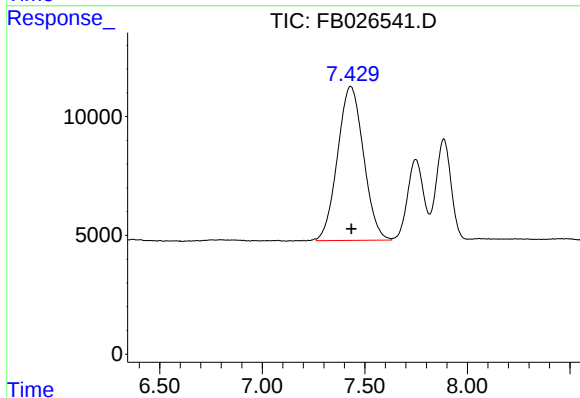


#2 2,2,4-Trimethylpentane

R.T.: 7.430 min
Delta R.T.: -0.005 min
Response: 570493
Conc: 28.77 ng/ml

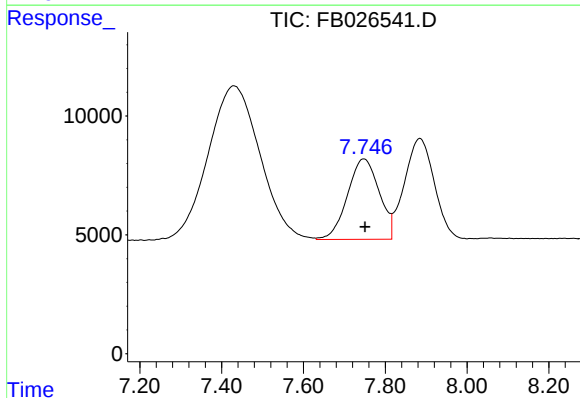


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.003 min
Response: 182434
Conc: 9.53 ng/ml

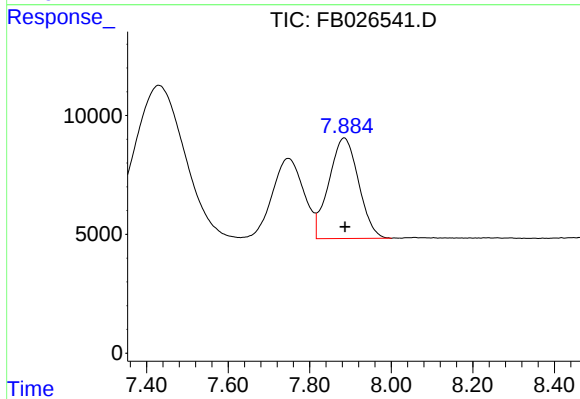

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.001 min
Response: 214306
Conc: 9.64 ng/ml

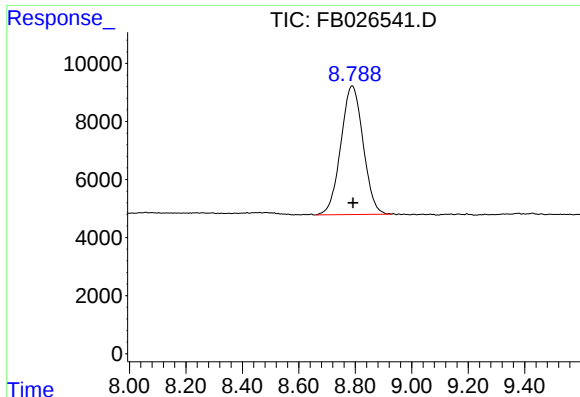

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.002 min
Response: 242700
Conc: 21.60 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1223SS1

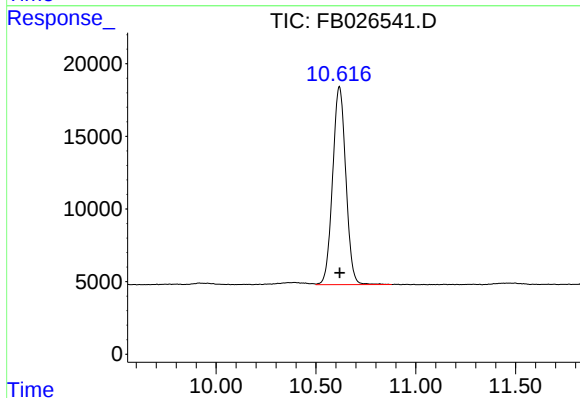


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.001 min
Response: 626580
Conc: 29.36 ng/ml

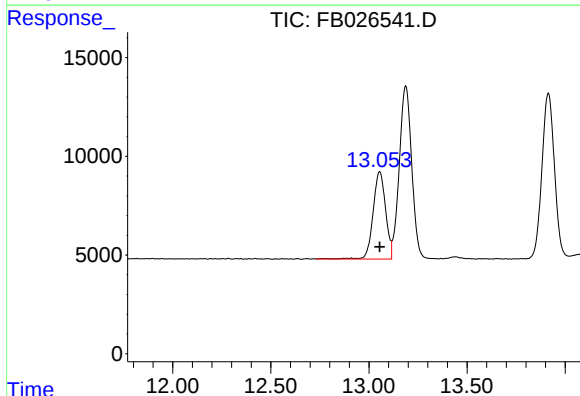


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: 0.000 min
Response: 196380
Conc: 9.95 ng/ml

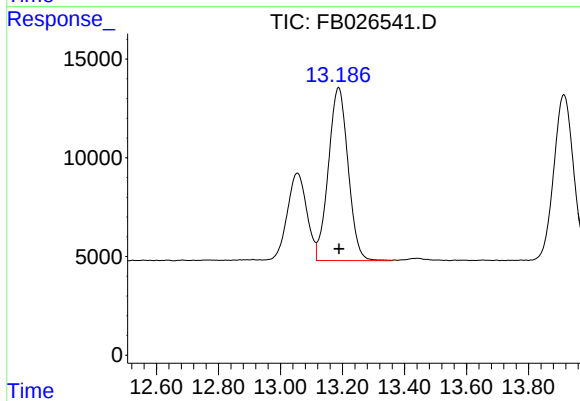

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.001 min
Response: 386998
Conc: 19.63 ng/ml

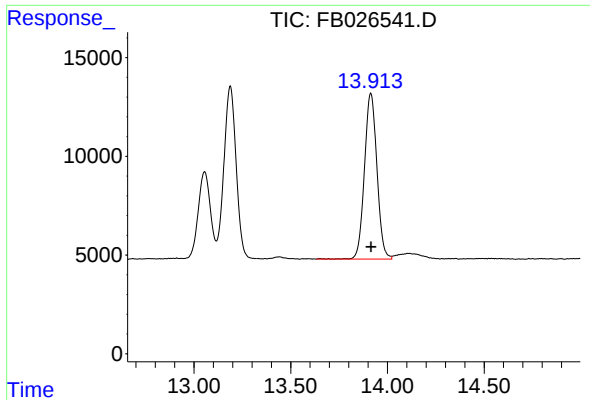

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.002 min
Response: 375462
Conc: 19.66 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1223SS1

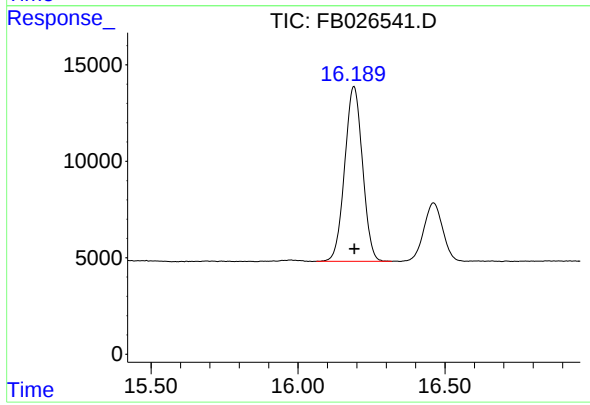

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.002 min
Response: 380725
Conc: 19.60 ng/ml