

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122324\
 Data File : FB031294.D
 Signal(s) : FID2B.CH
 Acq On : 23 Dec 2024 12:29
 Operator : YP/AJ
 Sample : BSF1223S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1223S1

Integration File: Calibration.e
 Quant Time: Dec 24 03:21:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121624.M
 Quant Title :
 QLast Update : Mon Dec 16 11:52:34 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.780	545535	20.678 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	917245	28.852 ng/ml
2) t 2,2,4-Trimethylpentane	7.409	1148076	29.761 ng/ml
3) t n-Heptane	7.743	317512	9.070 ng/ml
4) t Benzene	7.881	414717	9.411 ng/ml
6) t Toluene	10.608	1152475	27.647 ng/ml
7) t Ethylbenzene	13.043	342388	9.286 ng/ml
8) t m-Xylene	13.177	730203	18.316 ng/ml
9) t O-Xylene	13.905	678561	18.466 ng/ml
10) t 1,2,4-Trimethylbenzene	16.180	541958	18.165 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122324\
Data File : FB031294.D
Signal(s) : FID2B.CH
Acq On : 23 Dec 2024 12:29
Operator : YP/AJ
Sample : BSF1223S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1223S1

Integration File: Calibration.e
Quant Time: Dec 24 03:21:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121624.M
Quant Title :
QLast Update : Mon Dec 16 11:52:34 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

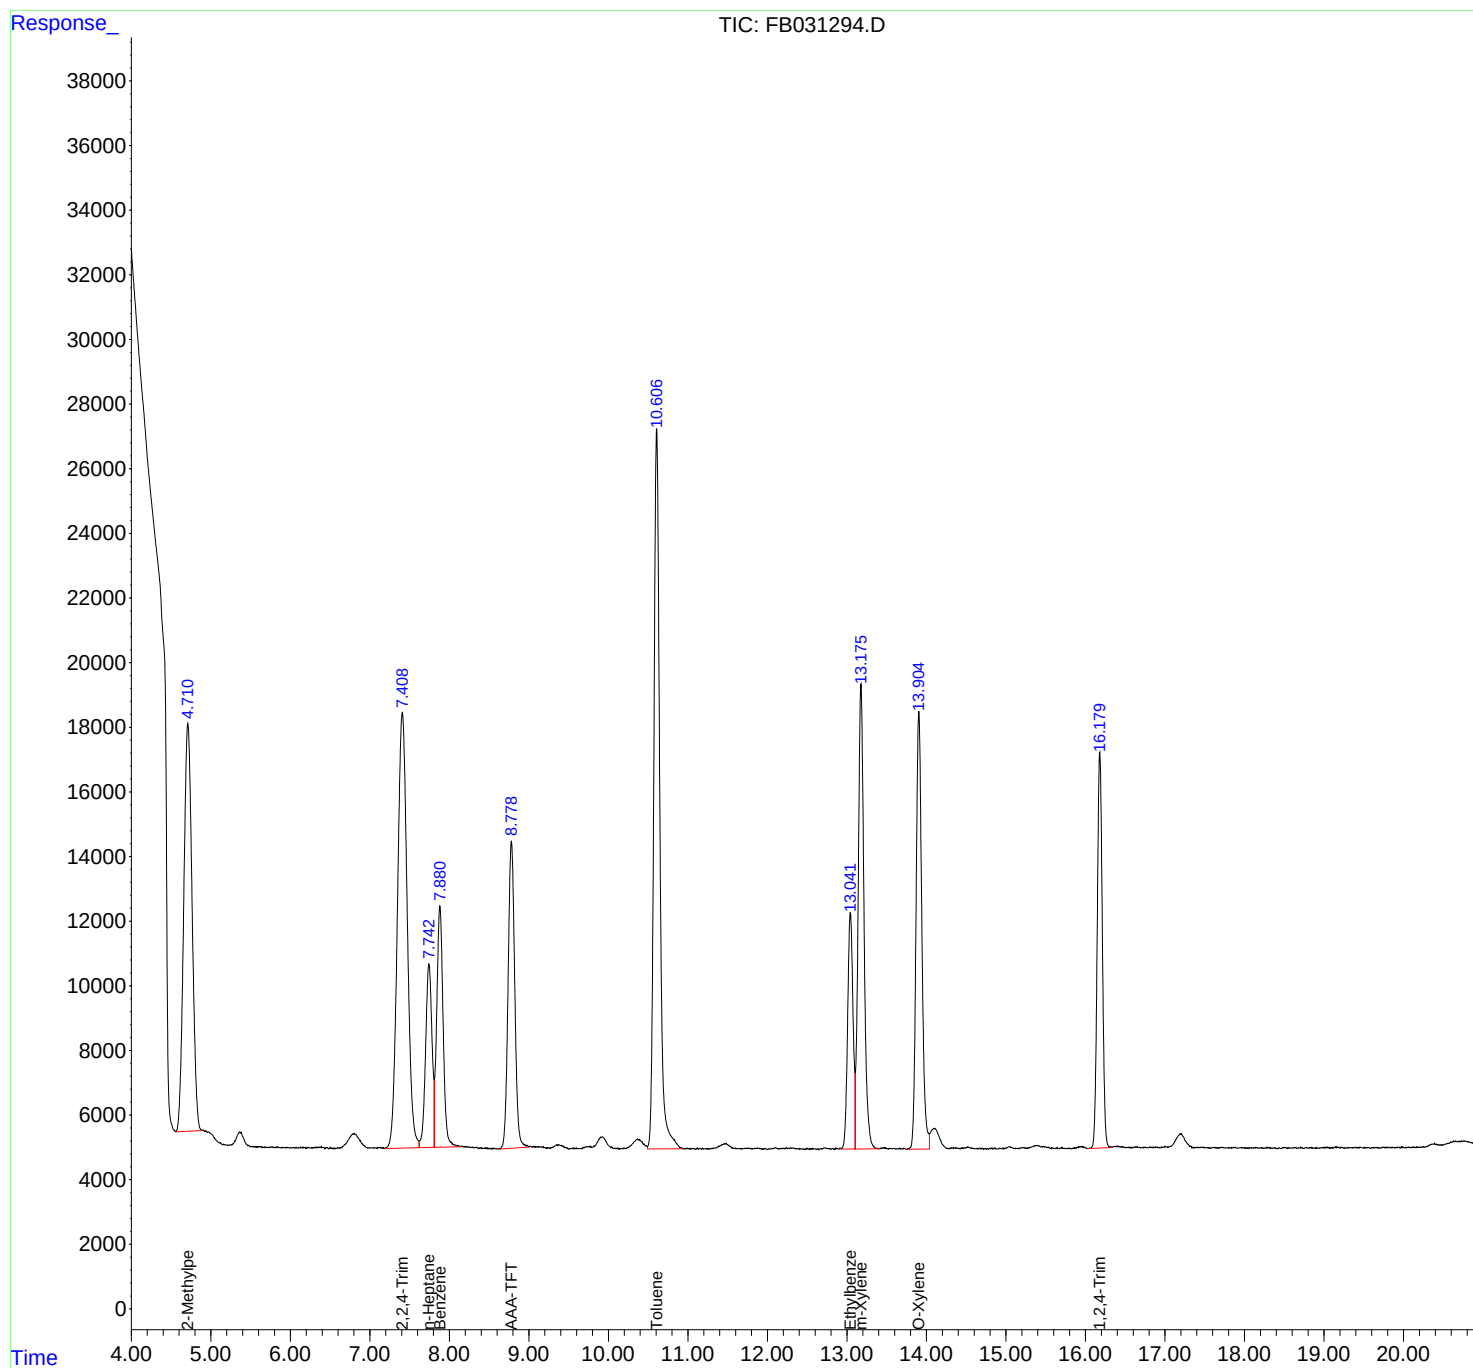


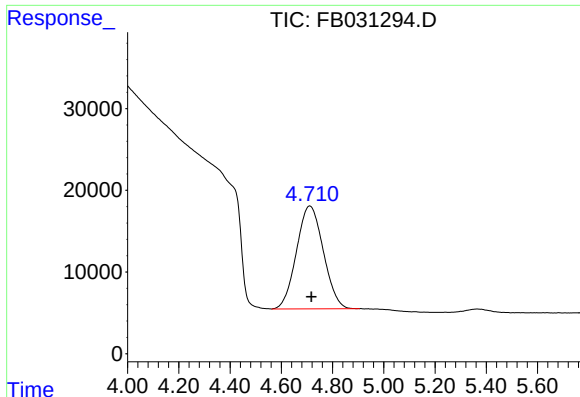

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: -0.005 min
Response: 917245
Conc: 28.85 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1223S1

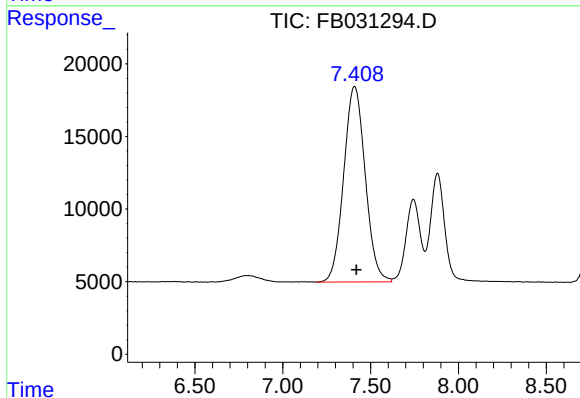


#2 2,2,4-Trimethylpentane

R.T.: 7.409 min
Delta R.T.: -0.010 min
Response: 1148076
Conc: 29.76 ng/ml

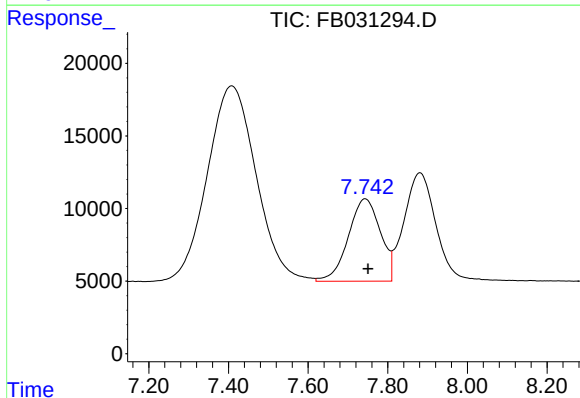


#3 n-Heptane

R.T.: 7.743 min
Delta R.T.: -0.007 min
Response: 317512
Conc: 9.07 ng/ml

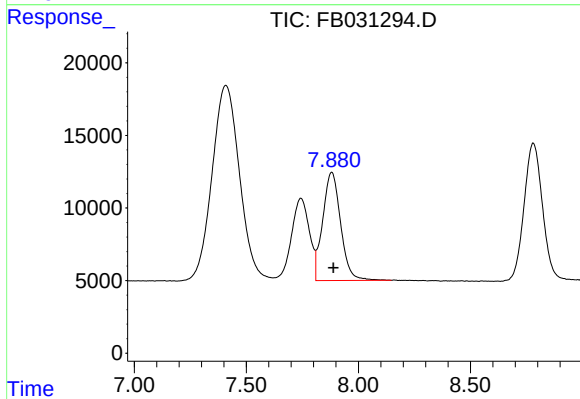

#4 Benzene


R.T.: 7.881 min
Delta R.T.: -0.007 min
Response: 414717
Conc: 9.41 ng/ml

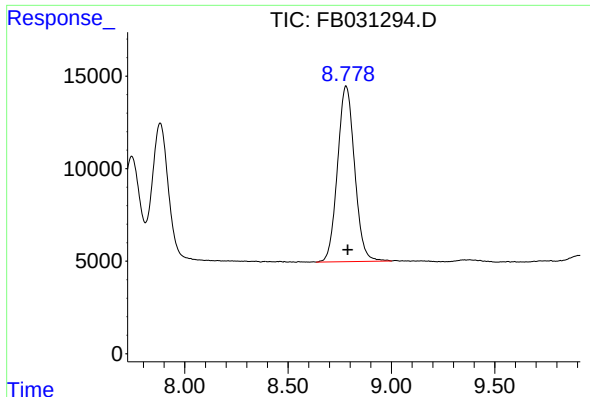

#5 AAA-TFT


R.T.: 8.780 min
Delta R.T.: -0.008 min
Response: 545535
Conc: 20.68 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1223S1

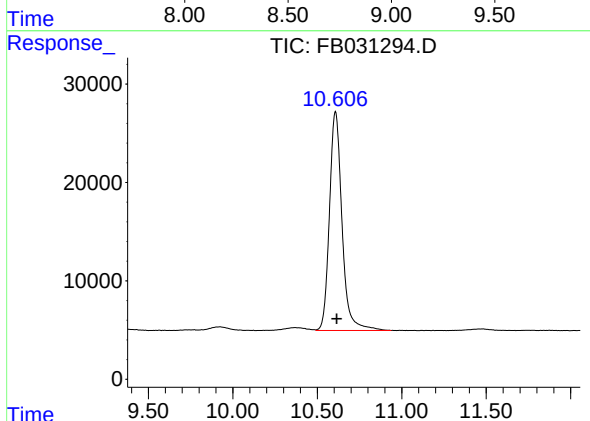


#6 Toluene

R.T.: 10.608 min
Delta R.T.: -0.008 min
Response: 1152475
Conc: 27.65 ng/ml

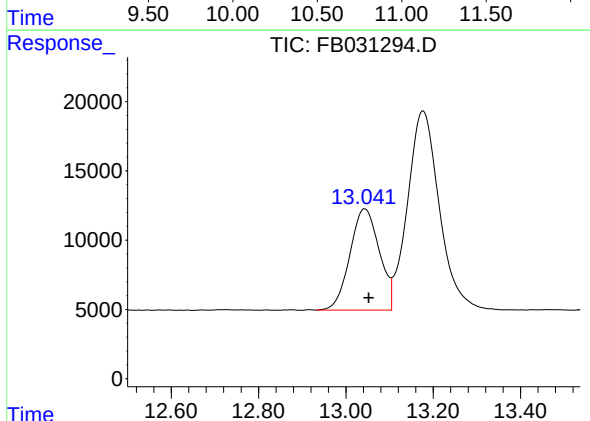


#7 Ethylbenzene

R.T.: 13.043 min
Delta R.T.: -0.009 min
Response: 342388
Conc: 9.29 ng/ml

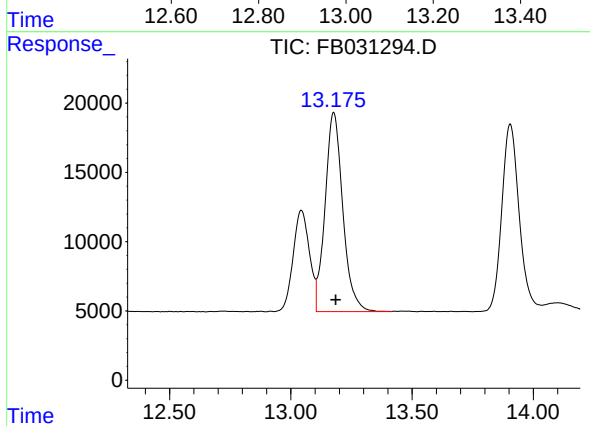

#8 m-Xylene


R.T.: 13.177 min
Delta R.T.: -0.009 min
Response: 730203
Conc: 18.32 ng/ml

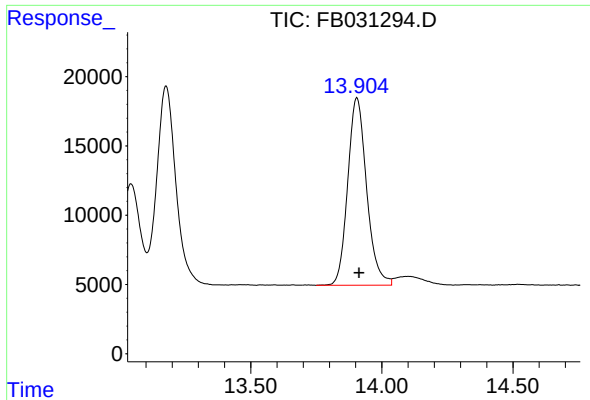

#9 O-Xylene

R.T.: 13.905 min
Delta R.T.: -0.008 min
Response: 678561
Conc: 18.47 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1223S1

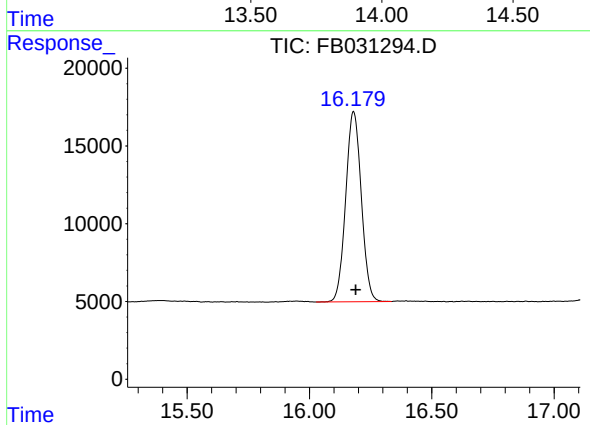

#10 1,2,4-Trimethylbenzene

R.T.: 16.180 min
Delta R.T.: -0.009 min
Response: 541958
Conc: 18.17 ng/ml