

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122324\
Data File : FB031296.D
Signal(s) : FID2B.CH
Acq On : 23 Dec 2024 13:45
Operator : YP/AJ
Sample : P5318-01
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
AU-06-122024

Integration File: Calibration.e
Quant Time: Dec 24 03:22:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121624.M
Quant Title :
QLast Update : Mon Dec 16 11:52:34 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122324\
Data File : FB031296.D
Signal(s) : FID2B.CH
Acq On : 23 Dec 2024 13:45
Operator : YP/AJ
Sample : P5318-01
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
AU-06-122024

Integration File: Calibration.e
Quant Time: Dec 24 03:22:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121624.M
Quant Title :
QLast Update : Mon Dec 16 11:52:34 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

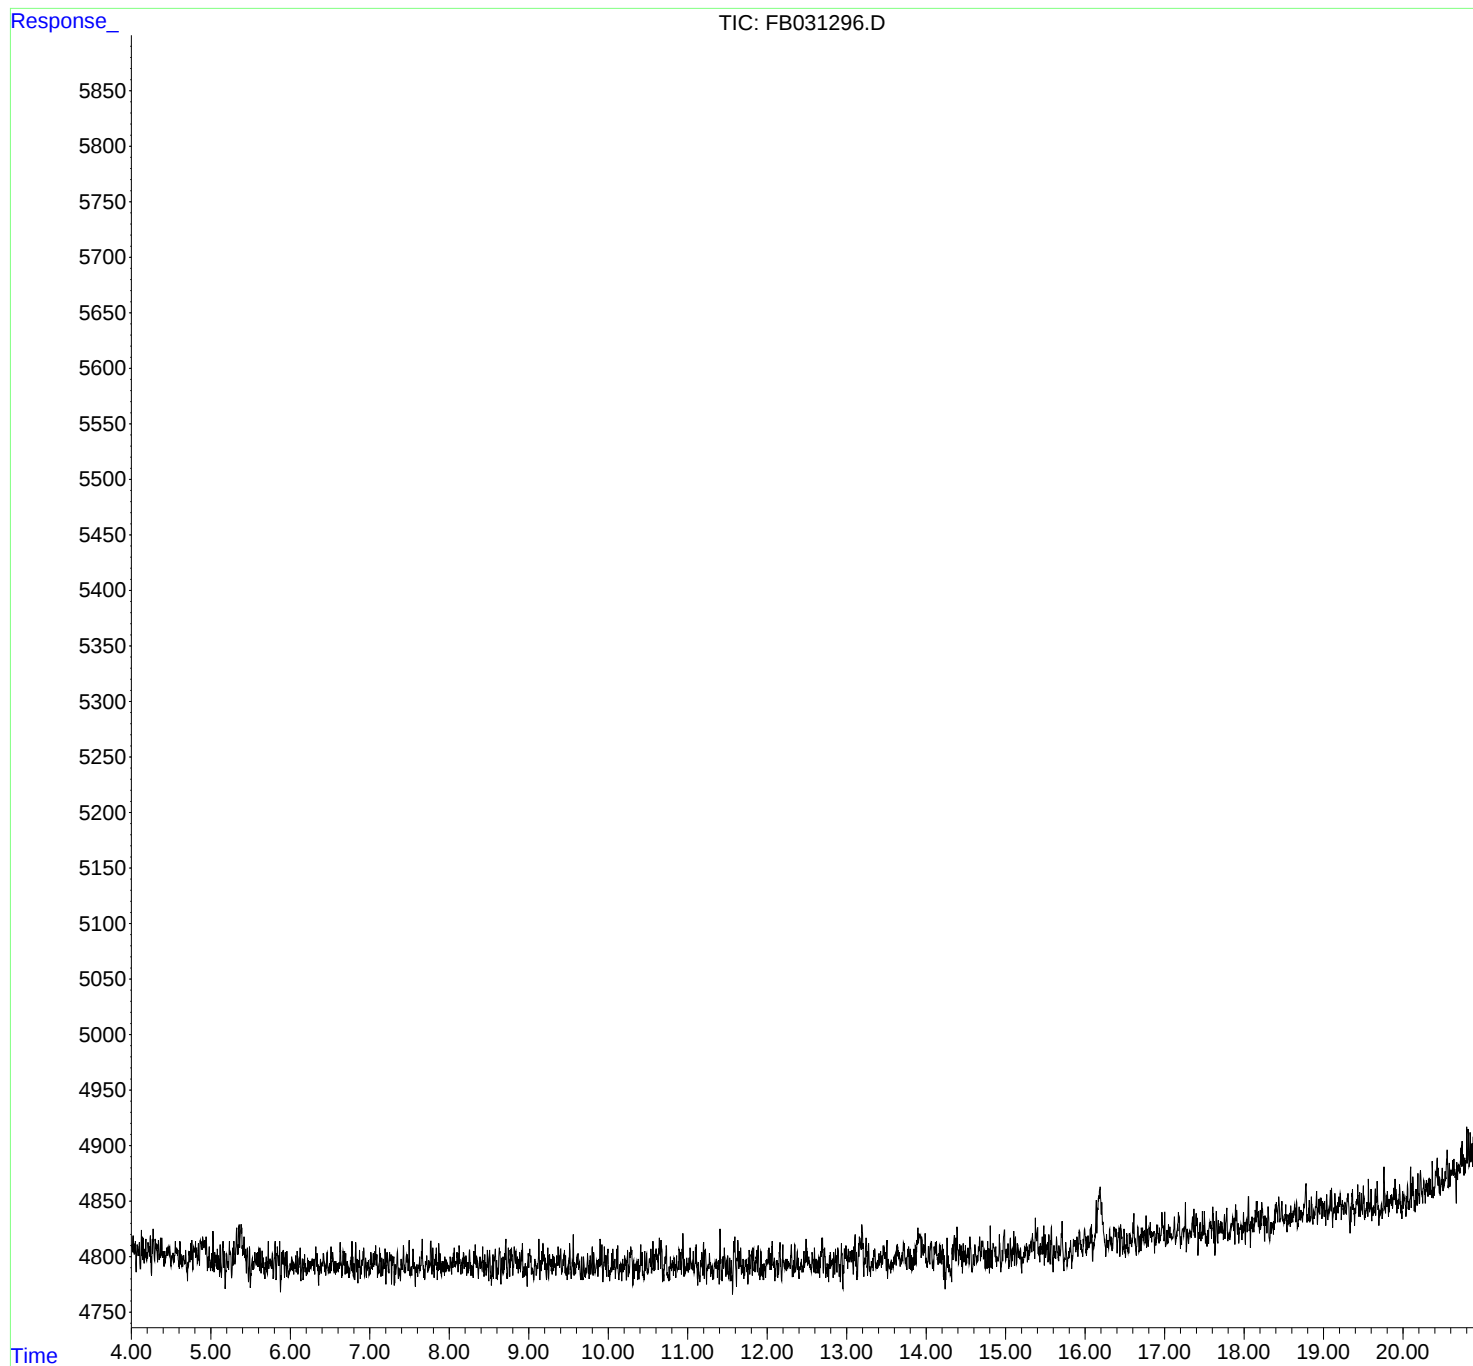

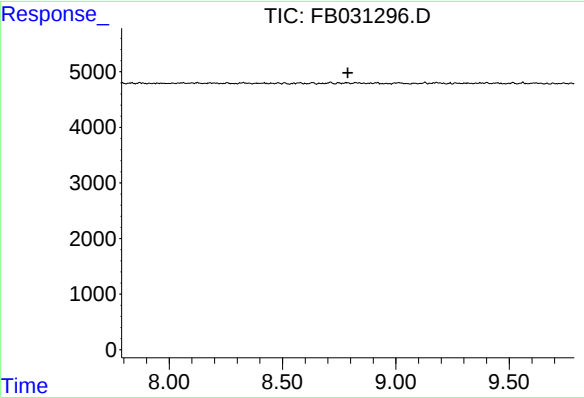

#5 AAA-TFT

R.T.: 0.000 min

Exp R.T. : 8.789 min

Response: 0

Conc: N.D.

Instrument :
FID_B
ClientSampleId :
AU-06-122024