

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122324\
 Data File : FB031298.D
 Signal(s) : FID2B.CH
 Acq On : 23 Dec 2024 14:37
 Operator : YP/AJ
 Sample : BSF1223S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1223S2

Integration File: Calibration.e
 Quant Time: Dec 24 03:22:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121624.M
 Quant Title :
 QLast Update : Mon Dec 16 11:52:34 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.783	537183	20.361 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	958632	30.153 ng/ml
2) t 2,2,4-Trimethylpentane	7.410	1197161	31.034 ng/ml
3) t n-Heptane	7.745	343145	9.802 ng/ml
4) t Benzene	7.882	448168	10.170 ng/ml
6) t Toluene	10.610	1242229	29.800 ng/ml
7) t Ethylbenzene	13.047	365379	9.909 ng/ml
8) t m-Xylene	13.180	775415	19.450 ng/ml
9) t O-Xylene	13.908	725497	19.743 ng/ml
10) t 1,2,4-Trimethylbenzene	16.184	582935	19.539 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122324\
Data File : FB031298.D
Signal(s) : FID2B.CH
Acq On : 23 Dec 2024 14:37
Operator : YP/AJ
Sample : BSF1223S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1223S2

Integration File: Calibration.e
Quant Time: Dec 24 03:22:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121624.M
Quant Title :
QLast Update : Mon Dec 16 11:52:34 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

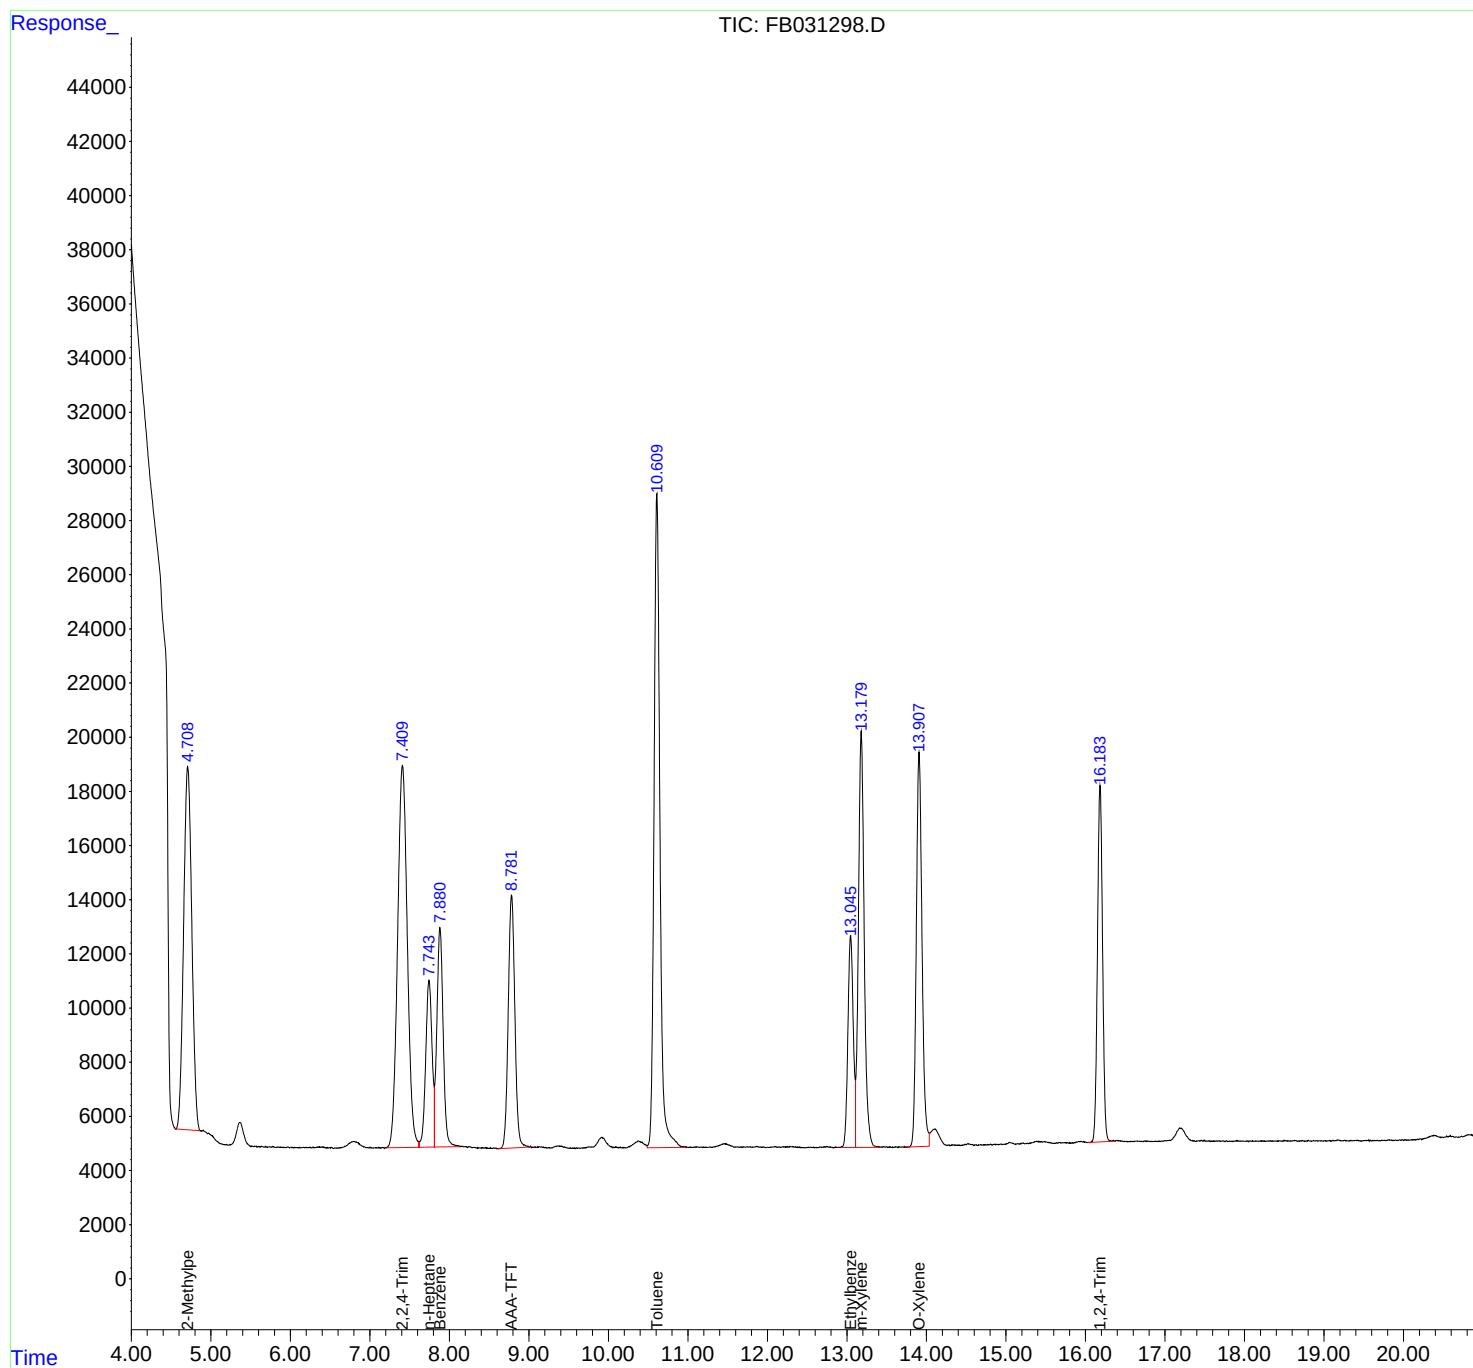


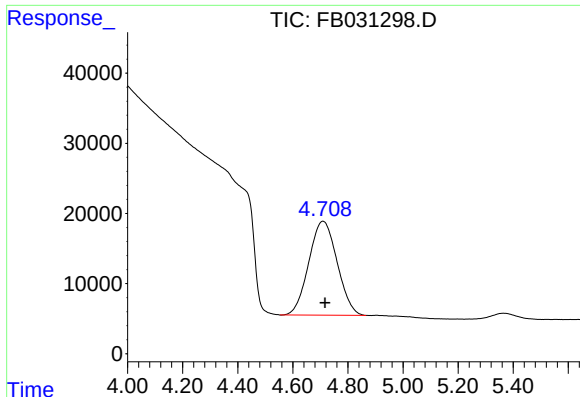

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: -0.008 min
Response: 958632
Conc: 30.15 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1223S2

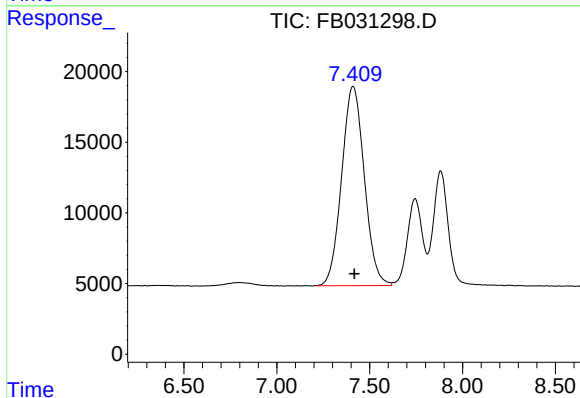


#2 2,2,4-Trimethylpentane

R.T.: 7.410 min
Delta R.T.: -0.008 min
Response: 1197161
Conc: 31.03 ng/ml

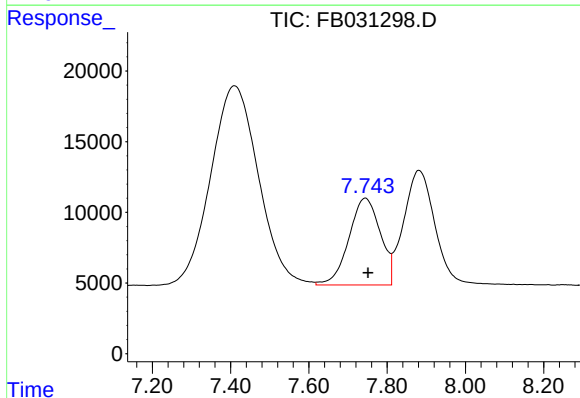


#3 n-Heptane

R.T.: 7.745 min
Delta R.T.: -0.006 min
Response: 343145
Conc: 9.80 ng/ml

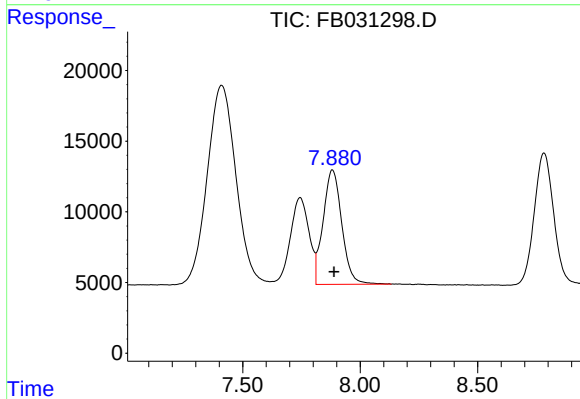

#4 Benzene


R.T.: 7.882 min
Delta R.T.: -0.007 min
Response: 448168
Conc: 10.17 ng/ml

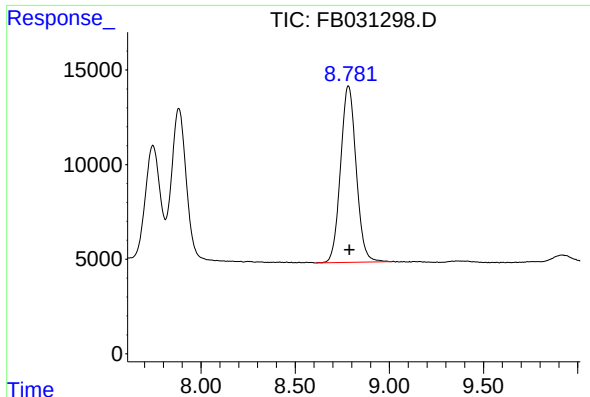

#5 AAA-TFT


R.T.: 8.783 min
Delta R.T.: -0.006 min
Response: 537183
Conc: 20.36 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1223S2

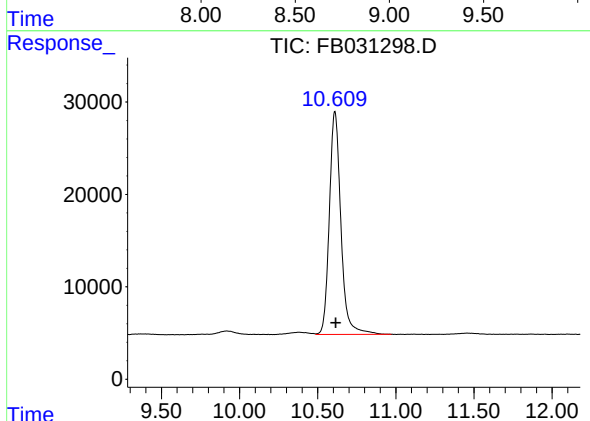


#6 Toluene

R.T.: 10.610 min
Delta R.T.: -0.006 min
Response: 1242229
Conc: 29.80 ng/ml

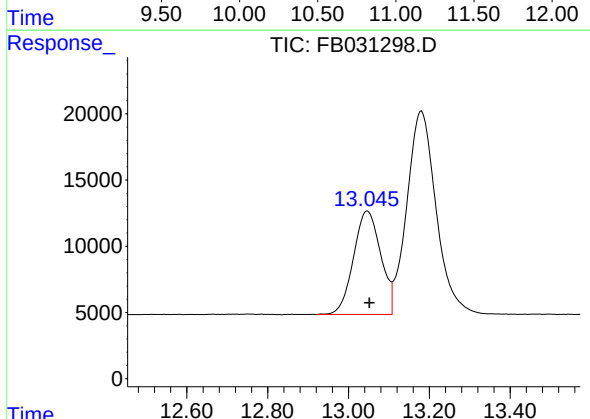


#7 Ethylbenzene

R.T.: 13.047 min
Delta R.T.: -0.006 min
Response: 365379
Conc: 9.91 ng/ml

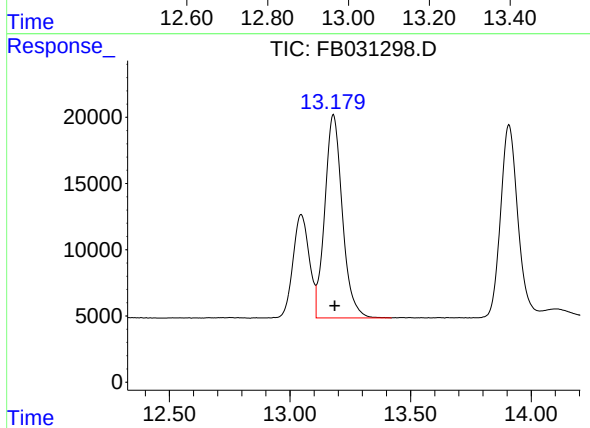

#8 m-Xylene


R.T.: 13.180 min
Delta R.T.: -0.005 min
Response: 775415
Conc: 19.45 ng/ml

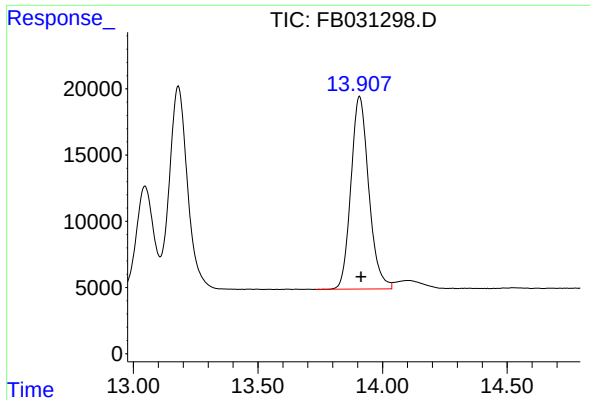

#9 O-Xylene

R.T.: 13.908 min
Delta R.T.: -0.006 min
Response: 725497
Conc: 19.74 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1223S2

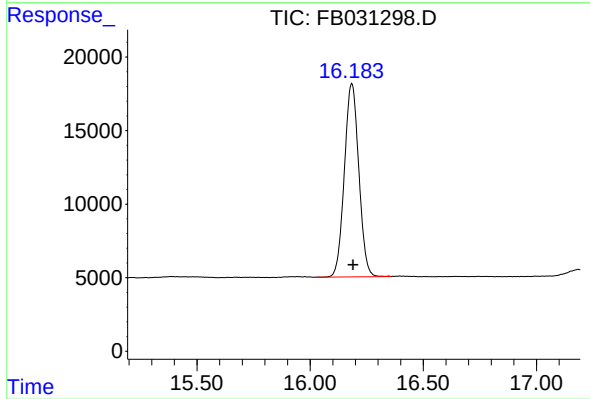

#10 1,2,4-Trimethylbenzene

R.T.: 16.184 min
Delta R.T.: -0.005 min
Response: 582935
Conc: 19.54 ng/ml