

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122419\
 Data File : FB023294.D
 Signal(s) : FID2B.CH
 Acq On : 24 Dec 2019 10:50
 Operator : DD/AJ
 Sample : BSF1224S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 25 00:17:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	464095	19.571 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	967948	31.275 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	1056319	31.621 ng/ml
3) t n-Heptane	7.753	349630	10.599 ng/ml
4) t Benzene	7.887	414154	10.371 ng/ml
6) t Toluene	10.626	1188986	30.880 ng/ml
7) t Ethylbenzene	13.066	378697	10.434 ng/ml
8) t m-Xylene	13.199	714286	20.577 ng/ml
9) t O-Xylene	13.927	683772	20.300 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	581631	20.730 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122419\
Data File : FB023294.D
Signal(s) : FID2B.CH
Acq On : 24 Dec 2019 10:50
Operator : DD/AJ
Sample : BSF1224S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 25 00:17:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

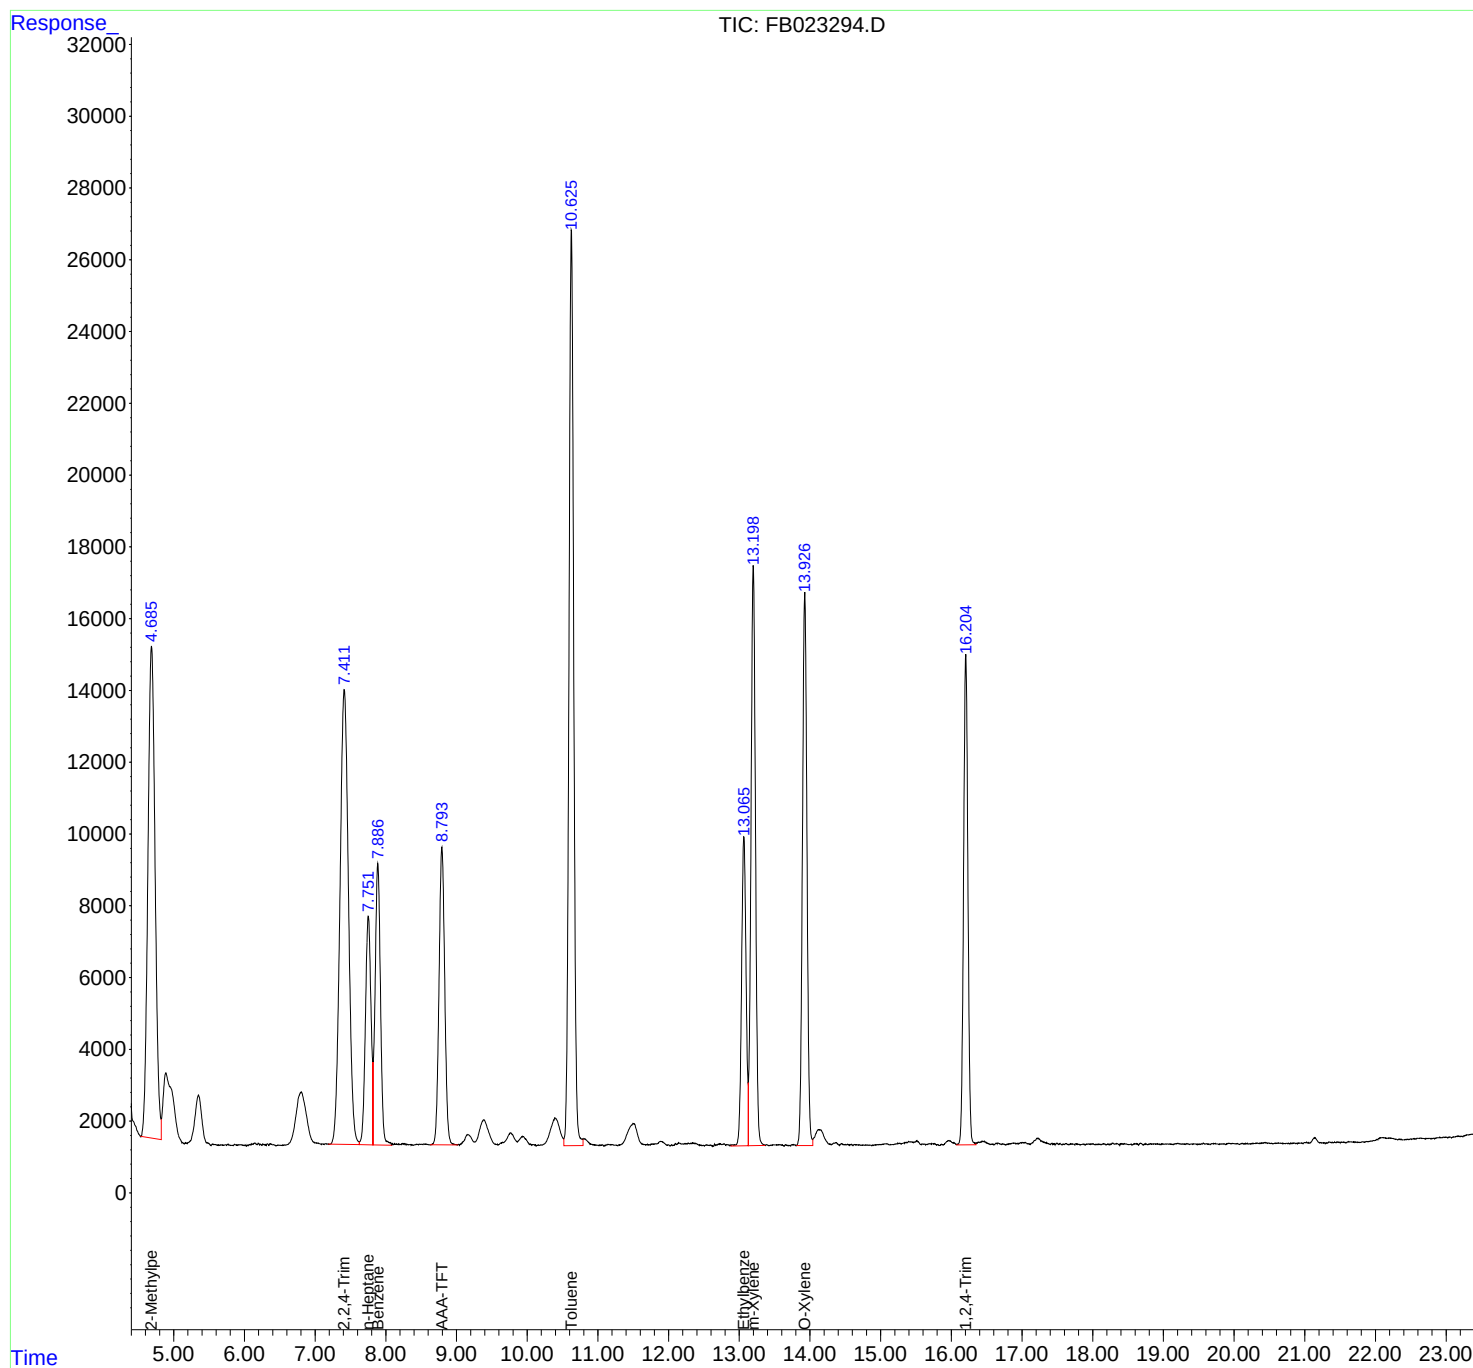

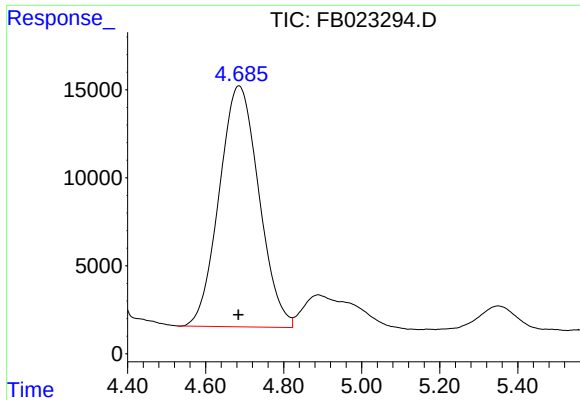


#1 2-Methylpentane

R.T.: 4.686 min
Delta R.T.: 0.002 min
Response: 967948
Conc: 31.27 ng/ml

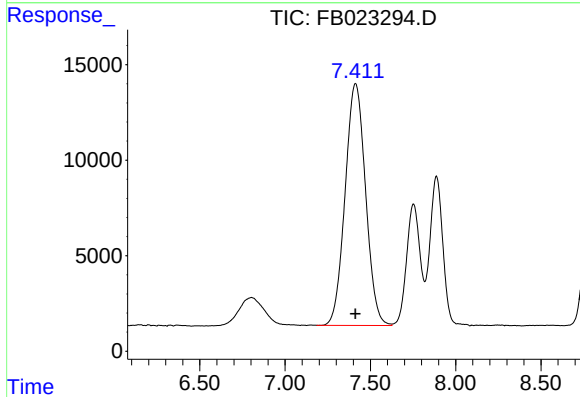


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: 0.001 min
Response: 1056319
Conc: 31.62 ng/ml

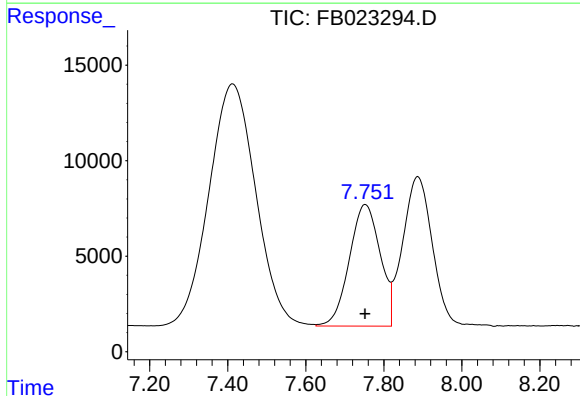


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.001 min
Response: 349630
Conc: 10.60 ng/ml

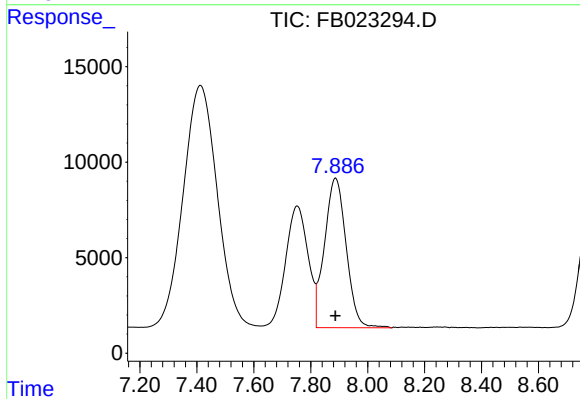


#4 Benzene

R.T.: 7.887 min
Delta R.T.: 0.001 min
Response: 414154
Conc: 10.37 ng/ml

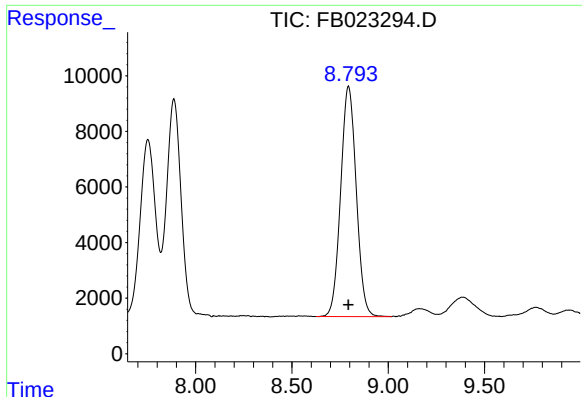


#5 AAA-TFT

R.T.: 8.794 min
Delta R.T.: 0.000 min
Response: 464095
Conc: 19.57 ng/ml

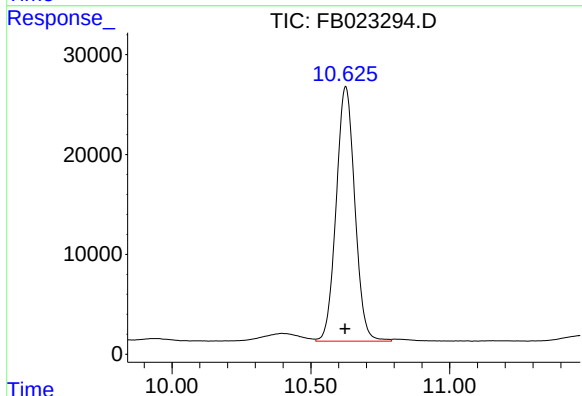


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.002 min
Response: 1188986
Conc: 30.88 ng/ml

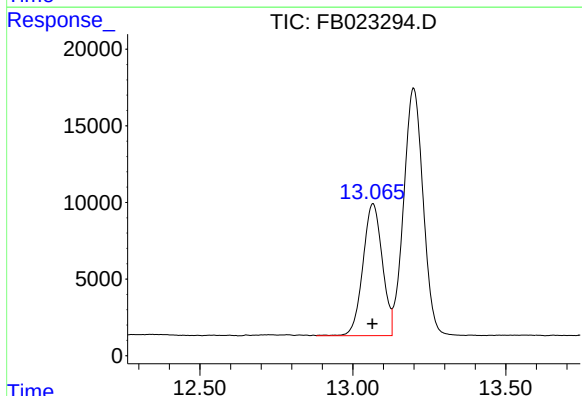


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: 0.002 min
Response: 378697
Conc: 10.43 ng/ml

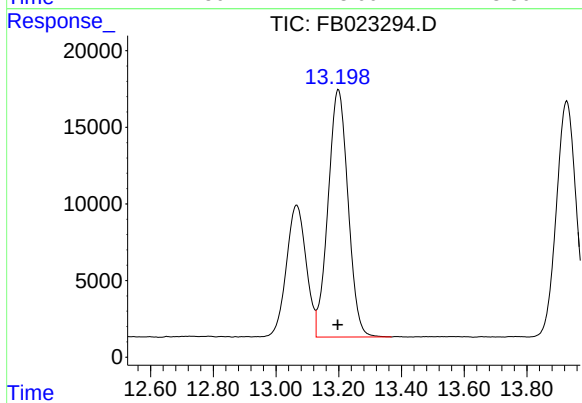

#8 m-Xylene

R.T.: 13.199 min
Delta R.T.: 0.002 min
Response: 714286
Conc: 20.58 ng/ml

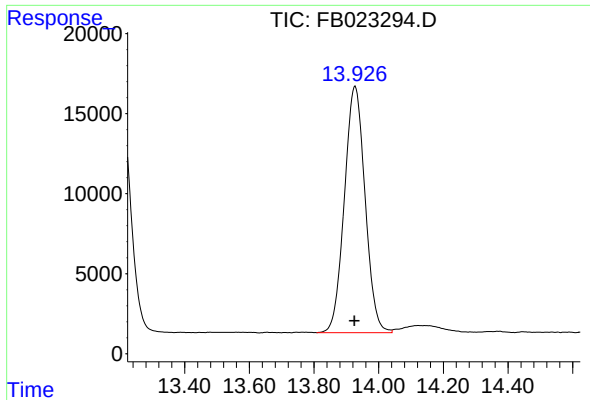


#9 O-Xylene

R.T.: 13.927 min

Delta R.T.: 0.002 min

Response: 683772

Conc: 20.30 ng/ml

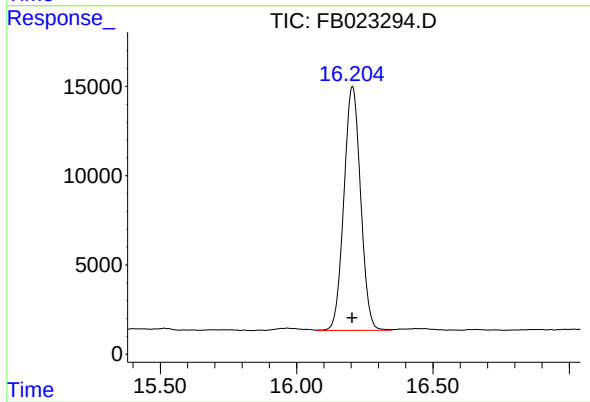

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min

Delta R.T.: 0.002 min

Response: 581631

Conc: 20.73 ng/ml