

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122618\
 Data File : FB019190.D
 Signal(s) : FID2B.CH
 Acq On : 26 Dec 2018 15:17
 Operator : MJ/SJ
 Sample : VBF1221S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 27 01:08:01 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
 Quant Title :
 QLast Update : Fri Dec 07 17:57:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.103	164094	18.774 ng/ml
Target Compounds			
4) t Benzene	8.195	11898	0.661 ng/ml
6) t Toluene	10.935	5660	0.373 ng/ml
8) t m-Xylene	13.570	13713	0.842 ng/ml
9) t O-Xylene	14.260	8913	0.527 ng/ml
10) t 1,2,4-Trimethylbenzene	16.558	7644	0.378 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122618\
Data File : FB019190.D
Signal(s) : FID2B.CH
Acq On : 26 Dec 2018 15:17
Operator : MJ/SJ
Sample : VBF1221S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 27 01:08:01 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
Quant Title :
QLast Update : Fri Dec 07 17:57:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

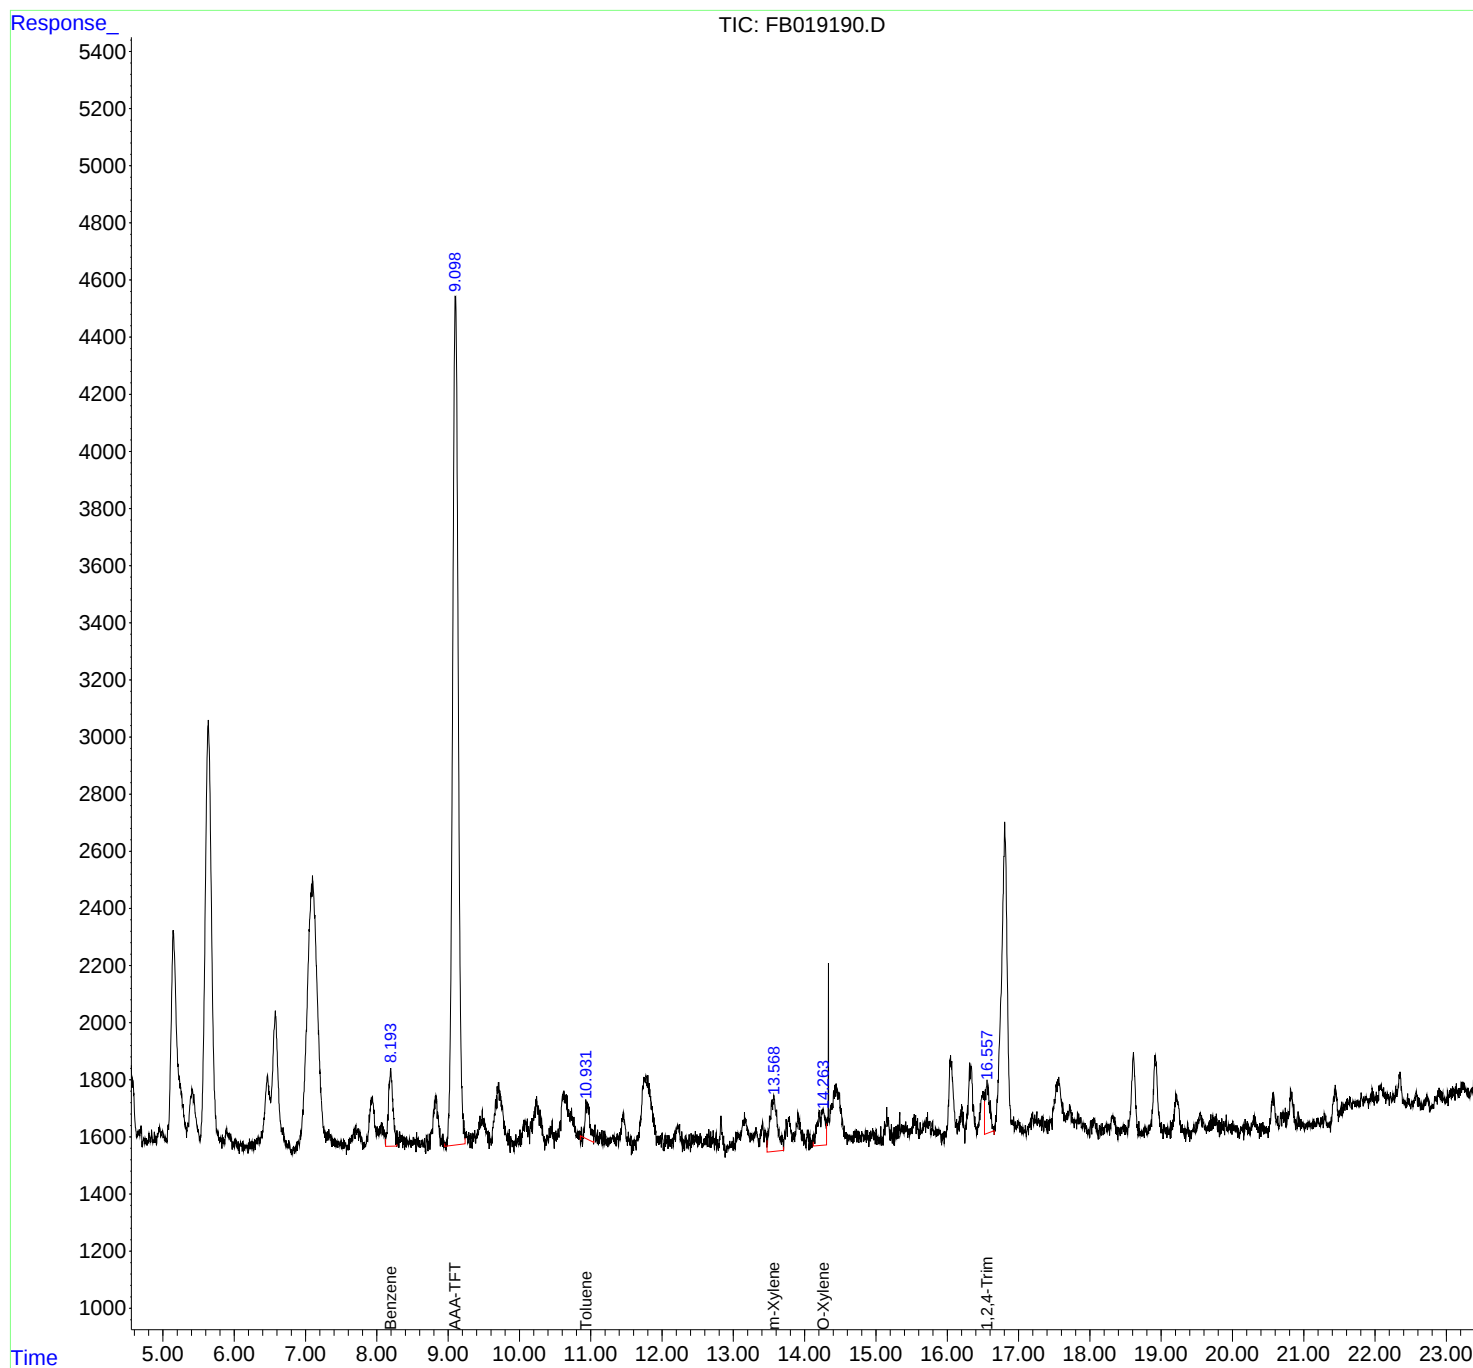


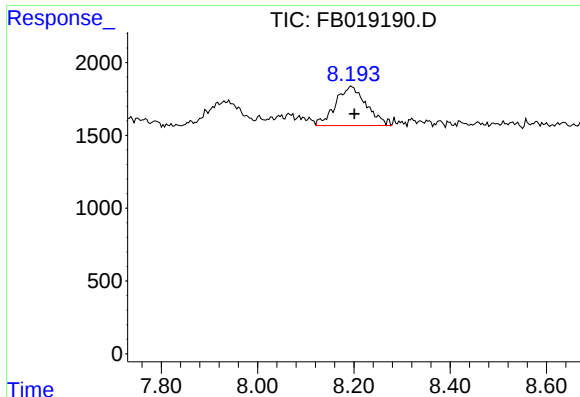

#4 Benzene


R.T.: 8.195 min
Delta R.T.: -0.006 min
Response: 11898
Conc: 0.66 ng/ml

Instrument :
FID_B
ClientSampleId :

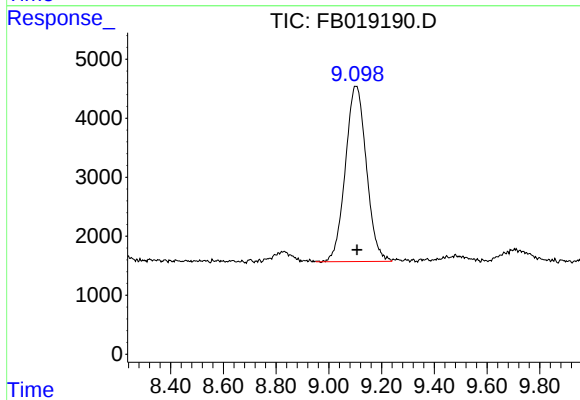


#5 AAA-TFT

R.T.: 9.103 min
Delta R.T.: -0.004 min
Response: 164094
Conc: 18.77 ng/ml

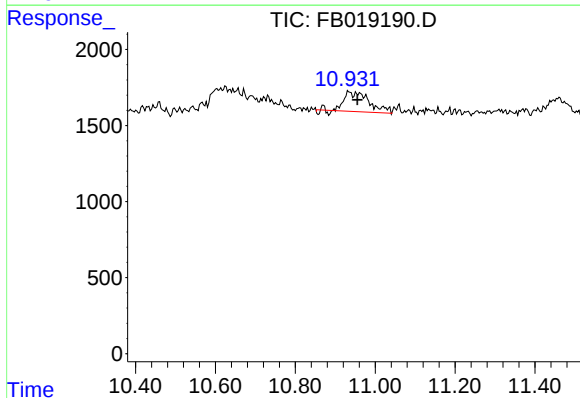


#6 Toluene

R.T.: 10.935 min
Delta R.T.: -0.020 min
Response: 5660
Conc: 0.37 ng/ml

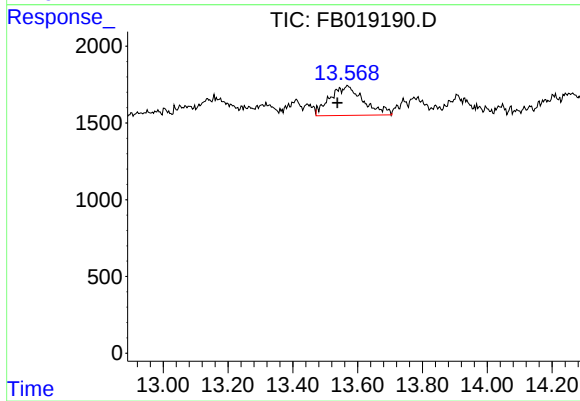

#8 m-Xylene


R.T.: 13.570 min
Delta R.T.: 0.032 min
Response: 13713
Conc: 0.84 ng/ml

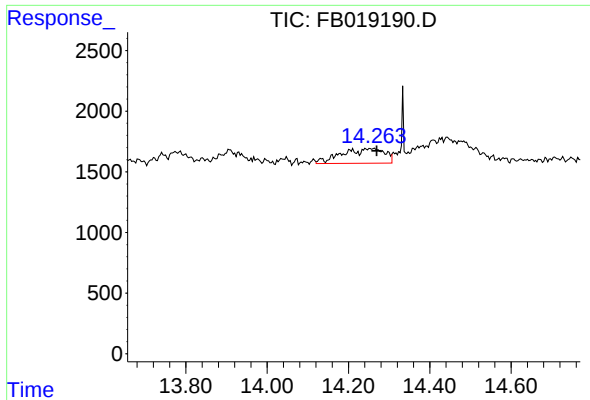

#9 O-Xylene

R.T.: 14.260 min
Delta R.T.: -0.010 min
Response: 8913
Conc: 0.53 ng/ml

Instrument :
FID_B
ClientSampleId :

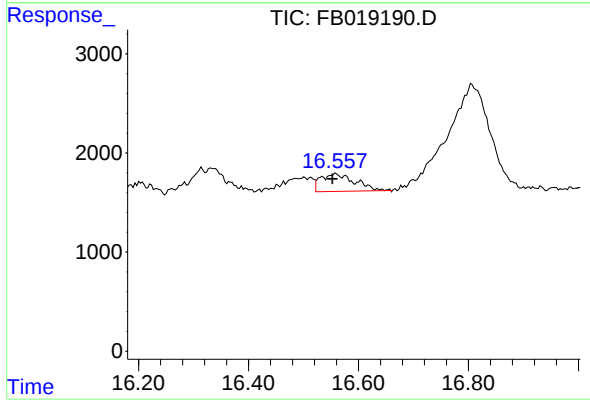

#10 1,2,4-Trimethylbenzene

R.T.: 16.558 min
Delta R.T.: 0.006 min
Response: 7644
Conc: 0.38 ng/ml