

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122618\
 Data File : FB019193.D
 Signal(s) : FID2B.CH
 Acq On : 26 Dec 2018 16:46
 Operator : MJ/SJ
 Sample : BSF1221W1
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 27 01:08:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
 Quant Title :
 QLast Update : Fri Dec 07 17:57:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.103	62422	7.142 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.960	143450	9.383 ng/ml
2) t 2,2,4-Trimethylpentane	7.723	160756	10.435 ng/ml
3) t n-Heptane	8.063	51583	3.471 ng/ml
4) t Benzene	8.198	40886	2.270 ng/ml
6) t Toluene	10.956	133282	8.781 ng/ml
7) t Ethylbenzene	13.400	50816	3.271 ng/ml
8) t m-Xylene	13.537	102269	6.277 ng/ml
9) t O-Xylene	14.268	85188	5.038 ng/ml
10) t 1,2,4-Trimethylbenzene	16.551	83726	4.137 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122618\
Data File : FB019193.D
Signal(s) : FID2B.CH
Acq On : 26 Dec 2018 16:46
Operator : MJ/SJ
Sample : BSF1221W1
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 27 01:08:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
Quant Title :
QLast Update : Fri Dec 07 17:57:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

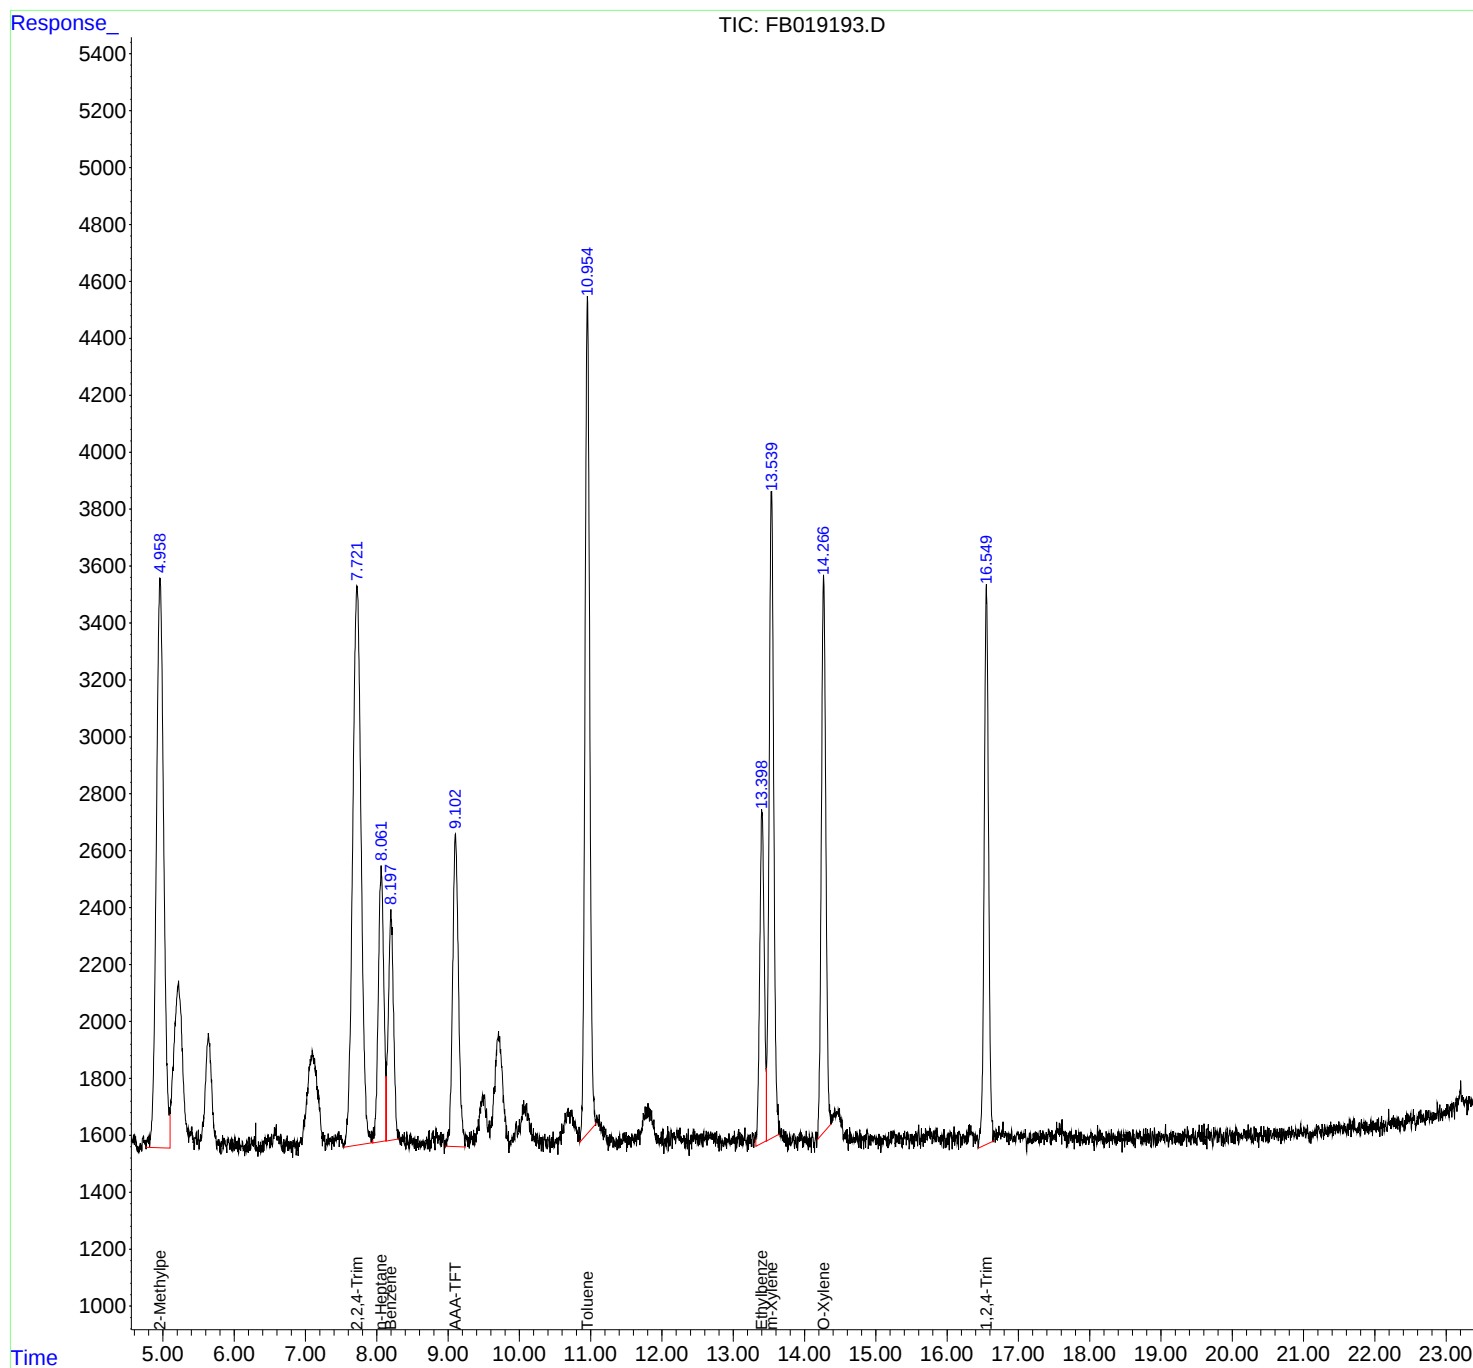


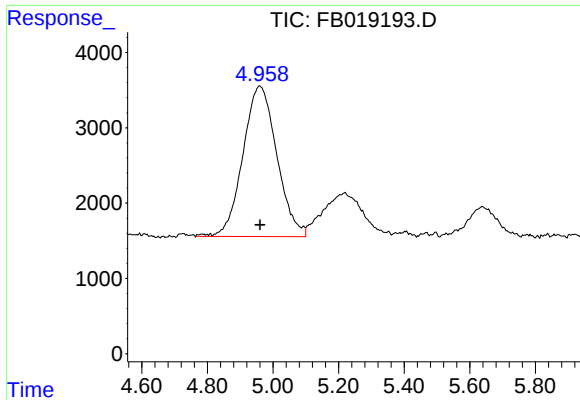

#1 2-Methylpentane


R.T.: 4.960 min
Delta R.T.: 0.000 min
Response: 143450
Conc: 9.38 ng/ml

Instrument :
FID_B
ClientSampleId :

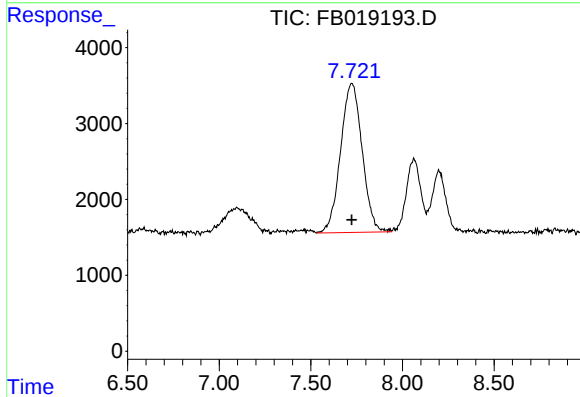


#2 2,2,4-Trimethylpentane

R.T.: 7.723 min
Delta R.T.: 0.000 min
Response: 160756
Conc: 10.43 ng/ml

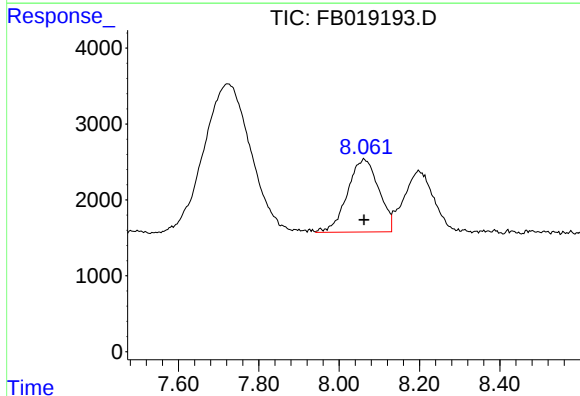


#3 n-Heptane

R.T.: 8.063 min
Delta R.T.: 0.000 min
Response: 51583
Conc: 3.47 ng/ml

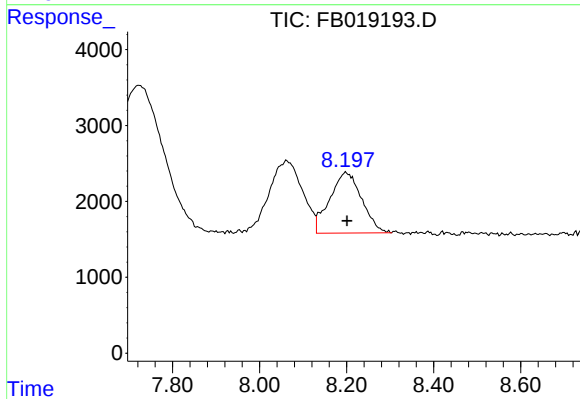

#4 Benzene


R.T.: 8.198 min
Delta R.T.: -0.003 min
Response: 40886
Conc: 2.27 ng/ml

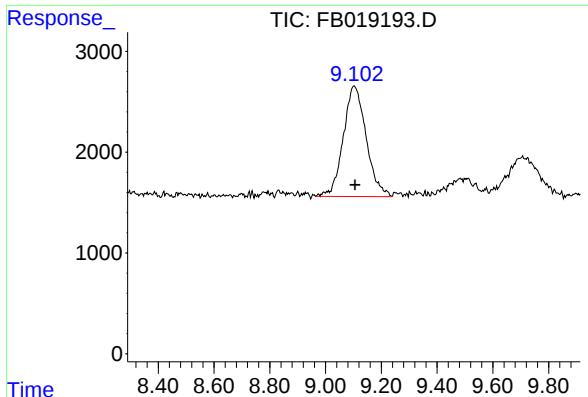

#5 AAA-TFT


R.T.: 9.103 min
Delta R.T.: -0.003 min
Response: 62422
Conc: 7.14 ng/ml

Instrument :
FID_B
ClientSampleId :

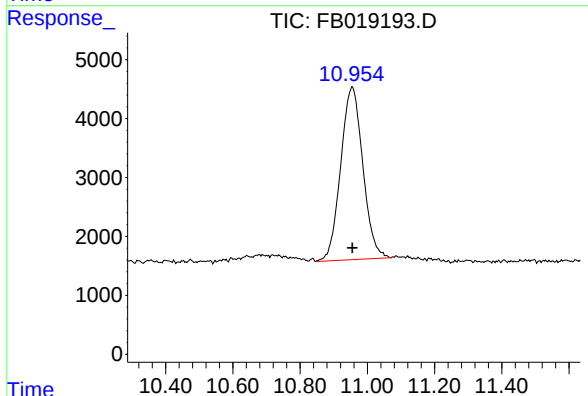


#6 Toluene

R.T.: 10.956 min
Delta R.T.: 0.000 min
Response: 133282
Conc: 8.78 ng/ml

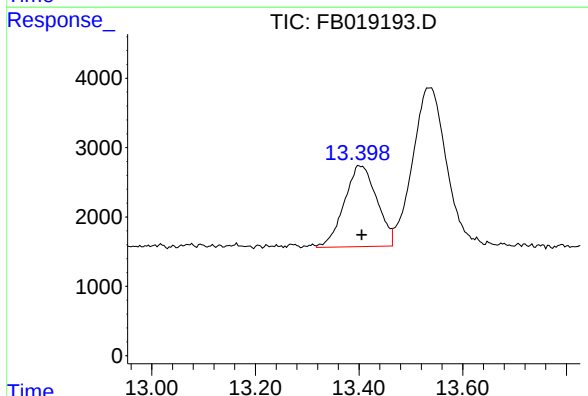


#7 Ethylbenzene

R.T.: 13.400 min
Delta R.T.: -0.005 min
Response: 50816
Conc: 3.27 ng/ml

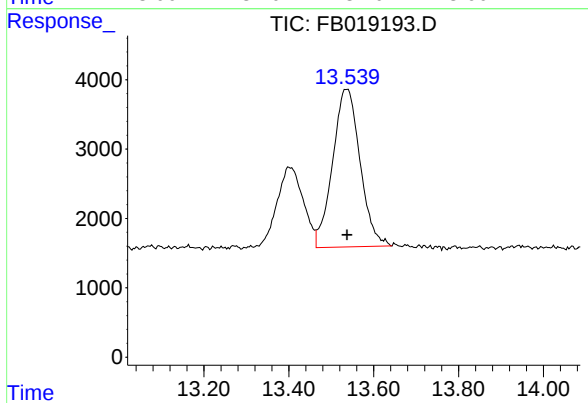

#8 m-Xylene


R.T.: 13.537 min
Delta R.T.: 0.000 min
Response: 102269
Conc: 6.28 ng/ml

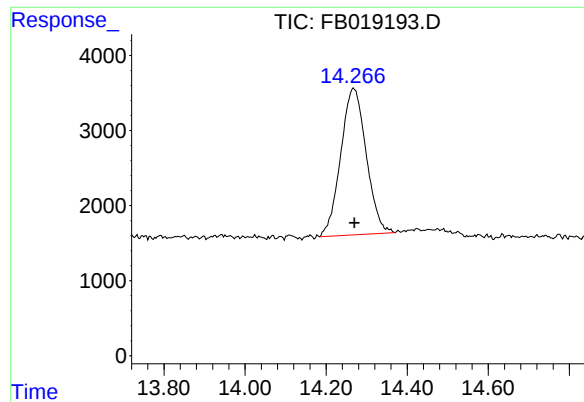

#9 O-Xylene

R.T.: 14.268 min
Delta R.T.: -0.001 min
Response: 85188
Conc: 5.04 ng/ml

Instrument :
FID_B
ClientSampleId :

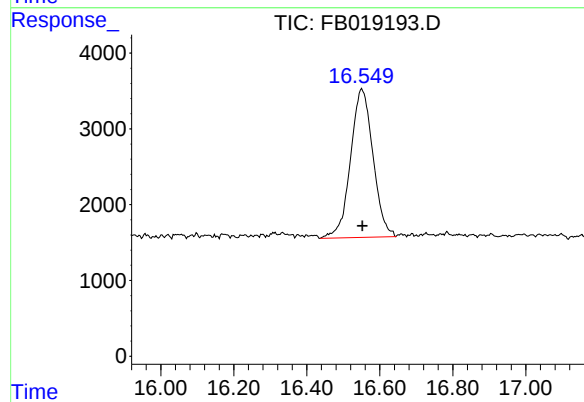

#10 1,2,4-Trimethylbenzene

R.T.: 16.551 min
Delta R.T.: -0.002 min
Response: 83726
Conc: 4.14 ng/ml