

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122618\
 Data File : FB019191.D
 Signal(s) : FID2B.CH
 Acq On : 26 Dec 2018 15:46
 Operator : MJ/SJ
 Sample : BSF1226S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1226S1

Integration File: Calibration.e
 Quant Time: Dec 27 01:08:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
 Quant Title :
 QLast Update : Fri Dec 07 17:57:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.103	186058	21.286 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.956	441582	28.885 ng/ml
2) t 2,2,4-Trimethylpentane	7.718	476653	30.940 ng/ml
3) t n-Heptane	8.060	151594	10.199 ng/ml
4) t Benzene	8.198	192530	10.689 ng/ml
6) t Toluene	10.952	486188	32.030 ng/ml
7) t Ethylbenzene	13.402	161097	10.369 ng/ml
8) t m-Xylene	13.535	341077	20.936 ng/ml
9) t O-Xylene	14.266	351870	20.810 ng/ml
10) t 1,2,4-Trimethylbenzene	16.550	415517	20.532 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122618\
Data File : FB019191.D
Signal(s) : FID2B.CH
Acq On : 26 Dec 2018 15:46
Operator : MJ/SJ
Sample : BSF1226S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1226S1

Integration File: Calibration.e
Quant Time: Dec 27 01:08:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
Quant Title :
QLast Update : Fri Dec 07 17:57:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

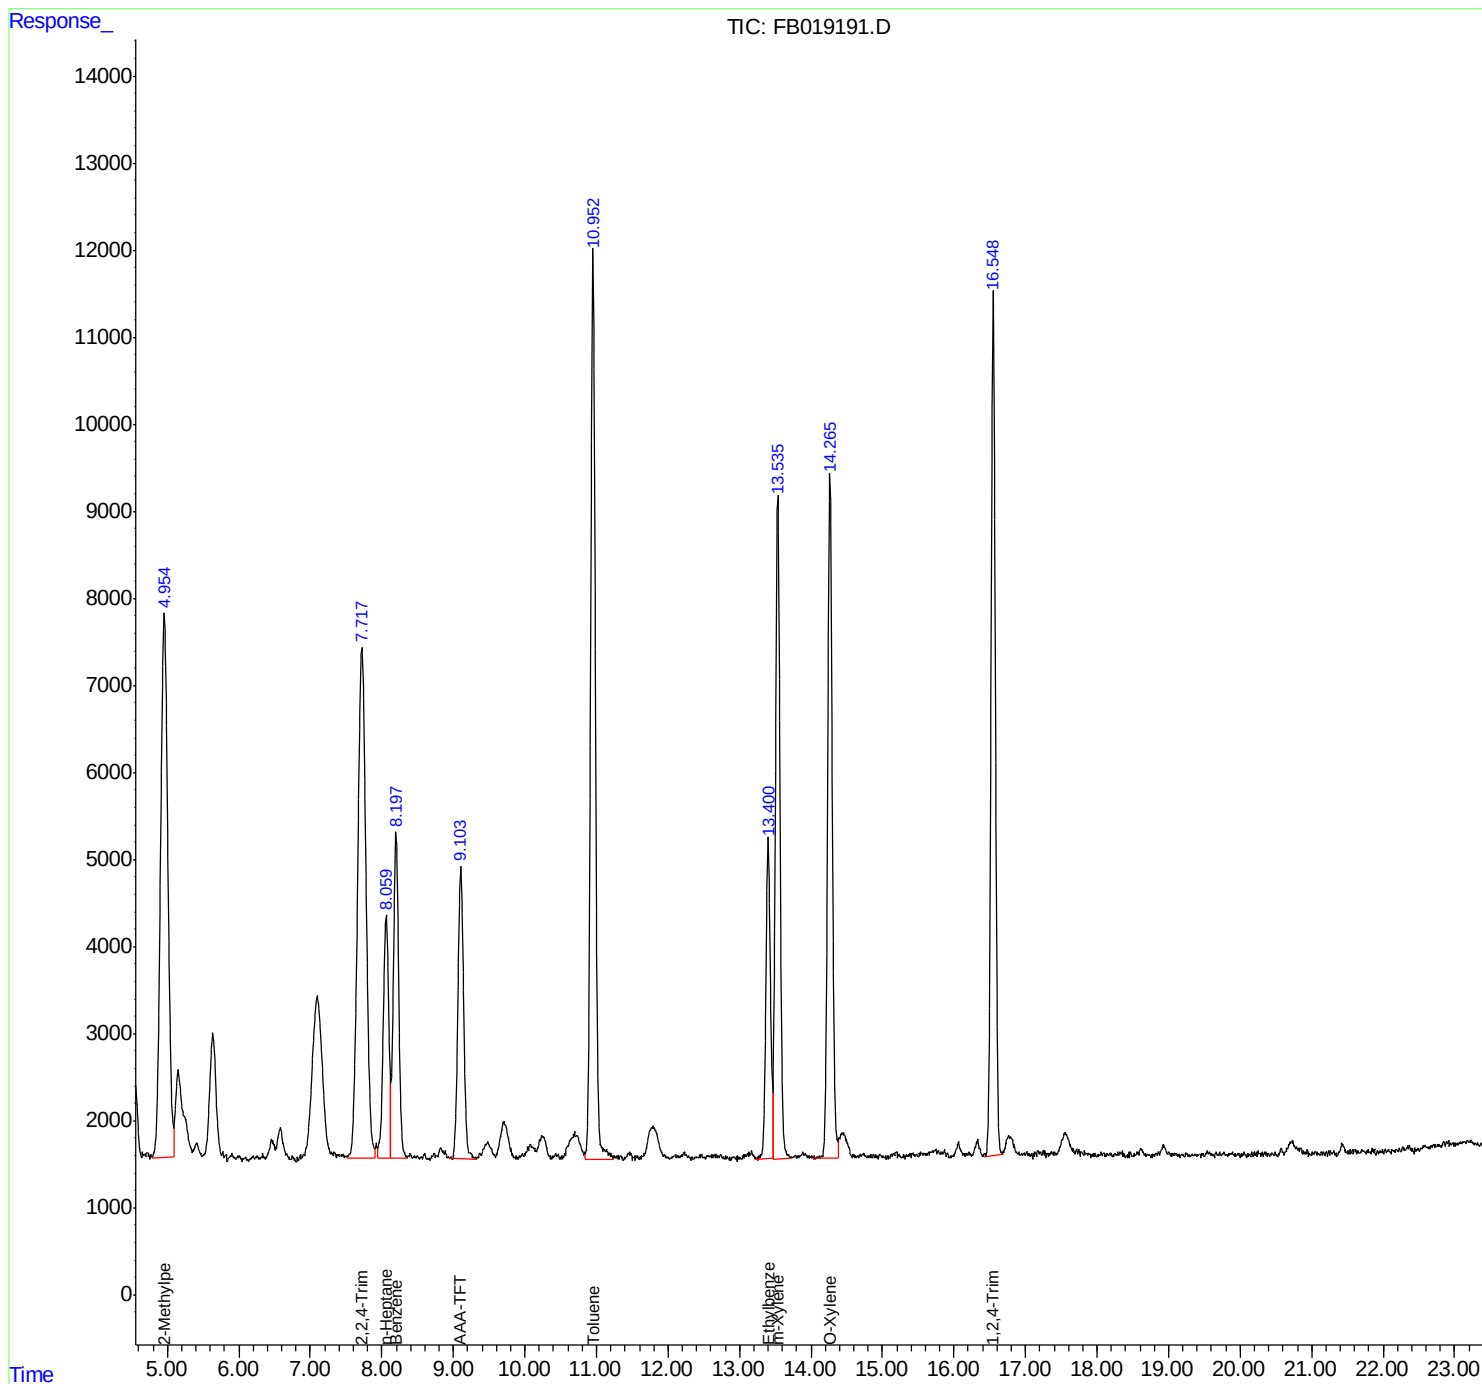


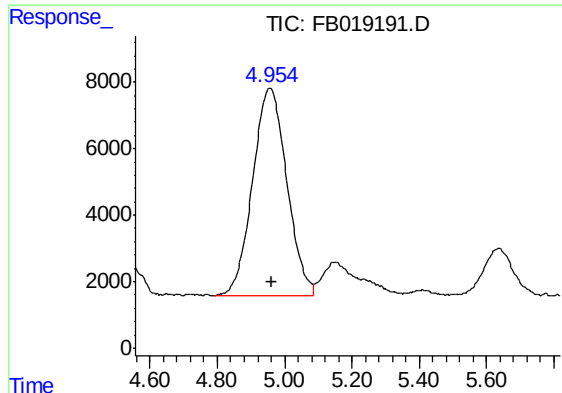

#1 2-Methylpentane


R.T.: 4.956 min
Delta R.T.: -0.005 min
Response: 441582
Conc: 28.88 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1226S1

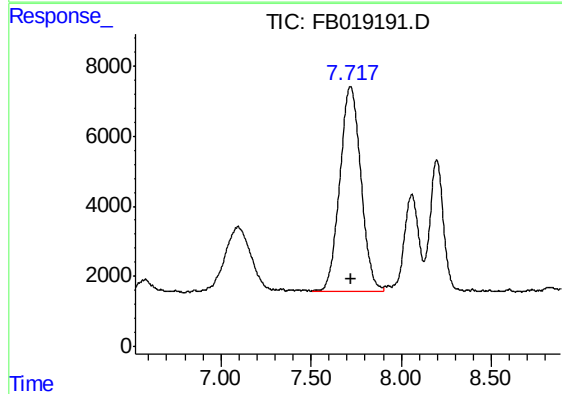


#2 2,2,4-Trimethylpentane

R.T.: 7.718 min
Delta R.T.: -0.004 min
Response: 476653
Conc: 30.94 ng/ml

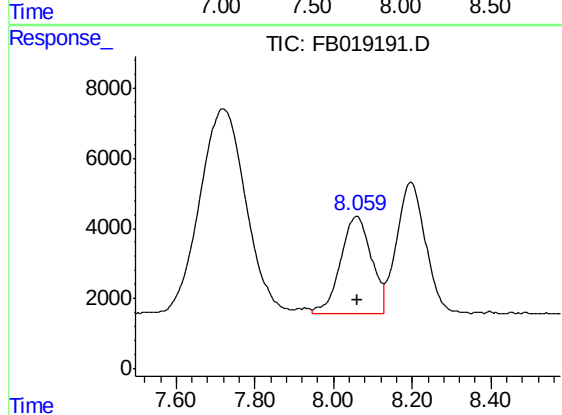


#3 n-Heptane

R.T.: 8.060 min
Delta R.T.: -0.002 min
Response: 151594
Conc: 10.20 ng/ml

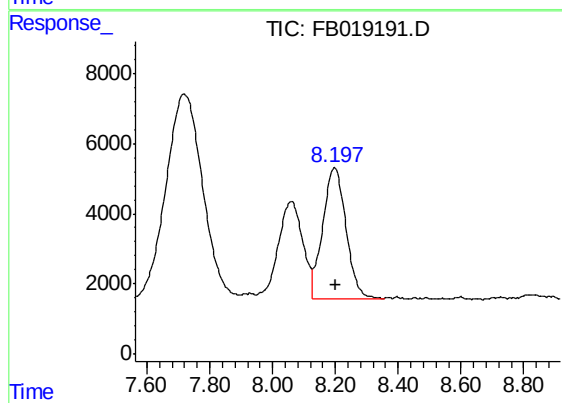

#4 Benzene


R.T.: 8.198 min
Delta R.T.: -0.003 min
Response: 192530
Conc: 10.69 ng/ml

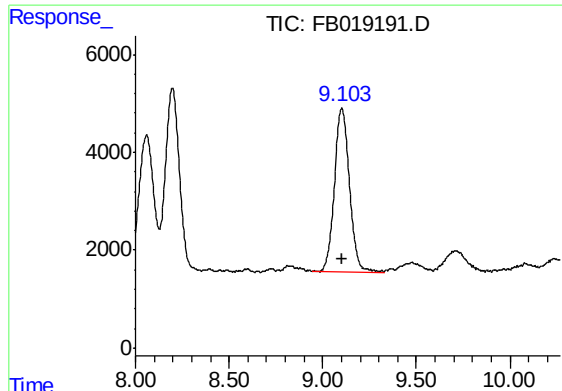

#5 AAA-TFT


R.T.: 9.103 min
Delta R.T.: -0.003 min
Response: 186058
Conc: 21.29 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1226S1

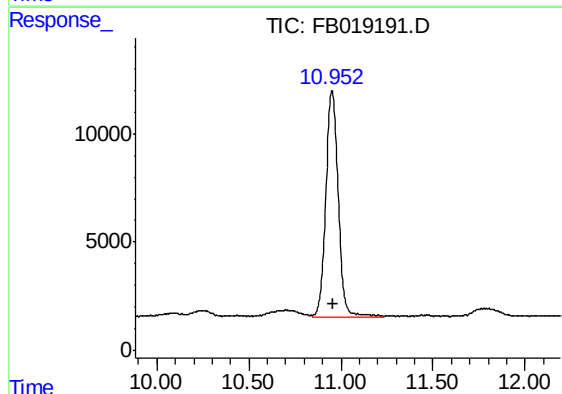


#6 Toluene

R.T.: 10.952 min
Delta R.T.: -0.003 min
Response: 486188
Conc: 32.03 ng/ml

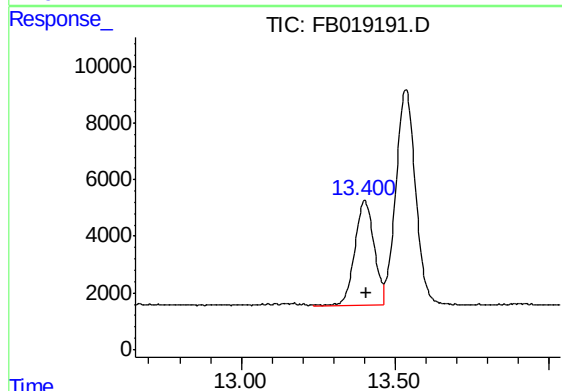


#7 Ethylbenzene

R.T.: 13.402 min
Delta R.T.: -0.004 min
Response: 161097
Conc: 10.37 ng/ml

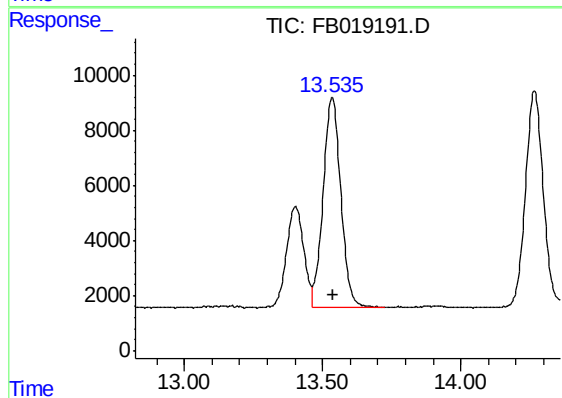

#8 m-Xylene


R.T.: 13.535 min
Delta R.T.: -0.003 min
Response: 341077
Conc: 20.94 ng/ml

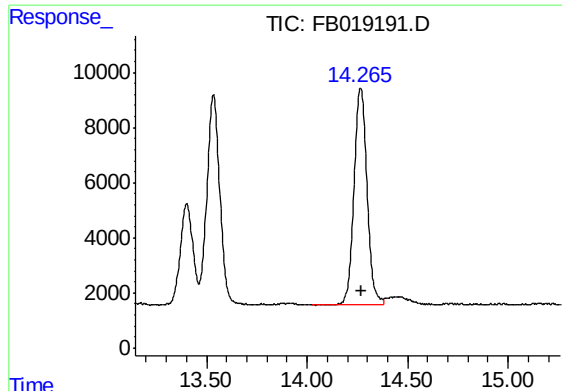

#9 O-Xylene

R.T.: 14.266 min
Delta R.T.: -0.003 min
Response: 351870
Conc: 20.81 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1226S1

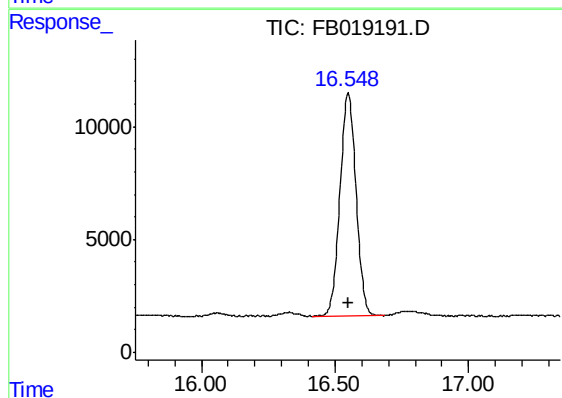

#10 1,2,4-Trimethylbenzene

R.T.: 16.550 min
Delta R.T.: -0.003 min
Response: 415517
Conc: 20.53 ng/ml