

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122618\
 Data File : FB019196.D
 Signal(s) : FID2B.CH
 Acq On : 26 Dec 2018 18:15
 Operator : MJ/SJ
 Sample : J6188-05MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BU-03-122118MS

Integration File: Calibration.e
 Quant Time: Dec 27 01:08:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
 Quant Title :
 QLast Update : Fri Dec 07 17:57:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.105	160083	18.315 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.957	376922	24.655 ng/ml
2) t 2,2,4-Trimethylpentane	7.720	374215	24.290 ng/ml
3) t n-Heptane	8.059	116824	7.860 ng/ml
4) t Benzene	8.198	176866	9.819 ng/ml
6) t Toluene	10.953	423989	27.933 ng/ml
7) t Ethylbenzene	13.402	137649	8.860 ng/ml
8) t m-Xylene	13.535	286948	17.613 ng/ml
9) t O-Xylene	14.267	302052	17.864 ng/ml
10) t 1,2,4-Trimethylbenzene	16.550	339207	16.761 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122618\
Data File : FB019196.D
Signal(s) : FID2B.CH
Acq On : 26 Dec 2018 18:15
Operator : MJ/SJ
Sample : J6188-05MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BU-03-122118MS

Integration File: Calibration.e
Quant Time: Dec 27 01:08:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
Quant Title :
QLast Update : Fri Dec 07 17:57:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

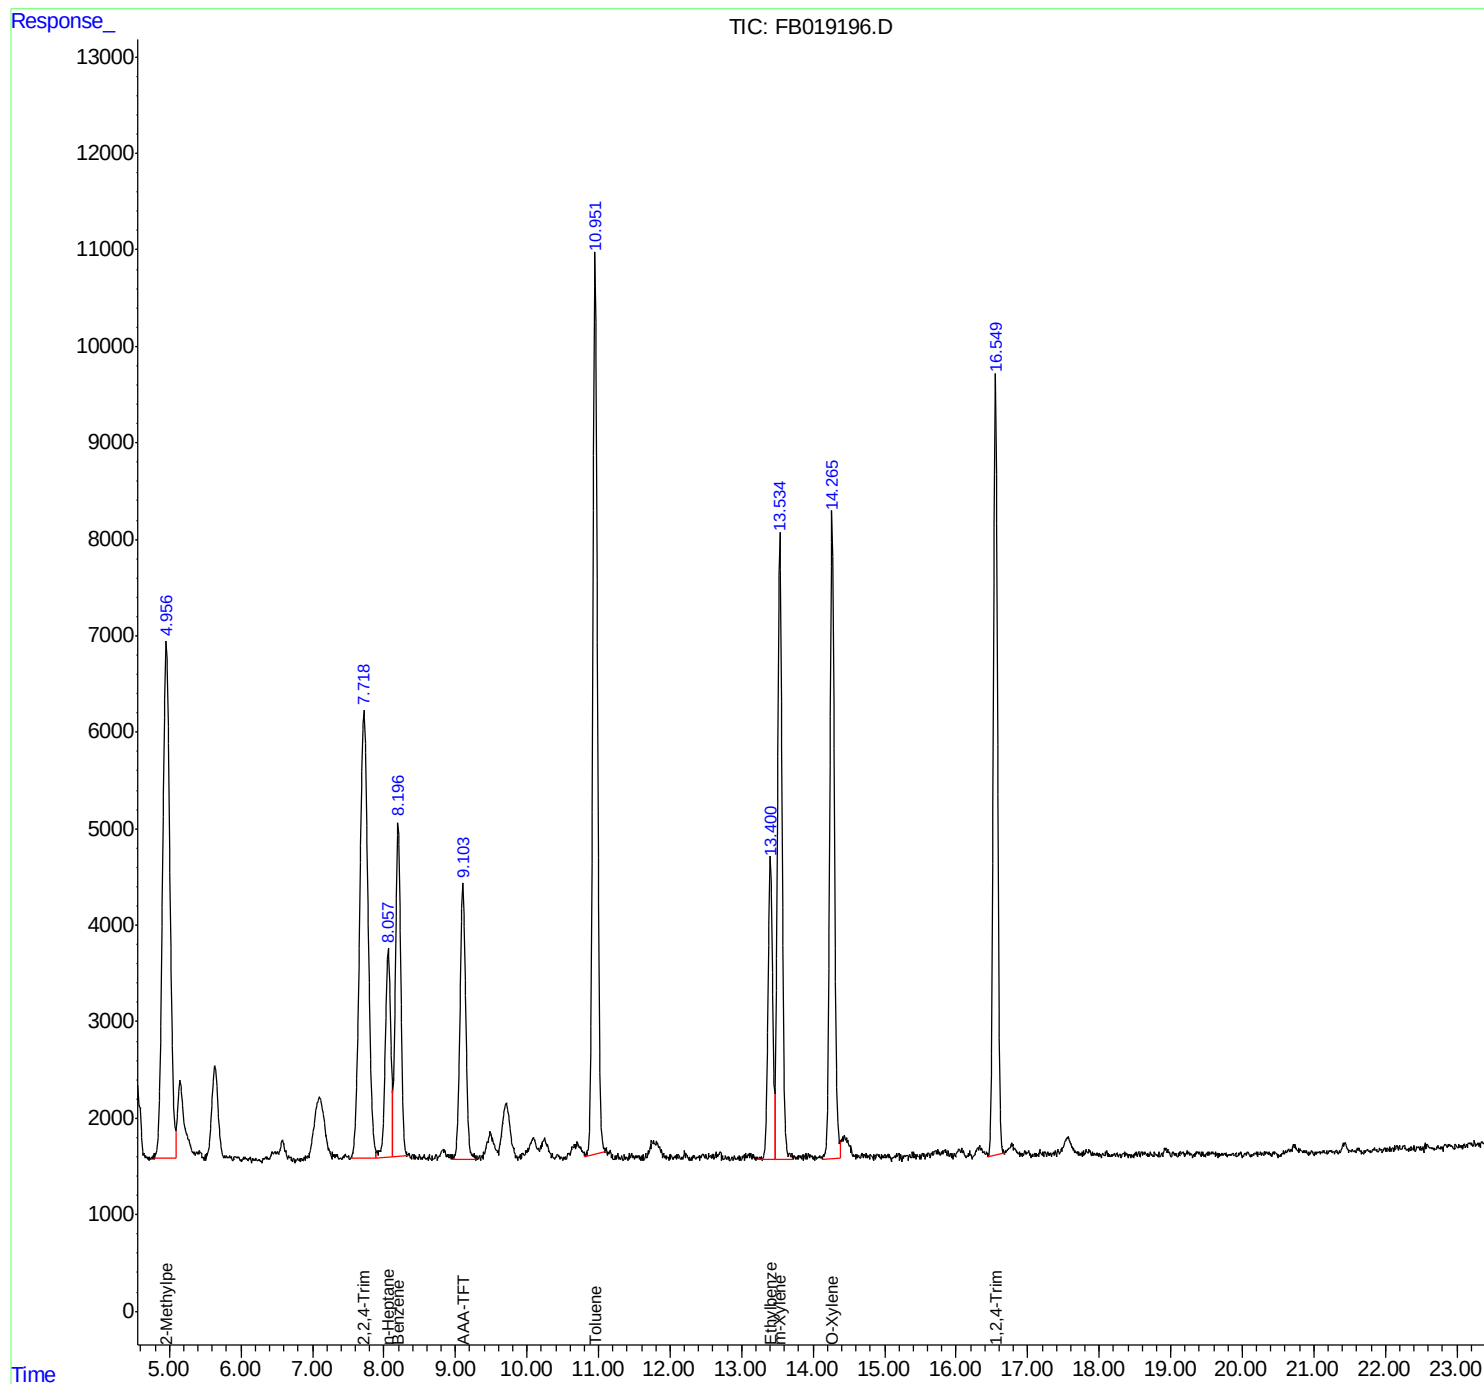


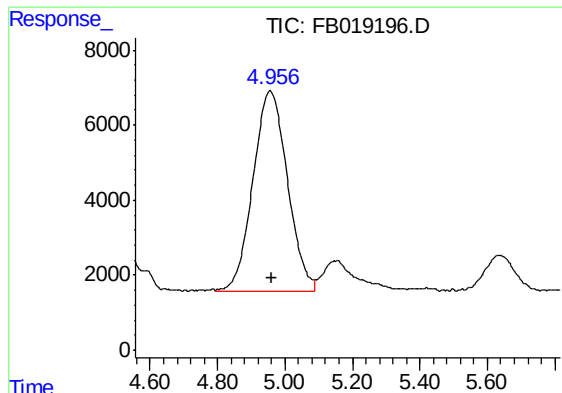

#1 2-Methylpentane


R.T.: 4.957 min
Delta R.T.: -0.004 min
Response: 376922
Conc: 24.66 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-122118MS

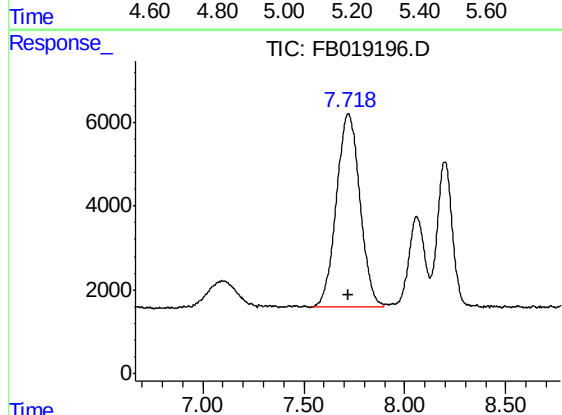


#2 2,2,4-Trimethylpentane

R.T.: 7.720 min
Delta R.T.: -0.003 min
Response: 374215
Conc: 24.29 ng/ml

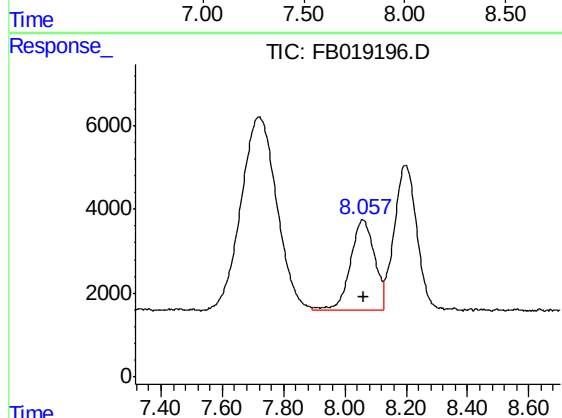


#3 n-Heptane

R.T.: 8.059 min
Delta R.T.: -0.003 min
Response: 116824
Conc: 7.86 ng/ml

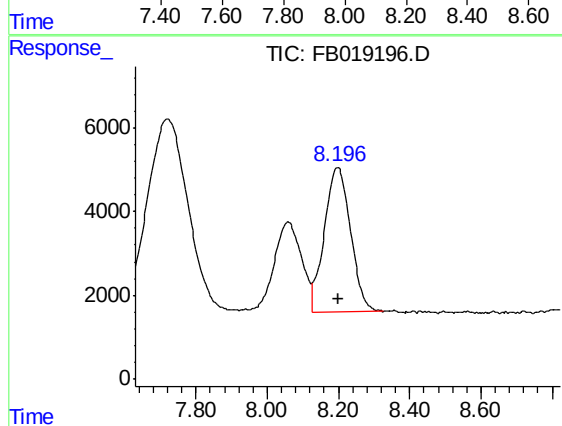

#4 Benzene


R.T.: 8.198 min
Delta R.T.: -0.003 min
Response: 176866
Conc: 9.82 ng/ml

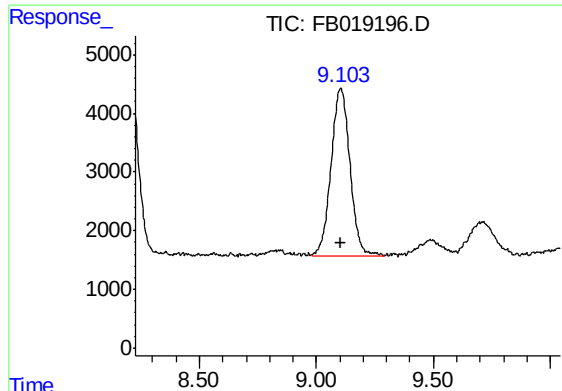

#5 AAA-TFT


R.T.: 9.105 min
Delta R.T.: -0.002 min
Response: 160083
Conc: 18.31 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-122118MS

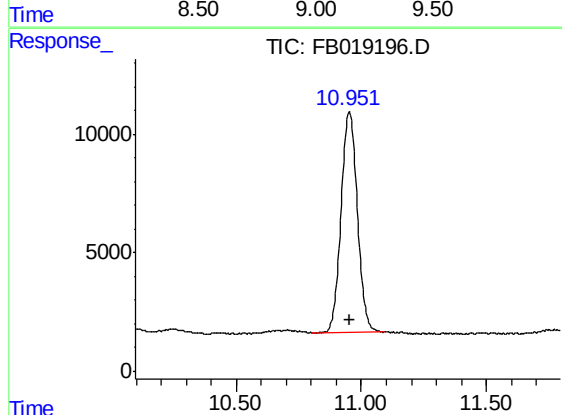


#6 Toluene

R.T.: 10.953 min
Delta R.T.: -0.003 min
Response: 423989
Conc: 27.93 ng/ml

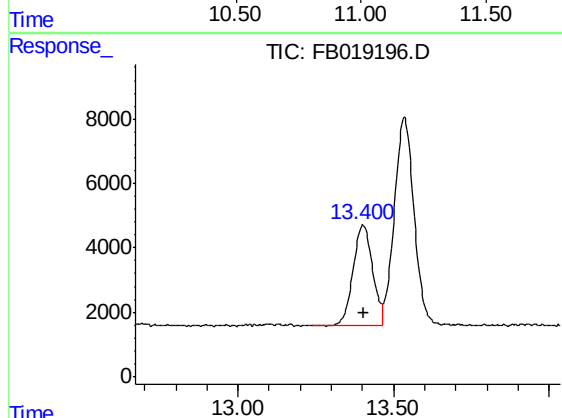


#7 Ethylbenzene

R.T.: 13.402 min
Delta R.T.: -0.003 min
Response: 137649
Conc: 8.86 ng/ml

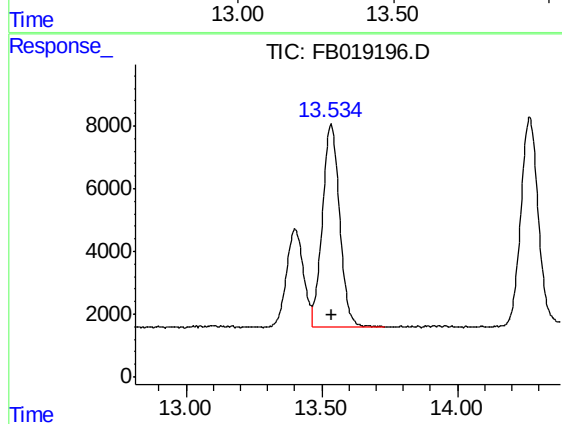

#8 m-Xylene


R.T.: 13.535 min
Delta R.T.: -0.002 min
Response: 286948
Conc: 17.61 ng/ml

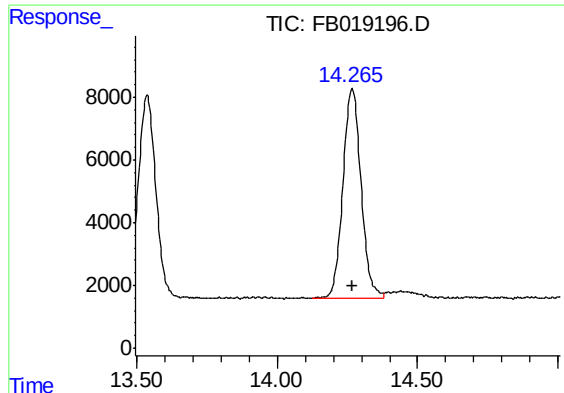

#9 O-Xylene

R.T.: 14.267 min
Delta R.T.: -0.003 min
Response: 302052
Conc: 17.86 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-122118MS

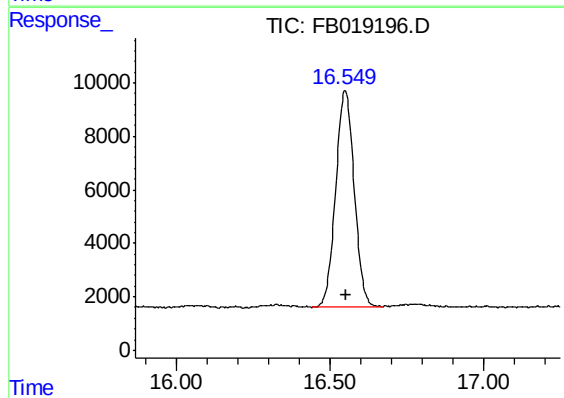

#10 1,2,4-Trimethylbenzene

R.T.: 16.550 min
Delta R.T.: -0.003 min
Response: 339207
Conc: 16.76 ng/ml