

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122618\
 Data File : FB019197.D
 Signal(s) : FID2B.CH
 Acq On : 26 Dec 2018 18:44
 Operator : MJ/SJ
 Sample : J6188-05MSD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BU-03-122118MSD

Integration File: Calibration.e
 Quant Time: Dec 27 01:09:10 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
 Quant Title :
 QLast Update : Fri Dec 07 17:57:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.100	159023	18.193 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.947	369647	24.180 ng/ml
2) t 2,2,4-Trimethylpentane	7.714	376217	24.420 ng/ml
3) t n-Heptane	8.055	117347	7.895 ng/ml
4) t Benzene	8.193	181786	10.092 ng/ml
6) t Toluene	10.950	419349	27.627 ng/ml
7) t Ethylbenzene	13.400	132622	8.536 ng/ml
8) t m-Xylene	13.533	278022	17.065 ng/ml
9) t O-Xylene	14.265	292240	17.284 ng/ml
10) t 1,2,4-Trimethylbenzene	16.549	324143	16.017 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122618\
Data File : FB019197.D
Signal(s) : FID2B.CH
Acq On : 26 Dec 2018 18:44
Operator : MJ/SJ
Sample : J6188-05MSD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BU-03-122118MSD

Integration File: Calibration.e
Quant Time: Dec 27 01:09:10 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
Quant Title :
QLast Update : Fri Dec 07 17:57:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

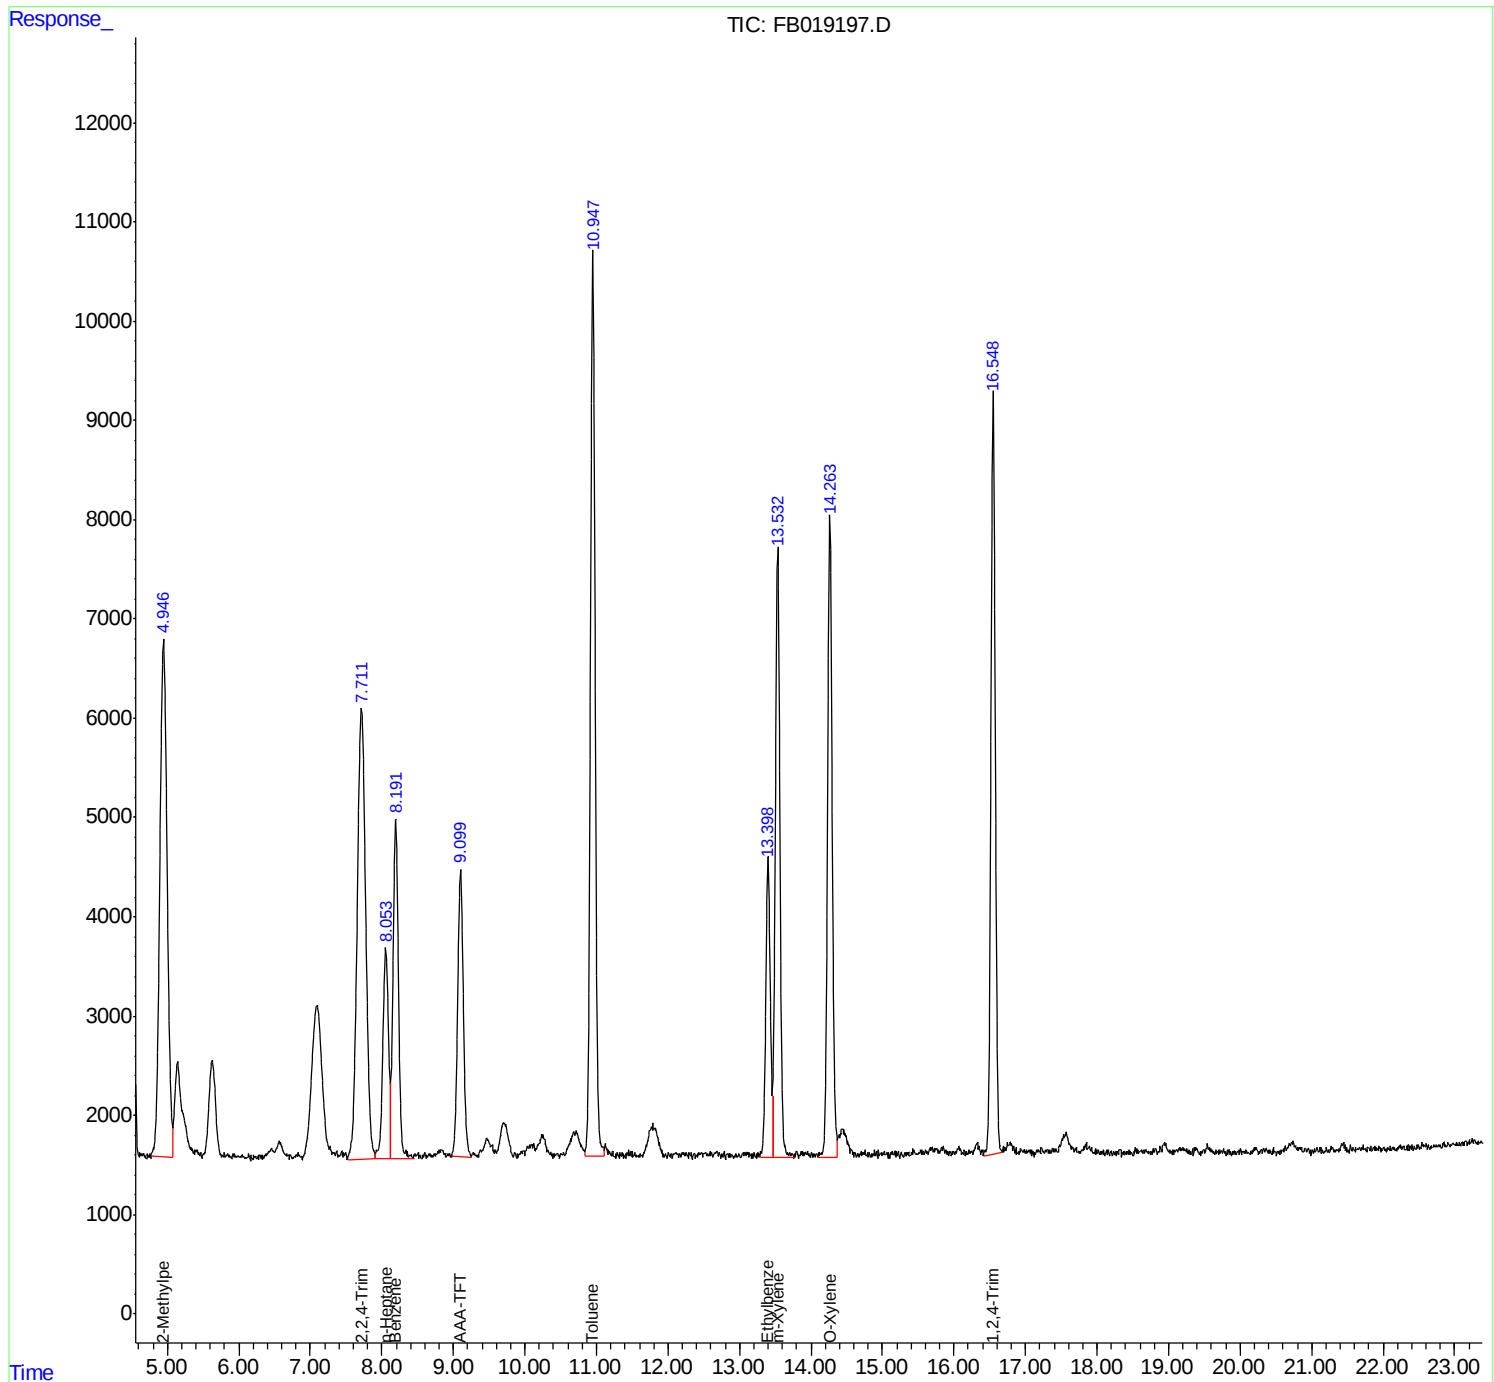


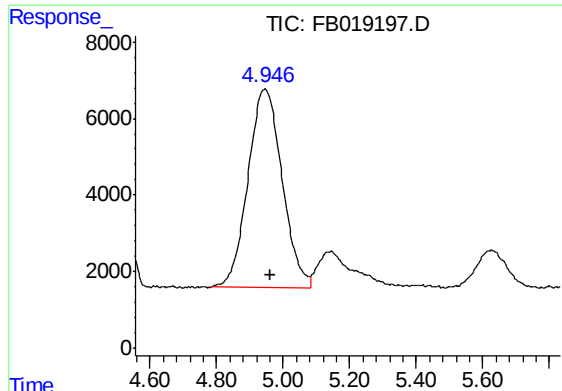

#1 2-Methylpentane


R.T.: 4.947 min
Delta R.T.: -0.014 min
Response: 369647
Conc: 24.18 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-122118MSD

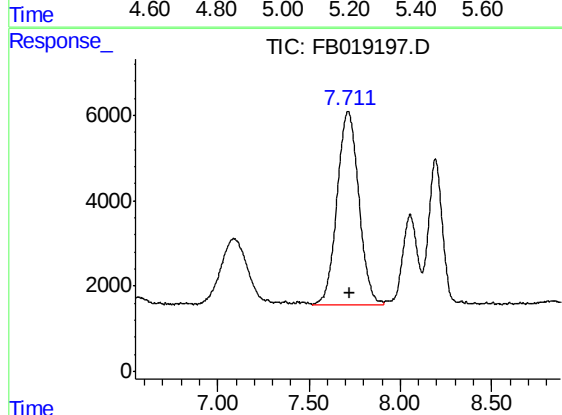


#2 2,2,4-Trimethylpentane

R.T.: 7.714 min
Delta R.T.: -0.009 min
Response: 376217
Conc: 24.42 ng/ml

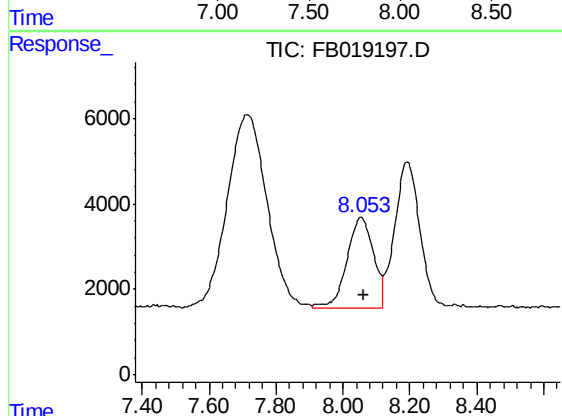


#3 n-Heptane

R.T.: 8.055 min
Delta R.T.: -0.008 min
Response: 117347
Conc: 7.90 ng/ml

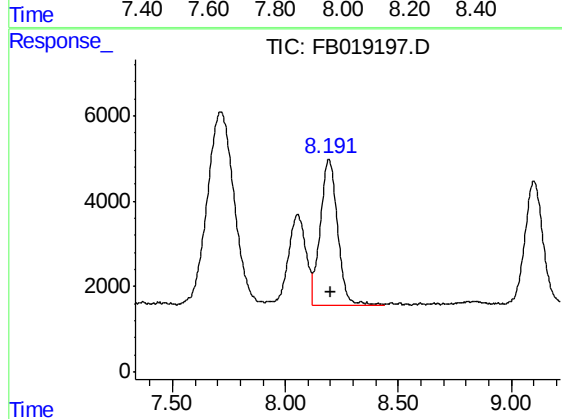

#4 Benzene


R.T.: 8.193 min
Delta R.T.: -0.008 min
Response: 181786
Conc: 10.09 ng/ml

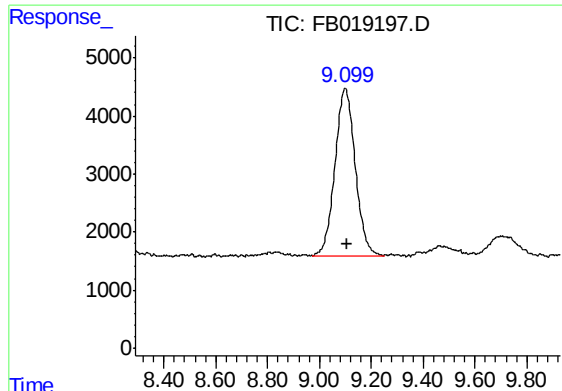

#5 AAA-TFT


R.T.: 9.100 min
Delta R.T.: -0.007 min
Response: 159023
Conc: 18.19 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-122118MSD

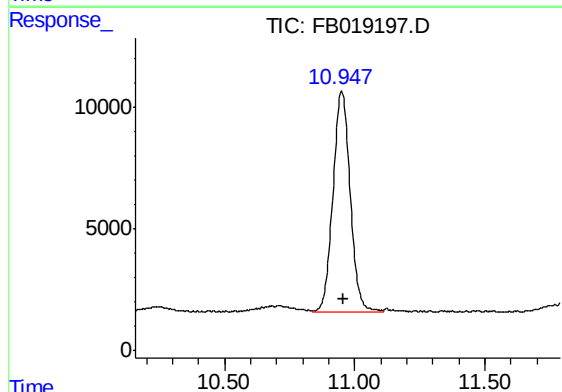


#6 Toluene

R.T.: 10.950 min
Delta R.T.: -0.006 min
Response: 419349
Conc: 27.63 ng/ml

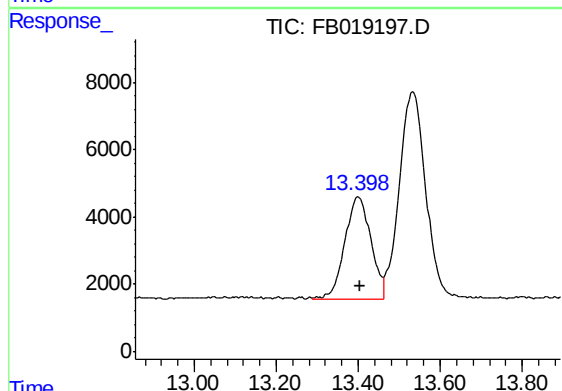


#7 Ethylbenzene

R.T.: 13.400 min
Delta R.T.: -0.005 min
Response: 132622
Conc: 8.54 ng/ml

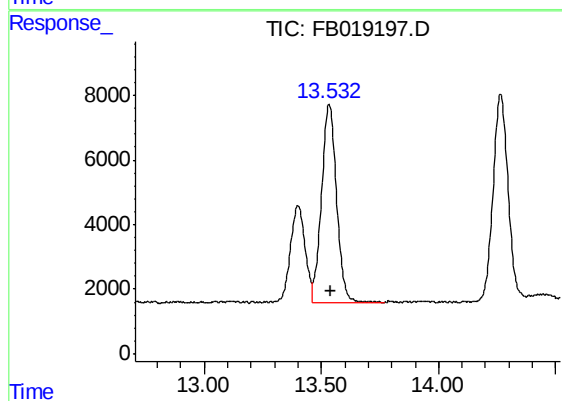

#8 m-Xylene


R.T.: 13.533 min
Delta R.T.: -0.004 min
Response: 278022
Conc: 17.07 ng/ml

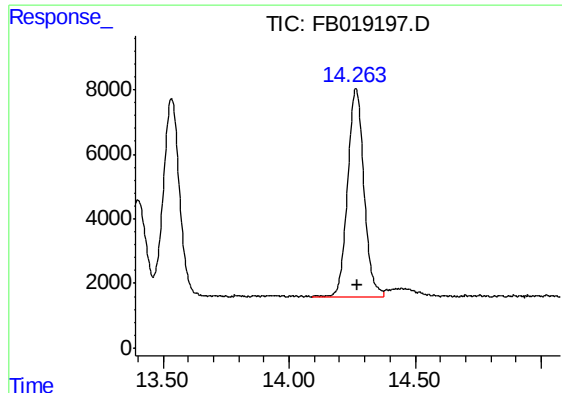

#9 O-Xylene

R.T.: 14.265 min
Delta R.T.: -0.005 min
Response: 292240
Conc: 17.28 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-122118MSD

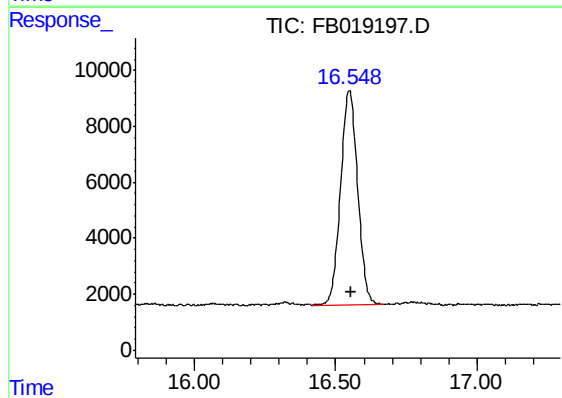

#10 1,2,4-Trimethylbenzene

R.T.: 16.549 min
Delta R.T.: -0.004 min
Response: 324143
Conc: 16.02 ng/ml