

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122619\
 Data File : FB023307.D
 Signal(s) : FID2B.CH
 Acq On : 26 Dec 2019 11:58
 Operator : DD/AJ
 Sample : VBF1226S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 VBF1226S1

Integration File: Calibration.e
 Quant Time: Dec 27 00:31:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	467931	19.732 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.682	5315	0.172 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	994	0.030 ng/ml
3) t n-Heptane	7.734	1322	0.040 ng/ml
6) t Toluene	10.631	5612	0.146 ng/ml
7) t Ethylbenzene	13.060	1636	0.045 ng/ml
8) t m-Xylene	13.197	4252	0.122 ng/ml
9) t O-Xylene	13.921	2159	0.064 ng/ml
10) t 1,2,4-Trimethylbenzene	16.212	4248	0.151 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122619\
Data File : FB023307.D
Signal(s) : FID2B.CH
Acq On : 26 Dec 2019 11:58
Operator : DD/AJ
Sample : VBF1226S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF1226S1

Integration File: Calibration.e
Quant Time: Dec 27 00:31:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

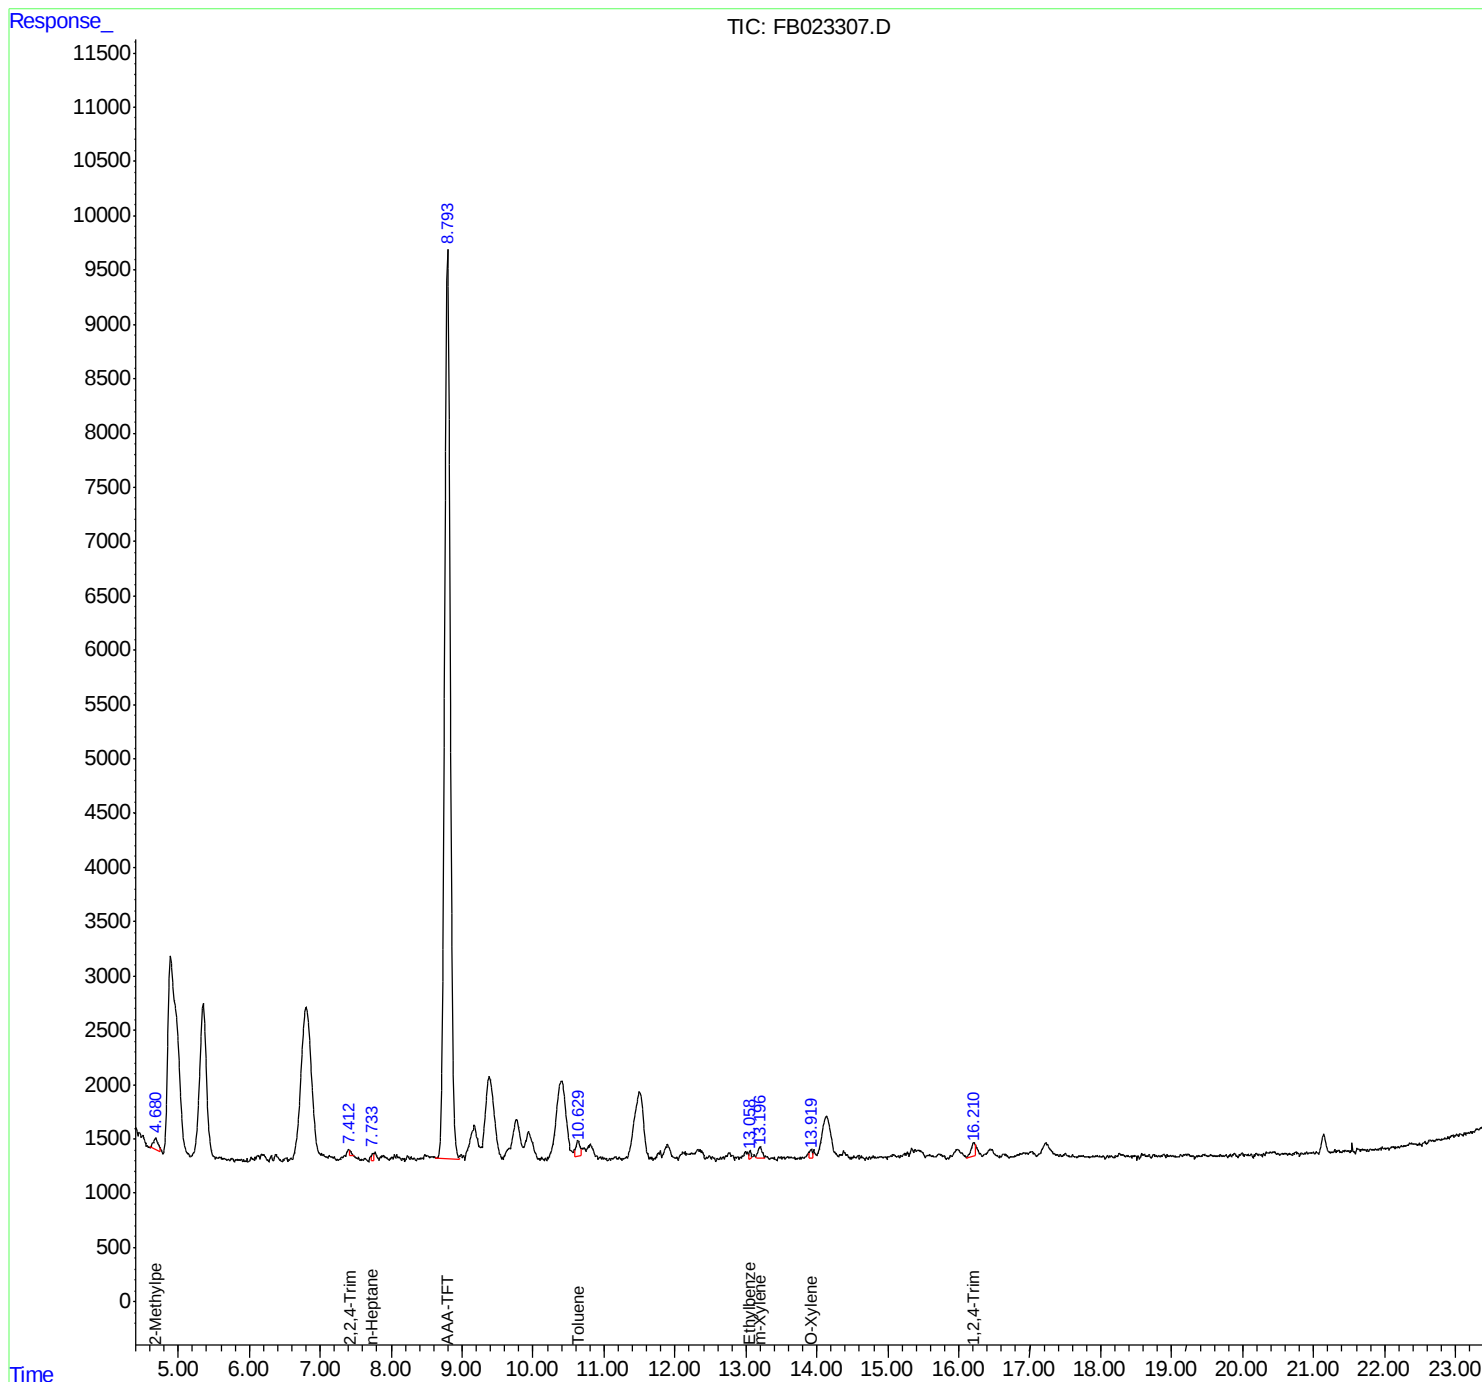


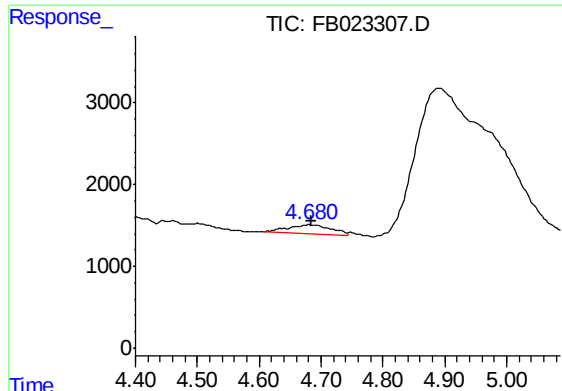

#1 2-Methylpentane


R.T.: 4.682 min
Delta R.T.: -0.002 min
Response: 5315
Conc: 0.17 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF1226S1

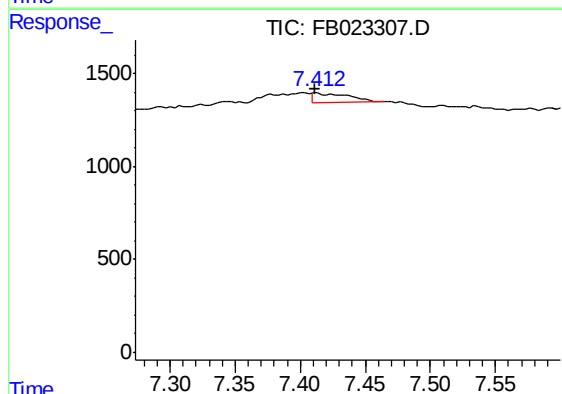


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: 0.002 min
Response: 994
Conc: 0.03 ng/ml

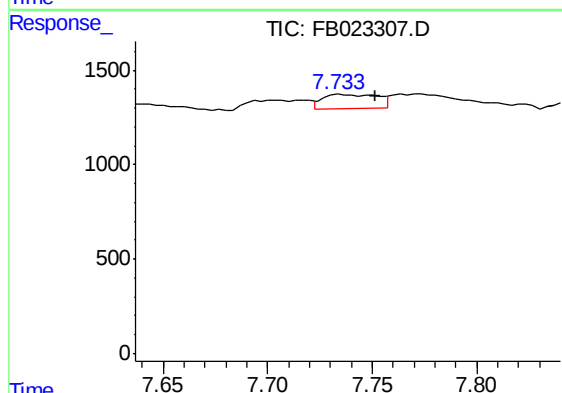


#3 n-Heptane

R.T.: 7.734 min
Delta R.T.: -0.017 min
Response: 1322
Conc: 0.04 ng/ml

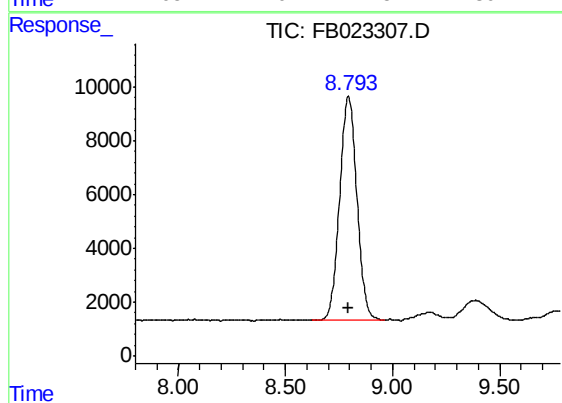

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.001 min
Response: 467931
Conc: 19.73 ng/ml

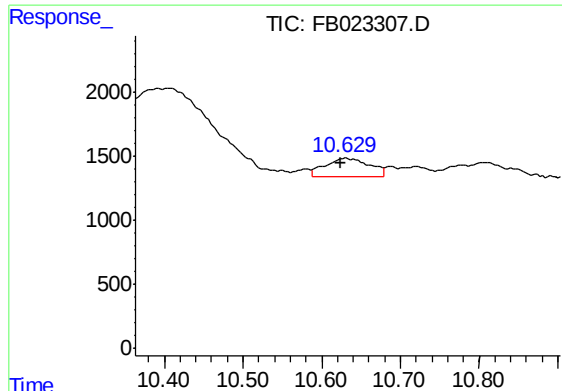

#6 Toluene


R.T.: 10.631 min
Delta R.T.: 0.007 min
Response: 5612
Conc: 0.15 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF1226S1

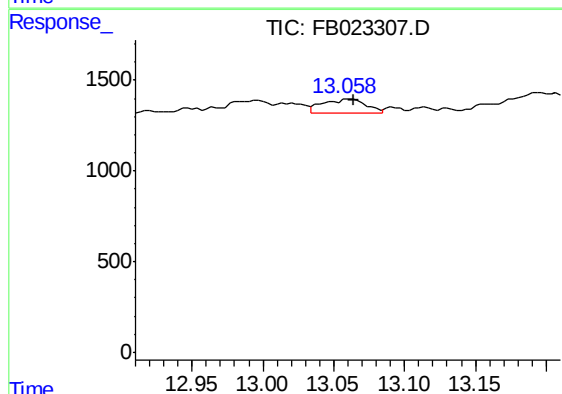


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: -0.004 min
Response: 1636
Conc: 0.05 ng/ml

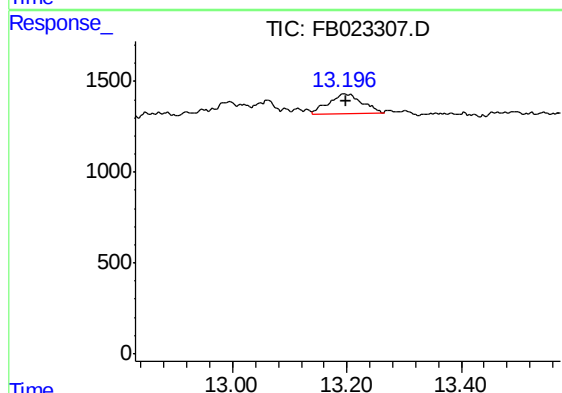


#8 m-Xylene

R.T.: 13.197 min
Delta R.T.: 0.000 min
Response: 4252
Conc: 0.12 ng/ml

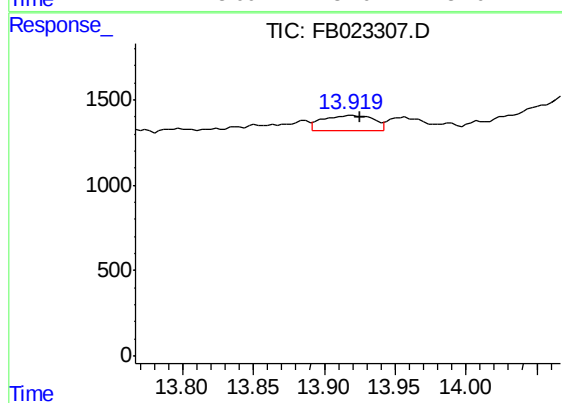

#9 O-Xylene

R.T.: 13.921 min
Delta R.T.: -0.004 min
Response: 2159
Conc: 0.06 ng/ml

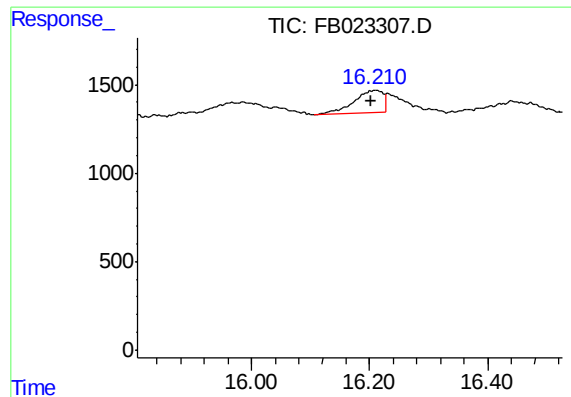

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min
Delta R.T.: 0.008 min
Response: 4248
Conc: 0.15 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF1226S1