

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122619\
 Data File : FB023308.D
 Signal(s) : FID2B.CH
 Acq On : 26 Dec 2019 12:28
 Operator : DD/AJ
 Sample : BSF1226S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1226S1

Integration File: Calibration.e
 Quant Time: Dec 27 00:31:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	481631	20.310 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.686	971511	31.390 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	1057079	31.644 ng/ml
3) t n-Heptane	7.752	346468	10.504 ng/ml
4) t Benzene	7.887	423379	10.602 ng/ml
6) t Toluene	10.625	1227722	31.886 ng/ml
7) t Ethylbenzene	13.065	390535	10.760 ng/ml
8) t m-Xylene	13.198	743685	21.424 ng/ml
9) t O-Xylene	13.926	714933	21.226 ng/ml
10) t 1,2,4-Trimethylbenzene	16.204	601914	21.452 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122619\
Data File : FB023308.D
Signal(s) : FID2B.CH
Acq On : 26 Dec 2019 12:28
Operator : DD/AJ
Sample : BSF1226S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1226S1

Integration File: Calibration.e
Quant Time: Dec 27 00:31:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

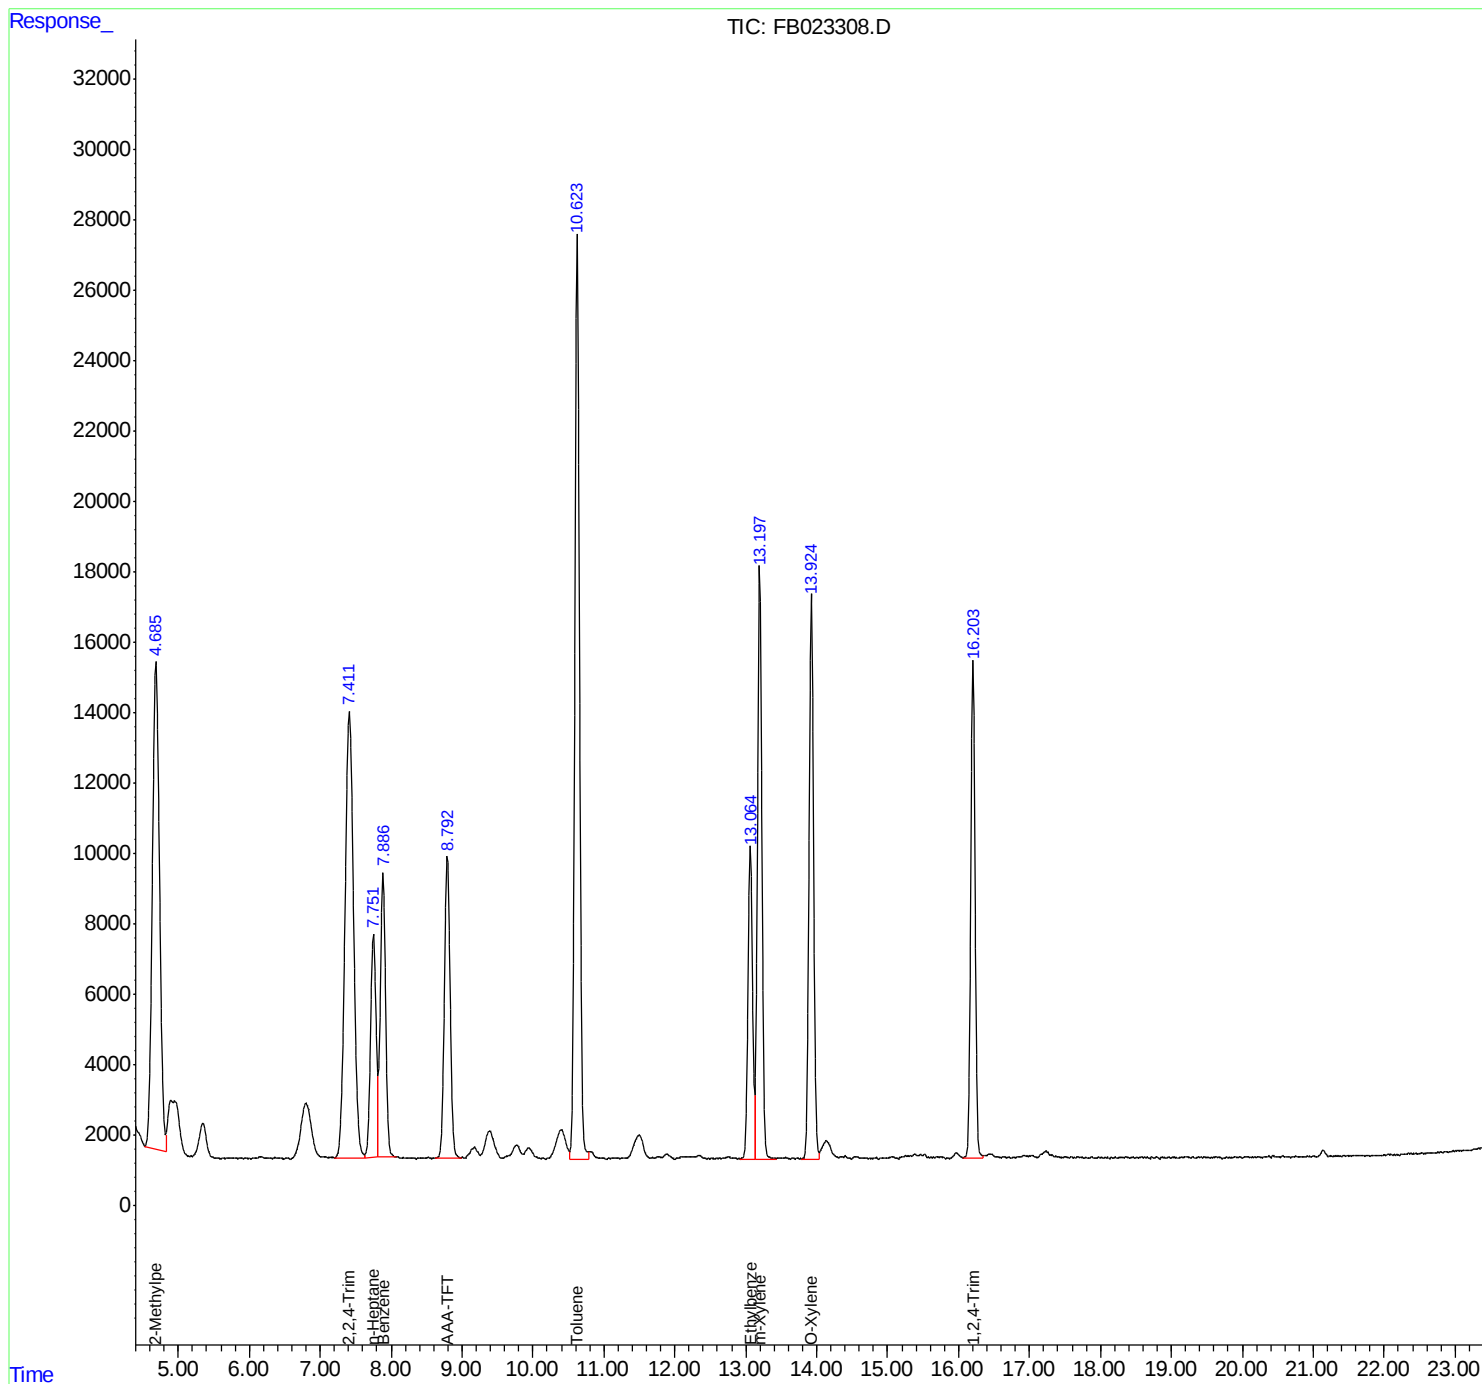


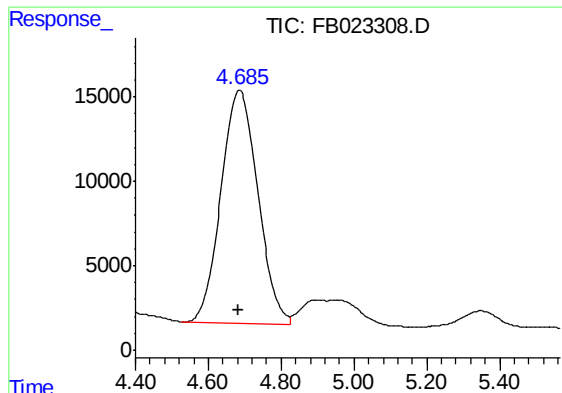

#1 2-Methylpentane


R.T.: 4.686 min
Delta R.T.: 0.002 min
Response: 971511
Conc: 31.39 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1226S1

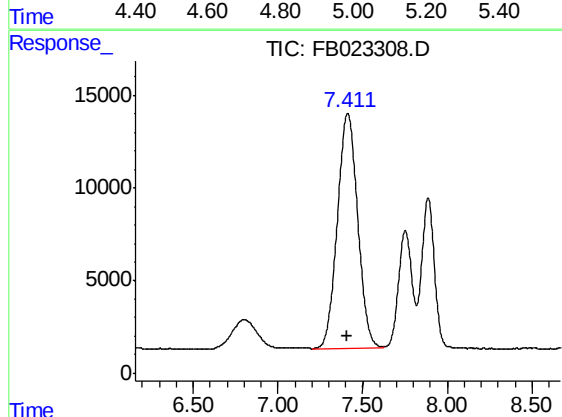


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: 0.000 min
Response: 1057079
Conc: 31.64 ng/ml

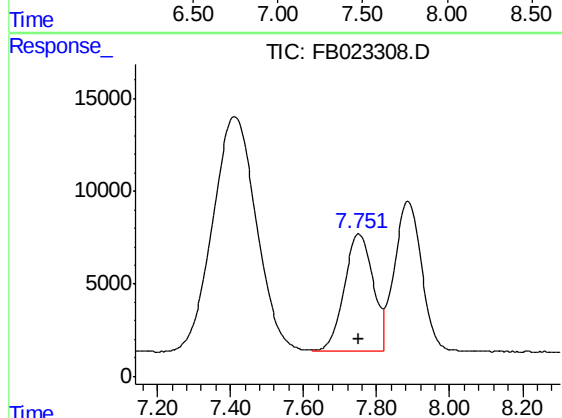


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 346468
Conc: 10.50 ng/ml

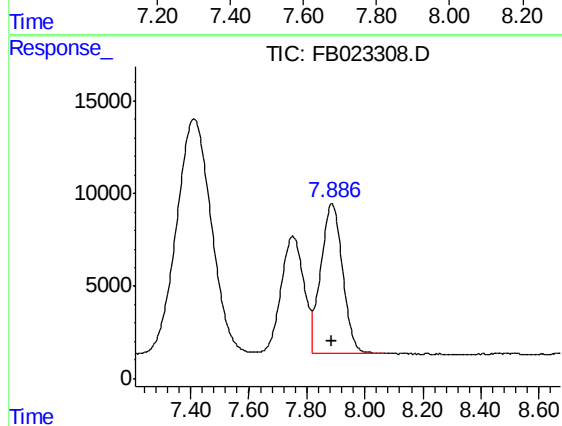

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.000 min
Response: 423379
Conc: 10.60 ng/ml

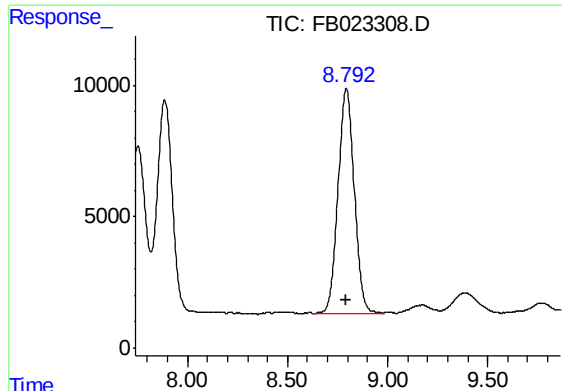

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.000 min
Response: 481631
Conc: 20.31 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1226S1

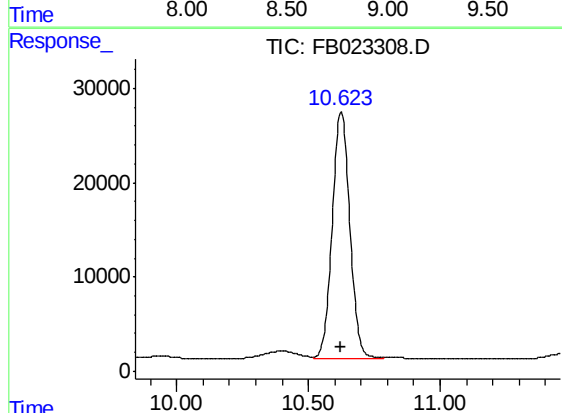


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.001 min
Response: 1227722
Conc: 31.89 ng/ml

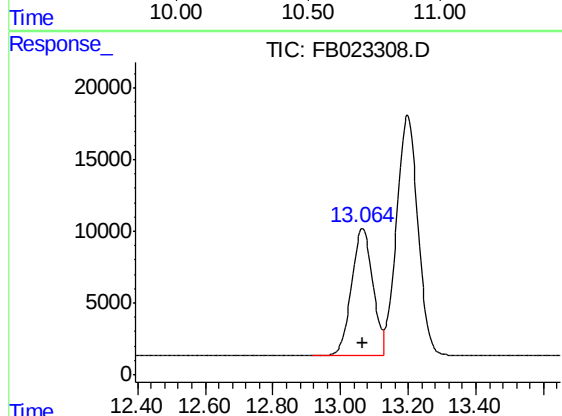


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: 0.001 min
Response: 390535
Conc: 10.76 ng/ml

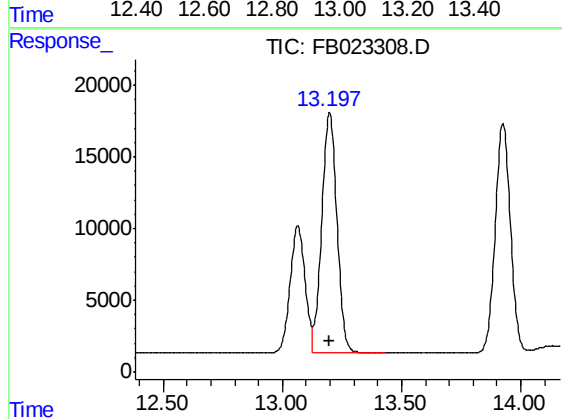

#8 m-Xylene


R.T.: 13.198 min
Delta R.T.: 0.000 min
Response: 743685
Conc: 21.42 ng/ml

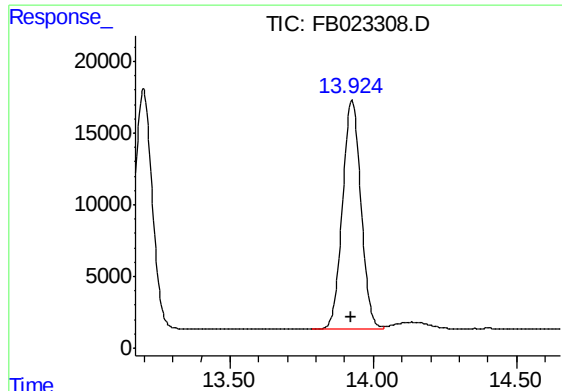

#9 O-Xylene

R.T.: 13.926 min
Delta R.T.: 0.001 min
Response: 714933
Conc: 21.23 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1226S1

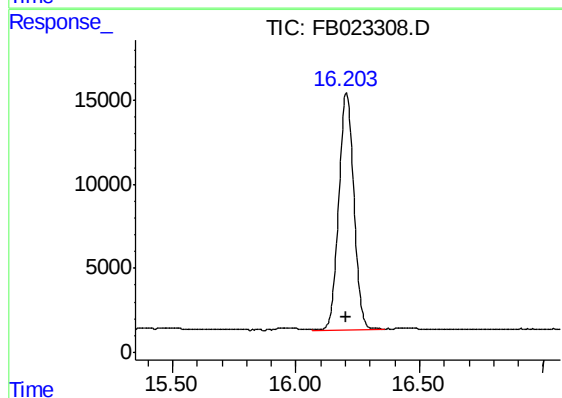

#10 1,2,4-Trimethylbenzene

R.T.: 16.204 min
Delta R.T.: 0.001 min
Response: 601914
Conc: 21.45 ng/ml