

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122619\
 Data File : FB023309.D
 Signal(s) : FID2B.CH
 Acq On : 26 Dec 2019 13:32
 Operator : DD/AJ
 Sample : K6118-11
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SU-01-122319

Integration File: Calibration.e
 Quant Time: Dec 27 00:31:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	443977	18.722 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	2580	0.083 ng/ml
2) t 2,2,4-Trimethylpentane	7.372	7706	0.231 ng/ml
6) t Toluene	10.624	12825	0.333 ng/ml
7) t Ethylbenzene	13.049	55937	1.541 ng/ml
8) t m-Xylene	13.192	32096	0.925 ng/ml
9) t o-Xylene	13.927	31610	0.938 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	40918	1.458 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122619\
Data File : FB023309.D
Signal(s) : FID2B.CH
Acq On : 26 Dec 2019 13:32
Operator : DD/AJ
Sample : K6118-11
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SU-01-122319

Integration File: Calibration.e
Quant Time: Dec 27 00:31:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

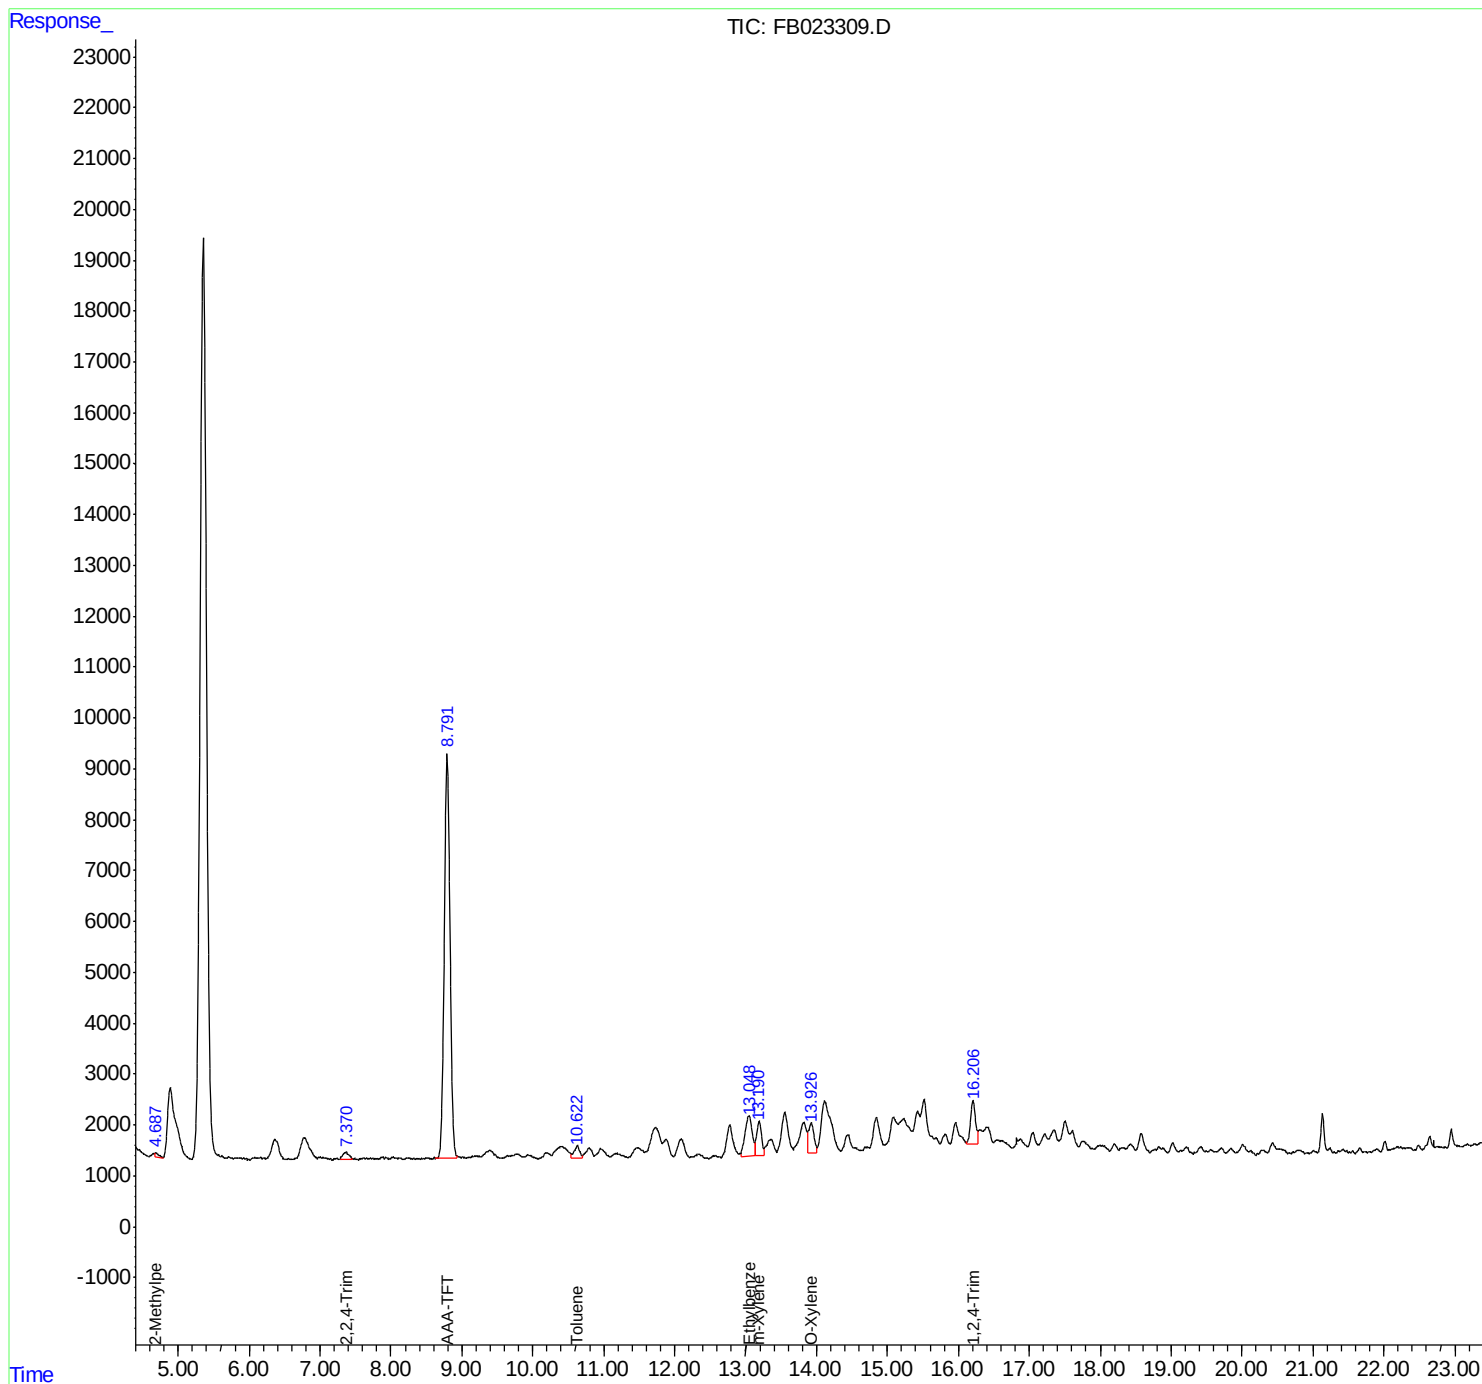


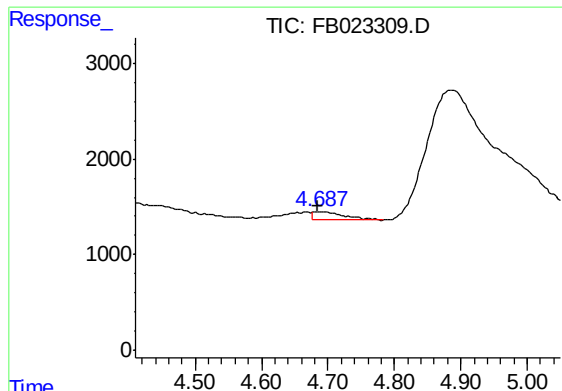

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.005 min
Response: 2580
Conc: 0.08 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-01-122319

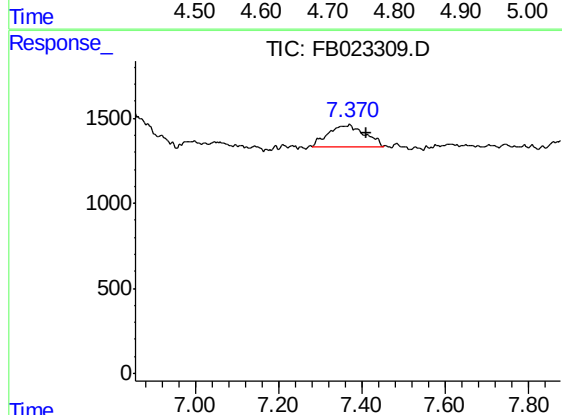


#2 2,2,4-Trimethylpentane

R.T.: 7.372 min
Delta R.T.: -0.039 min
Response: 7706
Conc: 0.23 ng/ml

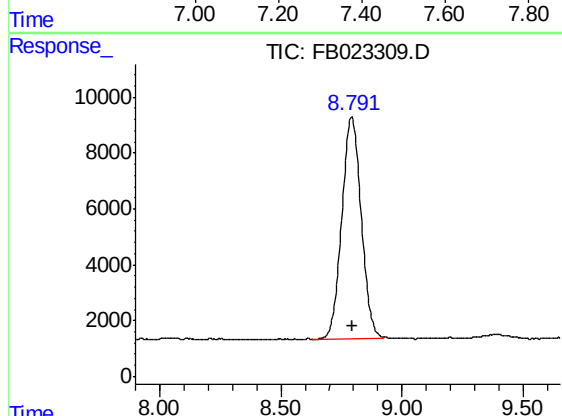


#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: -0.001 min
Response: 443977
Conc: 18.72 ng/ml

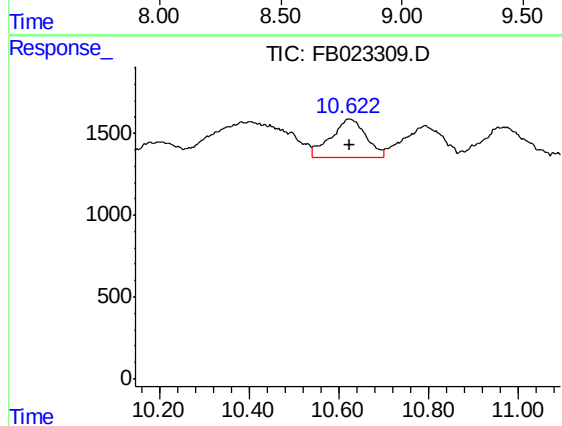

#6 Toluene


R.T.: 10.624 min
Delta R.T.: 0.000 min
Response: 12825
Conc: 0.33 ng/ml

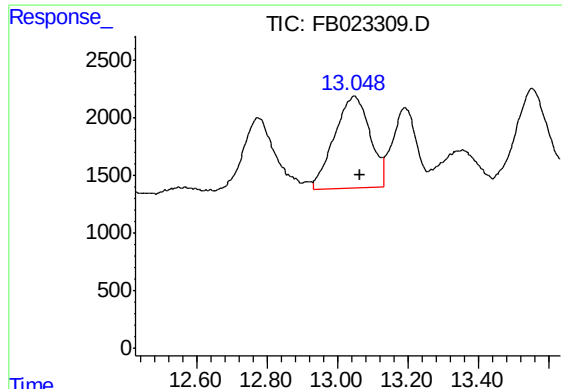

#7 Ethylbenzene


R.T.: 13.049 min
Delta R.T.: -0.015 min
Response: 55937
Conc: 1.54 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-01-122319

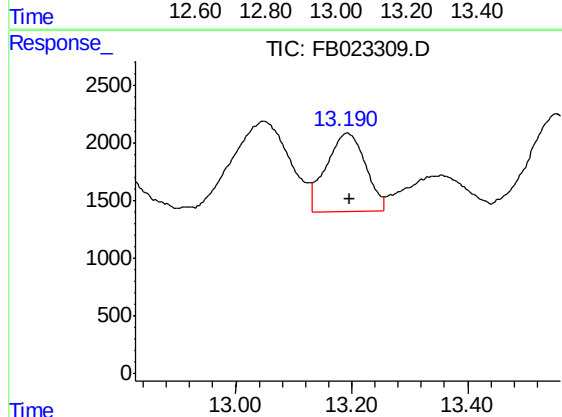


#8 m-Xylene

R.T.: 13.192 min
Delta R.T.: -0.005 min
Response: 32096
Conc: 0.92 ng/ml

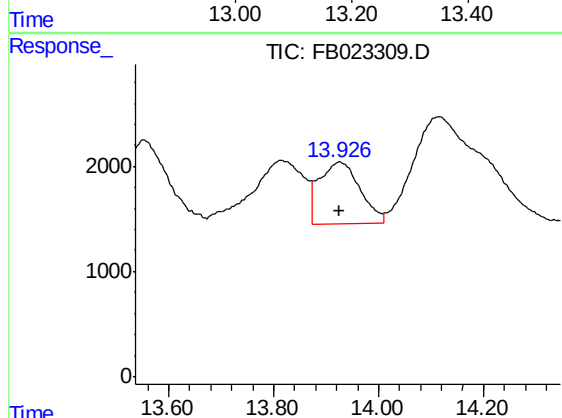

#9 o-Xylene

R.T.: 13.927 min
Delta R.T.: 0.002 min
Response: 31610
Conc: 0.94 ng/ml

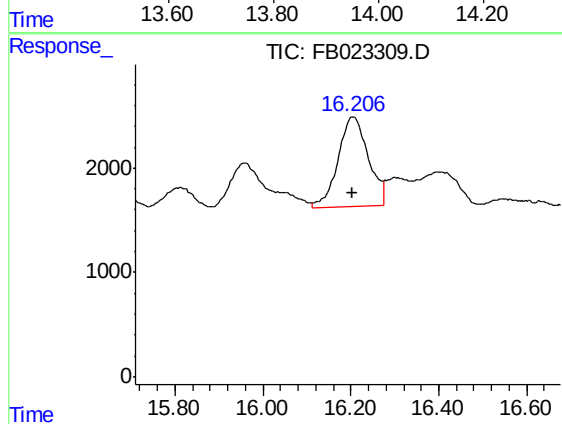

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: 0.003 min
Response: 40918
Conc: 1.46 ng/ml