

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122619\
Data File : FB023312.D
Signal(s) : FID2B.CH
Acq On : 26 Dec 2019 15:20
Operator : DD/AJ
Sample : K6117-11
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TR-05-122619

Integration File: Calibration.e
Quant Time: Dec 27 00:31:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	462119	19.487 ng/ml
Target Compounds			
6) t Toluene	10.623	4440	0.115 ng/ml
7) t Ethylbenzene	13.055	9405	0.259 ng/ml
8) t m-Xylene	13.197	18786	0.541 ng/ml
9) t O-Xylene	13.932	18067	0.536 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	61987	2.209 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122619\
Data File : FB023312.D
Signal(s) : FID2B.CH
Acq On : 26 Dec 2019 15:20
Operator : DD/AJ
Sample : K6117-11
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TR-05-122619

Integration File: Calibration.e
Quant Time: Dec 27 00:31:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

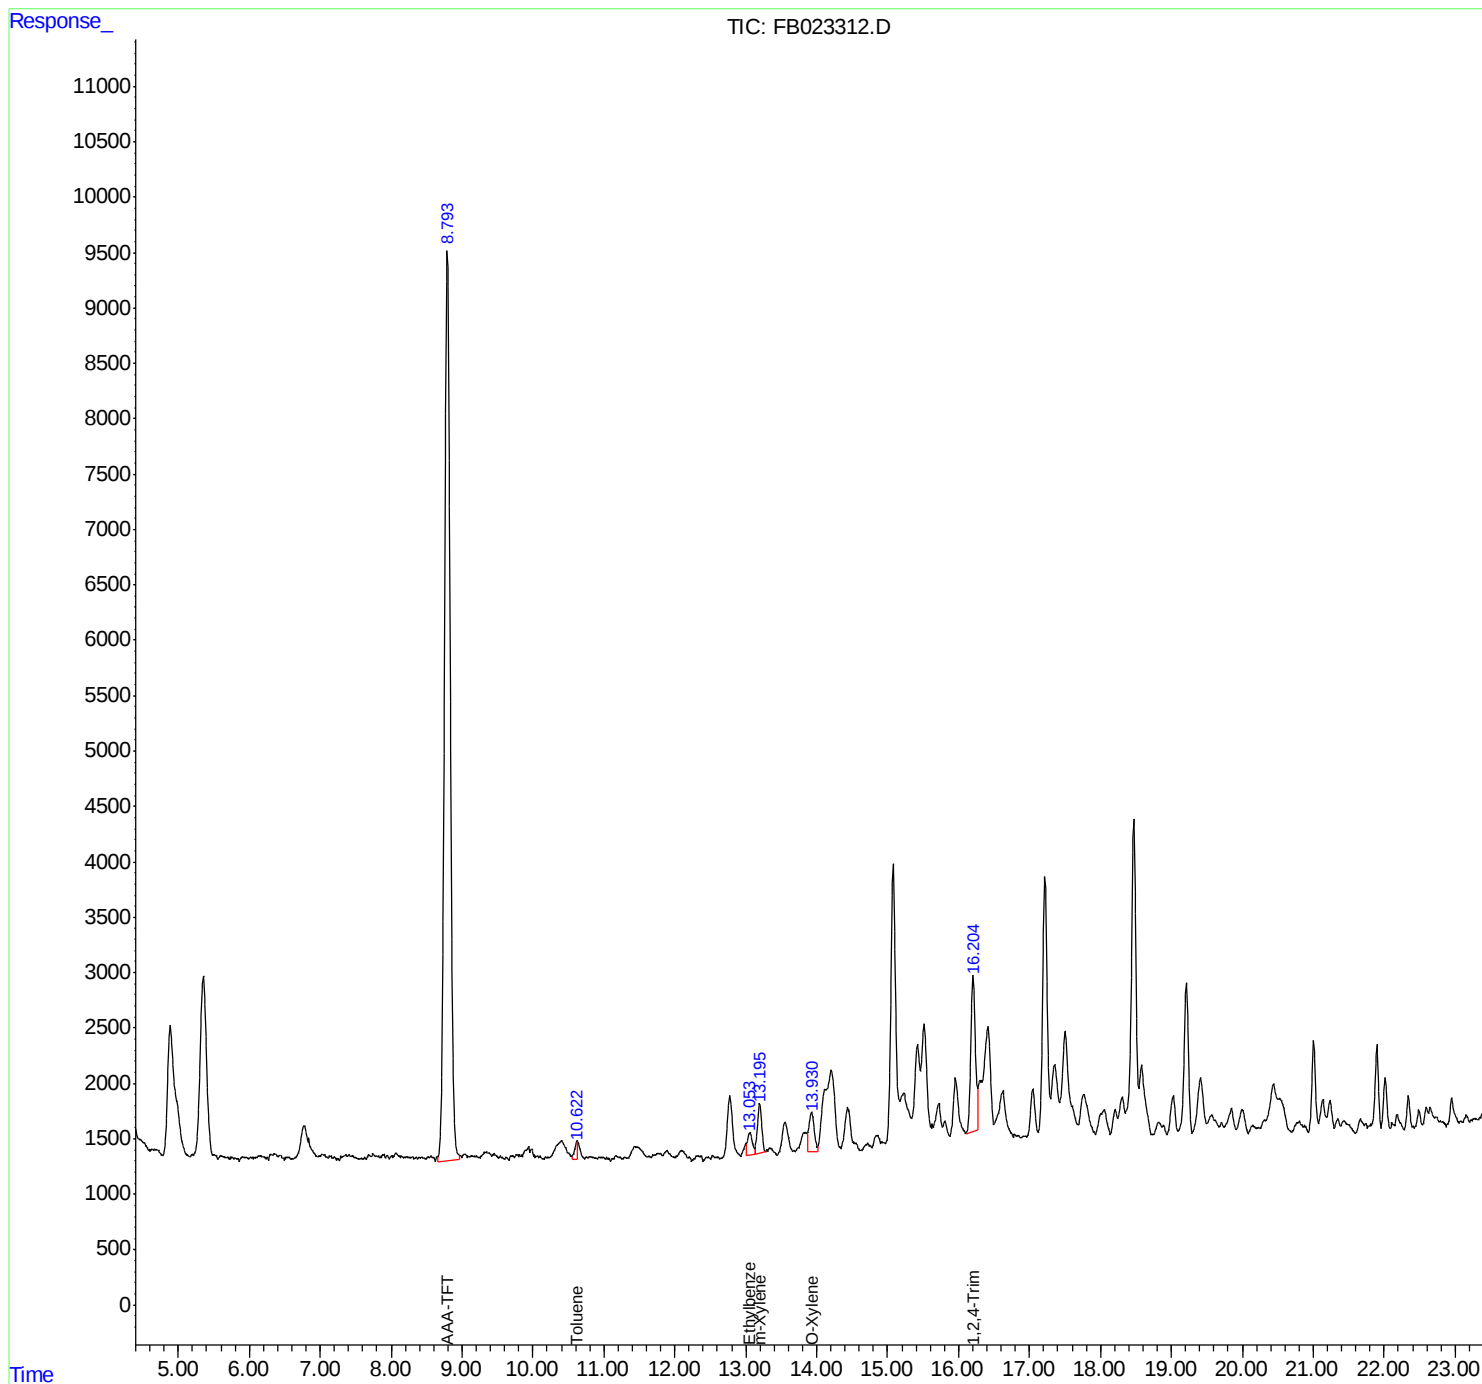


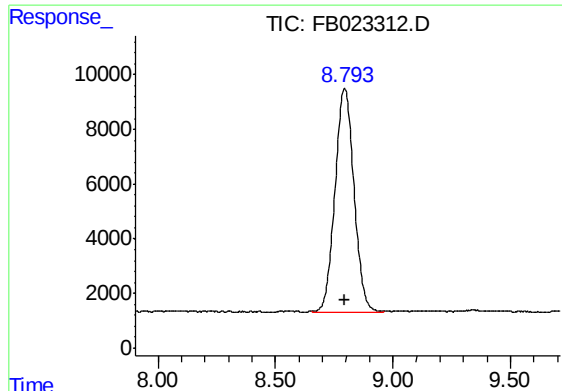

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.001 min
Response: 462119
Conc: 19.49 ng/ml

Instrument :
FID_B
ClientSampleId :
TR-05-122619

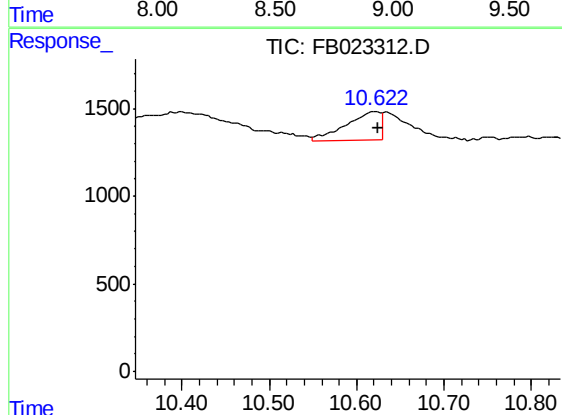


#6 Toluene

R.T.: 10.623 min
Delta R.T.: -0.001 min
Response: 4440
Conc: 0.12 ng/ml

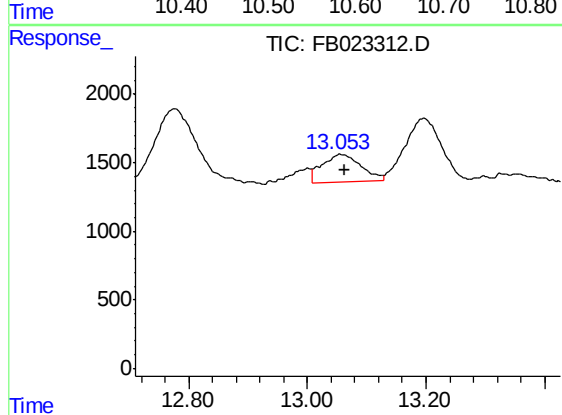


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.009 min
Response: 9405
Conc: 0.26 ng/ml

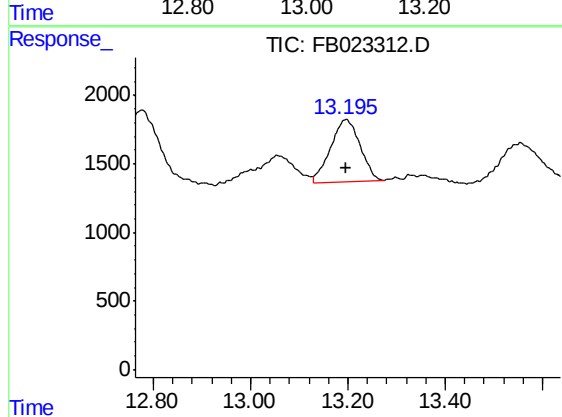

#8 m-Xylene


R.T.: 13.197 min
Delta R.T.: 0.000 min
Response: 18786
Conc: 0.54 ng/ml

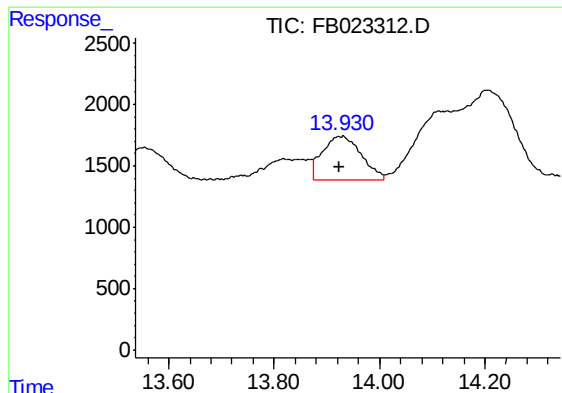

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.007 min
Response: 18067
Conc: 0.54 ng/ml

Instrument :
FID_B
ClientSampleId :
TR-05-122619

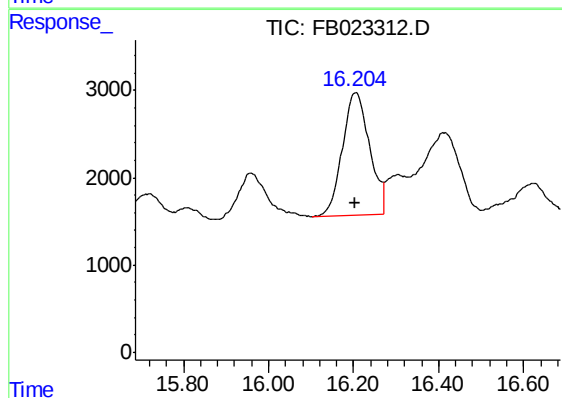

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: 0.002 min
Response: 61987
Conc: 2.21 ng/ml