

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122619\
 Data File : FB023310.D
 Signal(s) : FID2B.CH
 Acq On : 26 Dec 2019 14:02
 Operator : DD/AJ
 Sample : K6118-11MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SU-01-122319MS

Integration File: Calibration.e
 Quant Time: Dec 27 09:06:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	339800	14.329 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.685	774366	25.020 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	796101	23.831 ng/ml
3) t n-Heptane	7.754	254810	7.725 ng/ml
4) t Benzene	7.888	380574	9.530 ng/ml
6) t Toluene	10.626	1067315	27.720 ng/ml
7) t Ethylbenzene	13.066	330057	9.093 ng/ml
8) t m-Xylene	13.199	615487	17.731 ng/ml
9) t O-Xylene	13.927	601691	17.864 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	496152	17.683 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122619\
Data File : FB023310.D
Signal(s) : FID2B.CH
Acq On : 26 Dec 2019 14:02
Operator : DD/AJ
Sample : K6118-11MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SU-01-122319MS

Integration File: Calibration.e
Quant Time: Dec 27 09:06:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

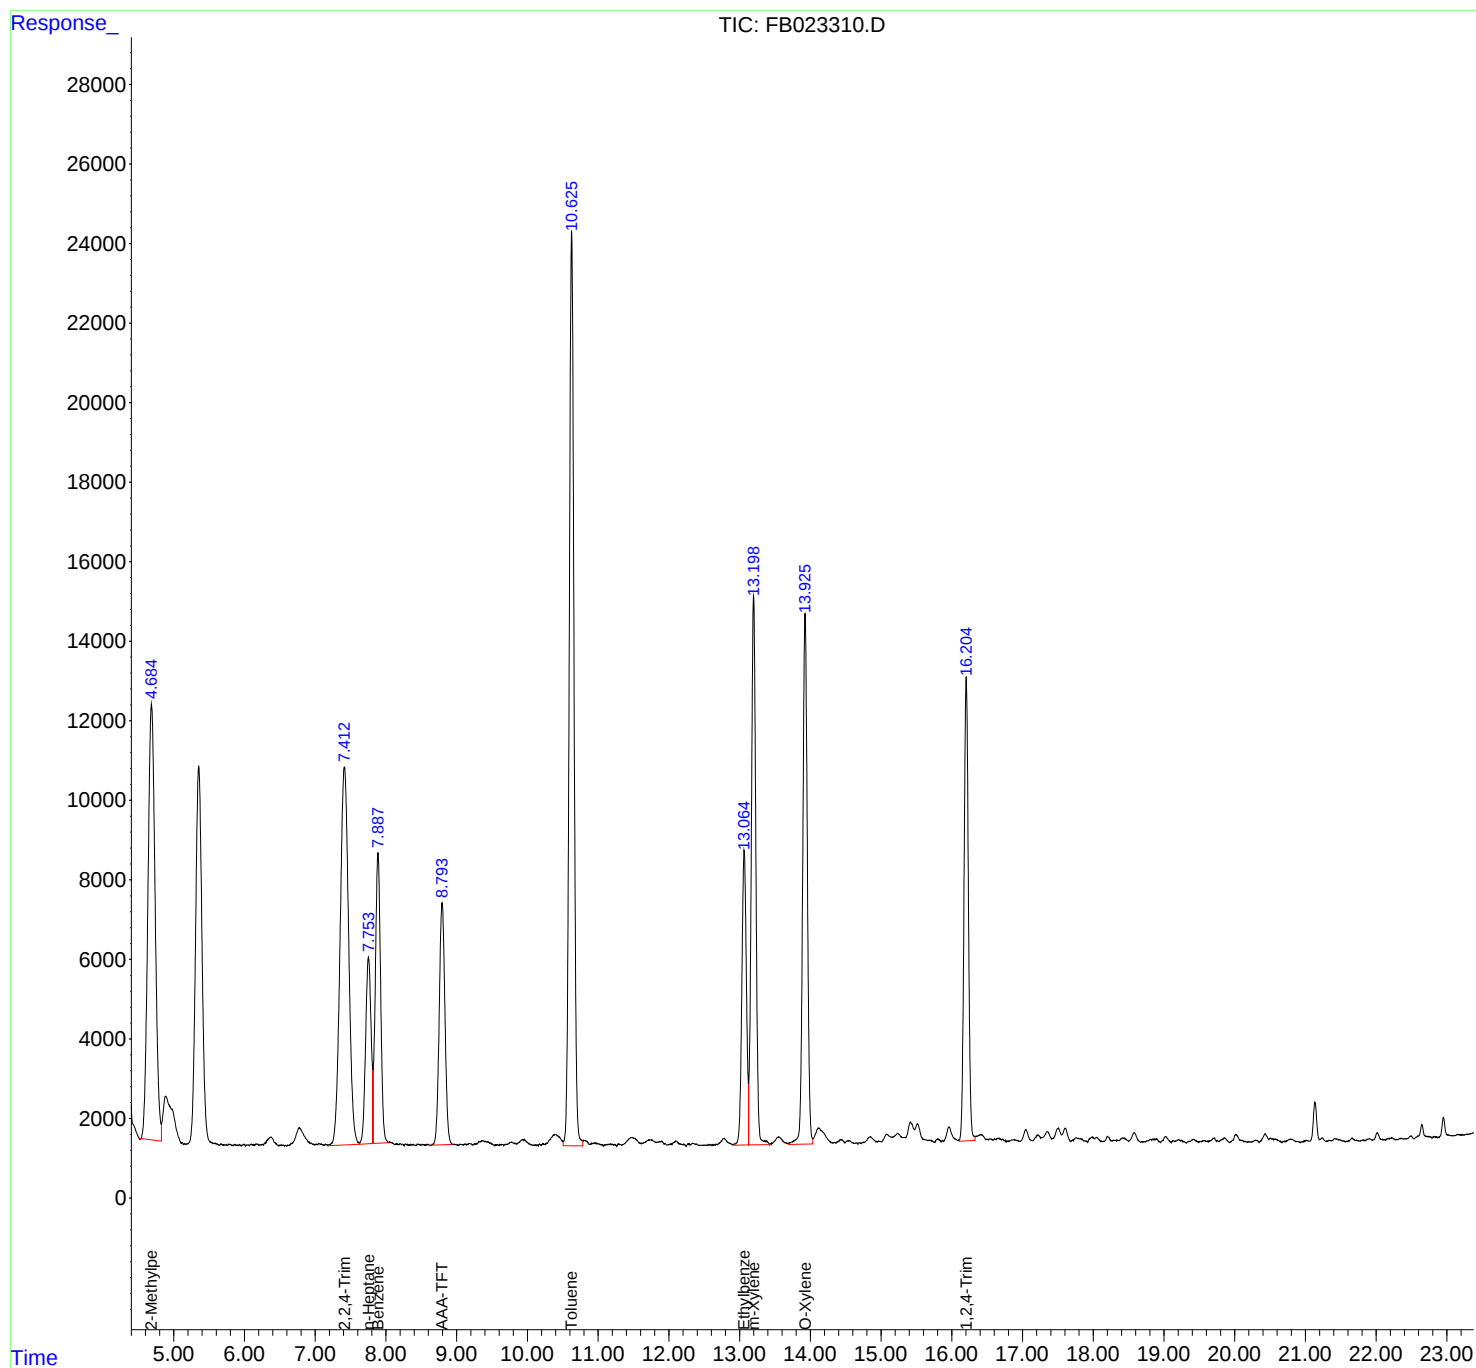


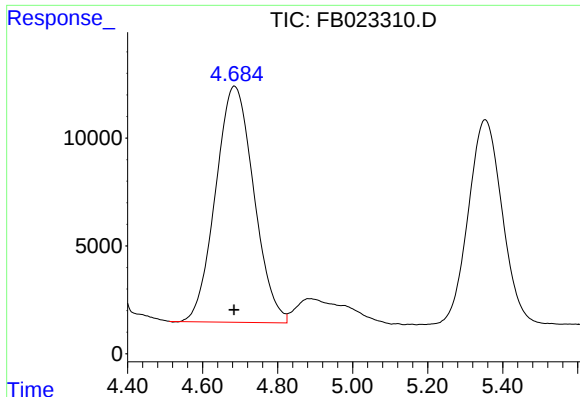

#1 2-Methylpentane


R.T.: 4.685 min
Delta R.T.: 0.001 min
Response: 774366
Conc: 25.02 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-01-122319MS

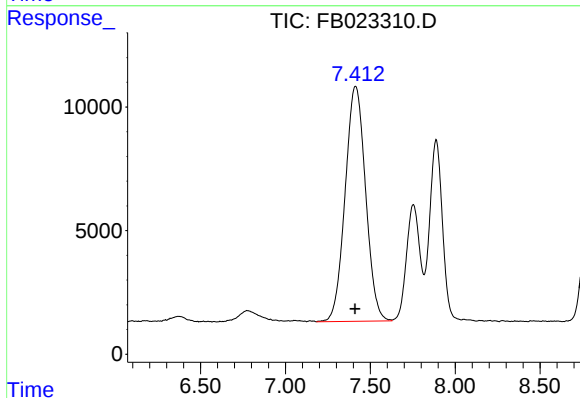


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: 0.002 min
Response: 796101
Conc: 23.83 ng/ml

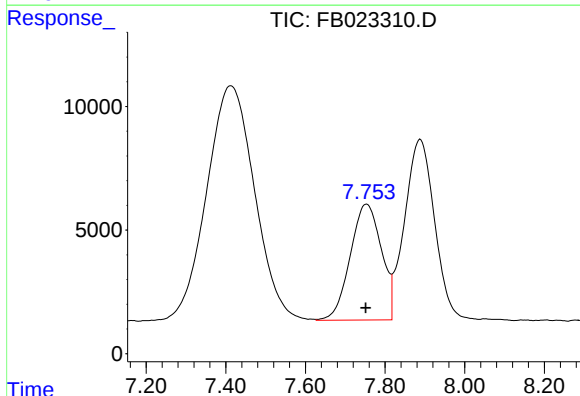


#3 n-Heptane

R.T.: 7.754 min
Delta R.T.: 0.002 min
Response: 254810
Conc: 7.72 ng/ml

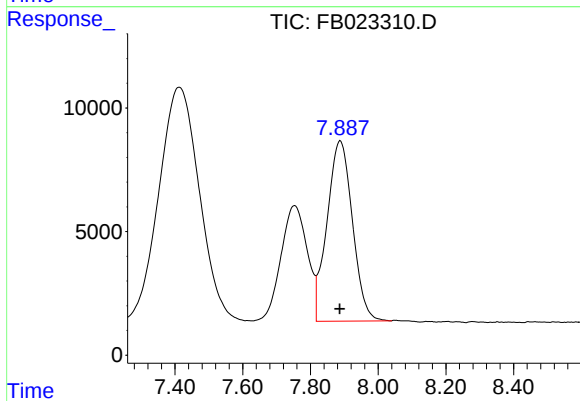


#4 Benzene

R.T.: 7.888 min
Delta R.T.: 0.002 min
Response: 380574
Conc: 9.53 ng/ml

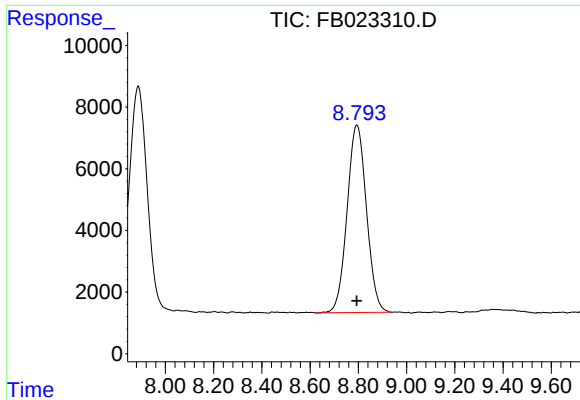


#5 AAA-TFT
 R.T.: 8.794 min
 Delta R.T.: 0.001 min
 Response: 339800
 Conc: 14.33 ng/ml


Instrument :
 FID_B
 ClientSampleId :
 SU-01-122319MS

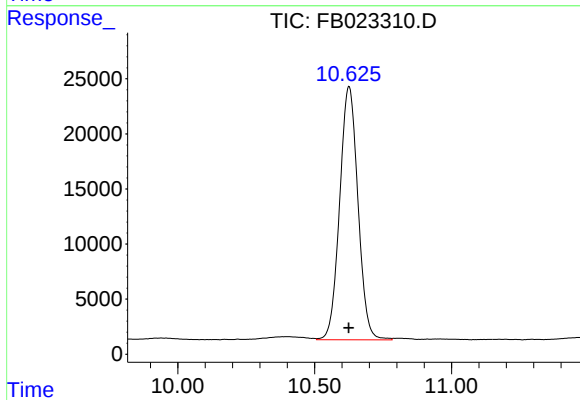


#6 Toluene
 R.T.: 10.626 min
 Delta R.T.: 0.002 min
 Response: 1067315
 Conc: 27.72 ng/ml

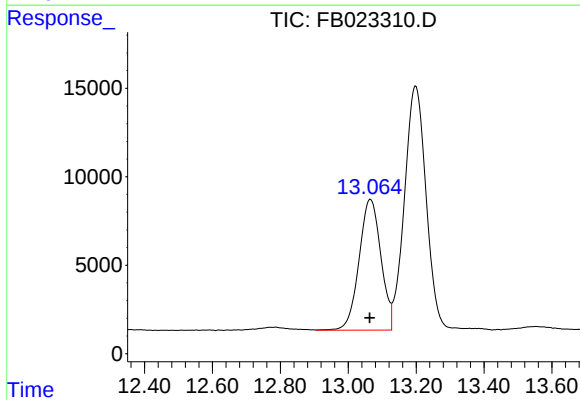

#7 Ethylbenzene
 R.T.: 13.066 min
 Delta R.T.: 0.002 min
 Response: 330057
 Conc: 9.09 ng/ml

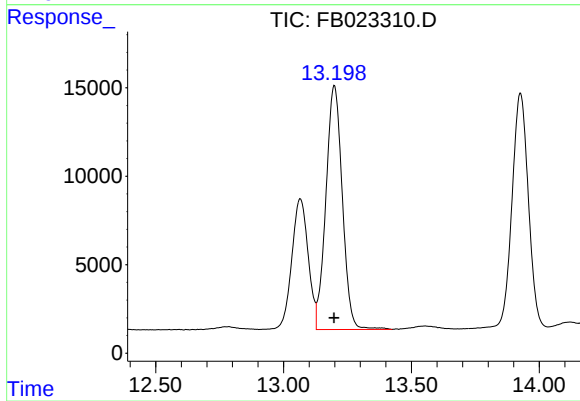


#8 m-Xylene
 R.T.: 13.199 min
 Delta R.T.: 0.002 min
 Response: 615487
 Conc: 17.73 ng/ml

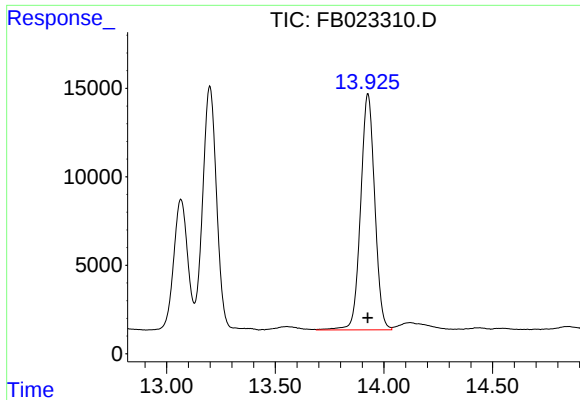

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: 0.002 min
Response: 601691
Conc: 17.86 ng/ml

Instrument :
FID_B
ClientSampleId :
SU-01-122319MS

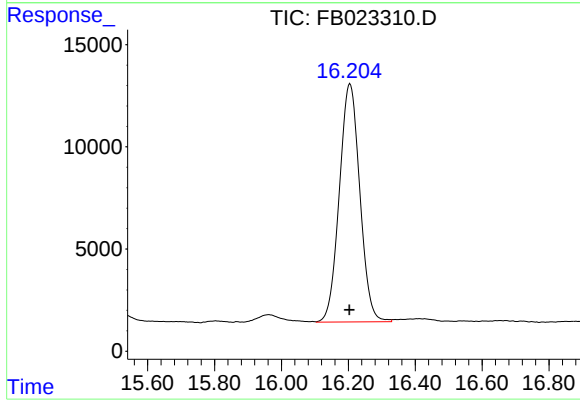

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: 0.002 min
Response: 496152
Conc: 17.68 ng/ml