

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB122718\
 Data File : FB019214.D
 Signal(s) : FID2B.CH
 Acq On : 27 Dec 2018 9:43
 Operator : MJ/SJ
 Sample : VBF1227S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: SAMPLE.e
 Quant Time: Dec 27 15:46:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
 Quant Title :
 QLast Update : Fri Dec 07 17:57:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.101	180690	20.672 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.972	1378	0.090 ng/ml
2) t 2,2,4-Trimethylpentane	7.731	7185	0.466 ng/ml
3) t n-Heptane	8.057	5523	0.372 ng/ml
4) t Benzene	8.194	3324	0.185 ng/ml
6) t Toluene	10.980	8374	0.552 ng/ml
7) t Ethylbenzene	13.365	9014	0.580 ng/ml
8) t m-Xylene	13.506	2049	0.126 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_B\Data\FB122718\
Data File : FB019214.D
Signal(s) : FID2B.CH
Acq On : 27 Dec 2018 9:43
Operator : MJ/SJ
Sample : VBF1227S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: SAMPLE.e
Quant Time: Dec 27 15:46:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
Quant Title :
QLast Update : Fri Dec 07 17:57:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

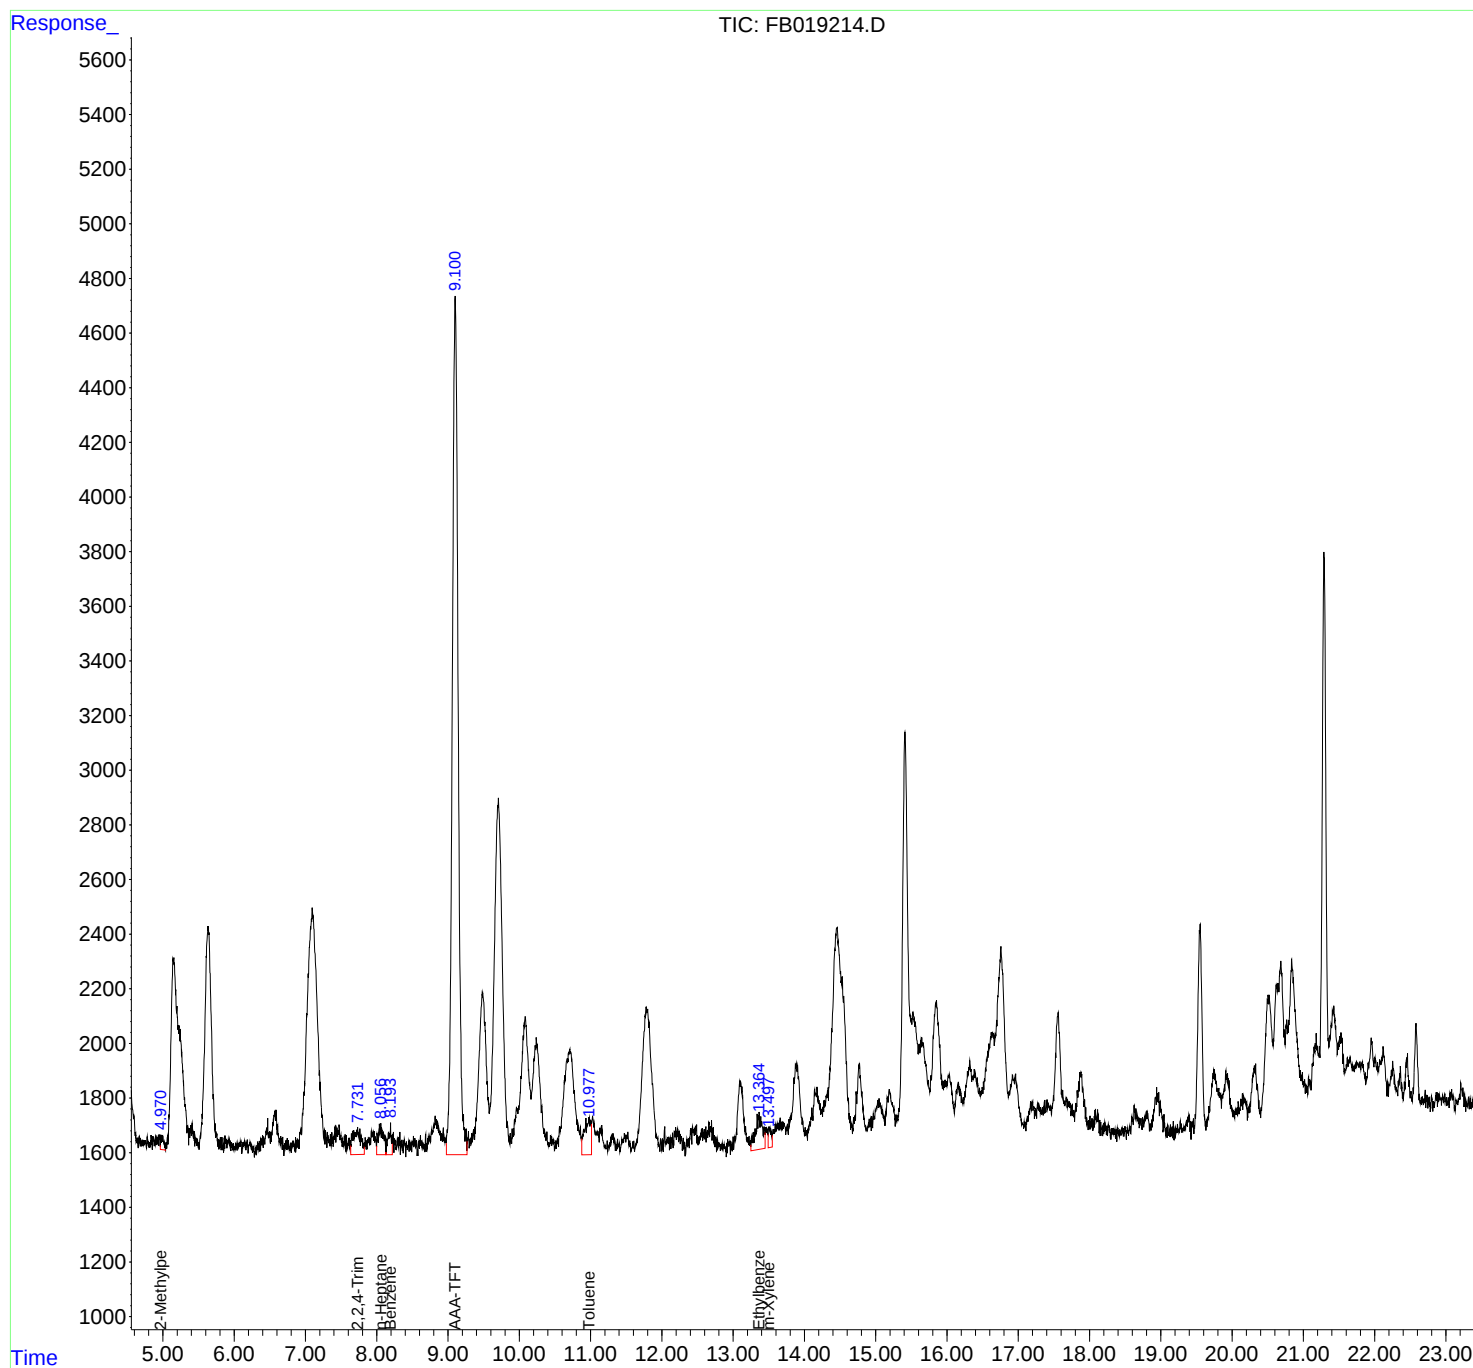


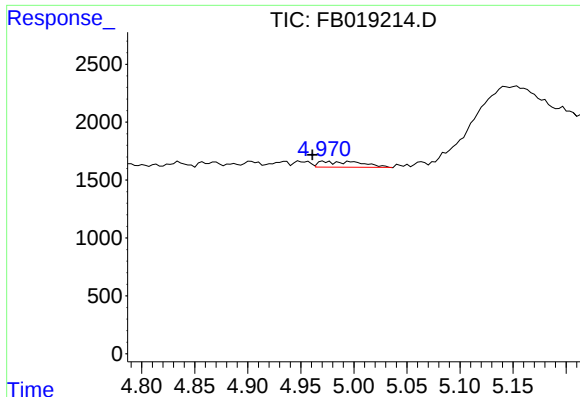

#1 2-Methylpentane


R.T.: 4.972 min
Delta R.T.: 0.011 min
Response: 1378
Conc: 0.09 ng/ml

Instrument :
FID_B
ClientSampleId :

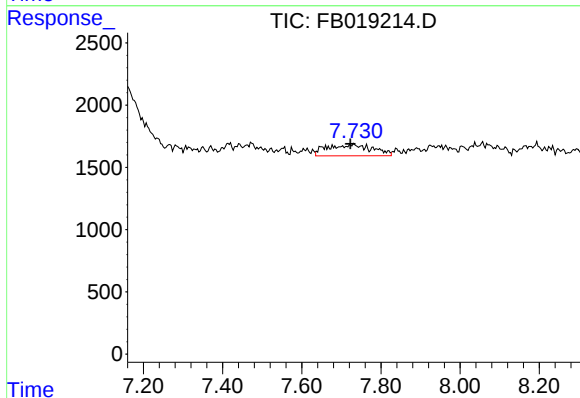


#2 2,2,4-Trimethylpentane

R.T.: 7.731 min
Delta R.T.: 0.008 min
Response: 7185
Conc: 0.47 ng/ml

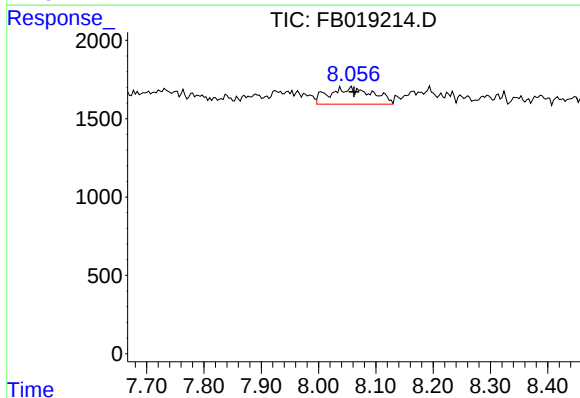


#3 n-Heptane

R.T.: 8.057 min
Delta R.T.: -0.005 min
Response: 5523
Conc: 0.37 ng/ml

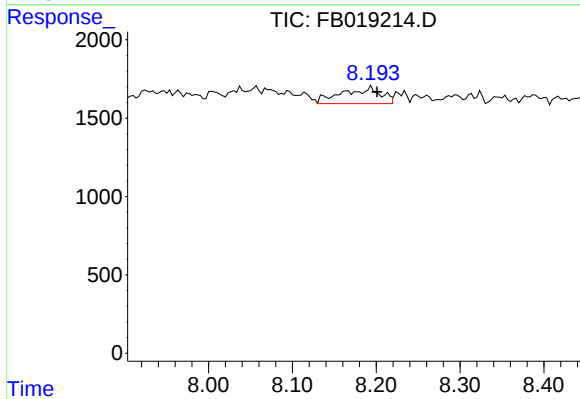

#4 Benzene


R.T.: 8.194 min
Delta R.T.: -0.007 min
Response: 3324
Conc: 0.18 ng/ml

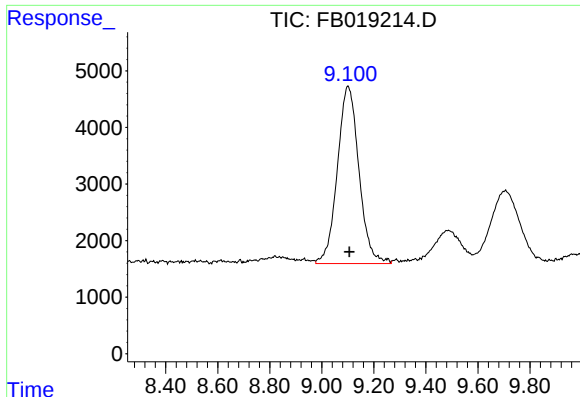

#5 AAA-TFT


R.T.: 9.101 min
Delta R.T.: -0.005 min
Response: 180690
Conc: 20.67 ng/ml

Instrument :
FID_B
ClientSampleId :

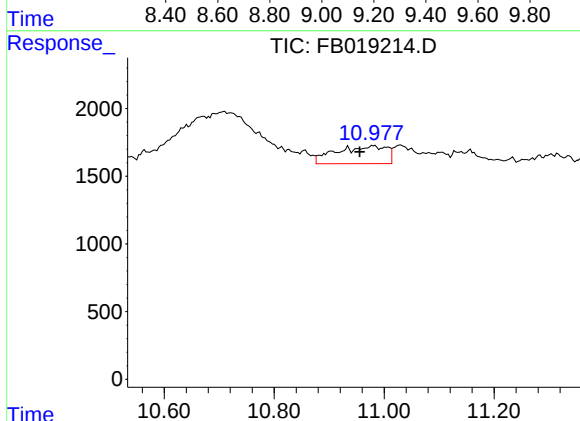


#6 Toluene

R.T.: 10.980 min
Delta R.T.: 0.025 min
Response: 8374
Conc: 0.55 ng/ml

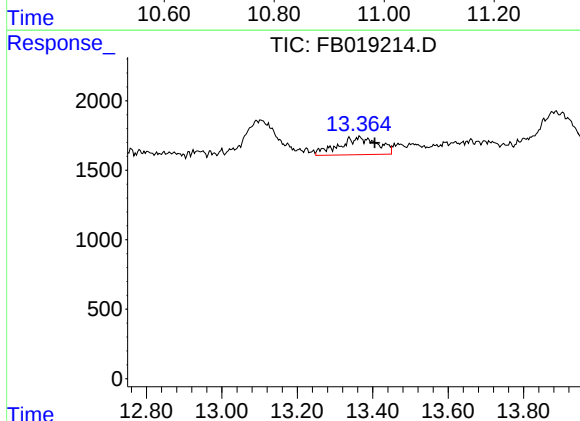

#7 Ethylbenzene

R.T.: 13.365 min
Delta R.T.: -0.040 min
Response: 9014
Conc: 0.58 ng/ml

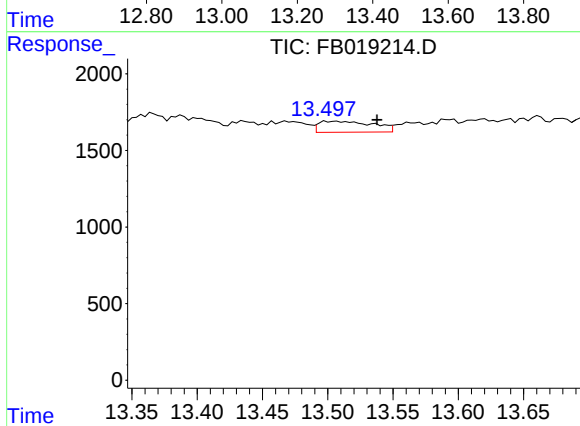

#8 m-Xylene

R.T.: 13.506 min
Delta R.T.: -0.032 min
Response: 2049
Conc: 0.13 ng/ml