

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122718\
 Data File : FB019215.D
 Signal(s) : FID2B.CH
 Acq On : 27 Dec 2018 10:12
 Operator : MJ/SJ
 Sample : BSF1227S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 27 15:46:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
 Quant Title :
 QLast Update : Fri Dec 07 17:57:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.102	184644	21.125 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.956	470826	30.798 ng/ml
2) t 2,2,4-Trimethylpentane	7.718	518694	33.669 ng/ml
3) t n-Heptane	8.058	167637	11.279 ng/ml
4) t Benzene	8.198	204878	11.374 ng/ml
6) t Toluene	10.951	502256	33.089 ng/ml
7) t Ethylbenzene	13.401	163100	10.498 ng/ml
8) t m-Xylene	13.534	344454	21.143 ng/ml
9) t O-Xylene	14.265	369036	21.826 ng/ml
10) t 1,2,4-Trimethylbenzene	16.548	413281	20.421 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122718\
Data File : FB019215.D
Signal(s) : FID2B.CH
Acq On : 27 Dec 2018 10:12
Operator : MJ/SJ
Sample : BSF1227S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 27 15:46:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120718.M
Quant Title :
QLast Update : Fri Dec 07 17:57:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

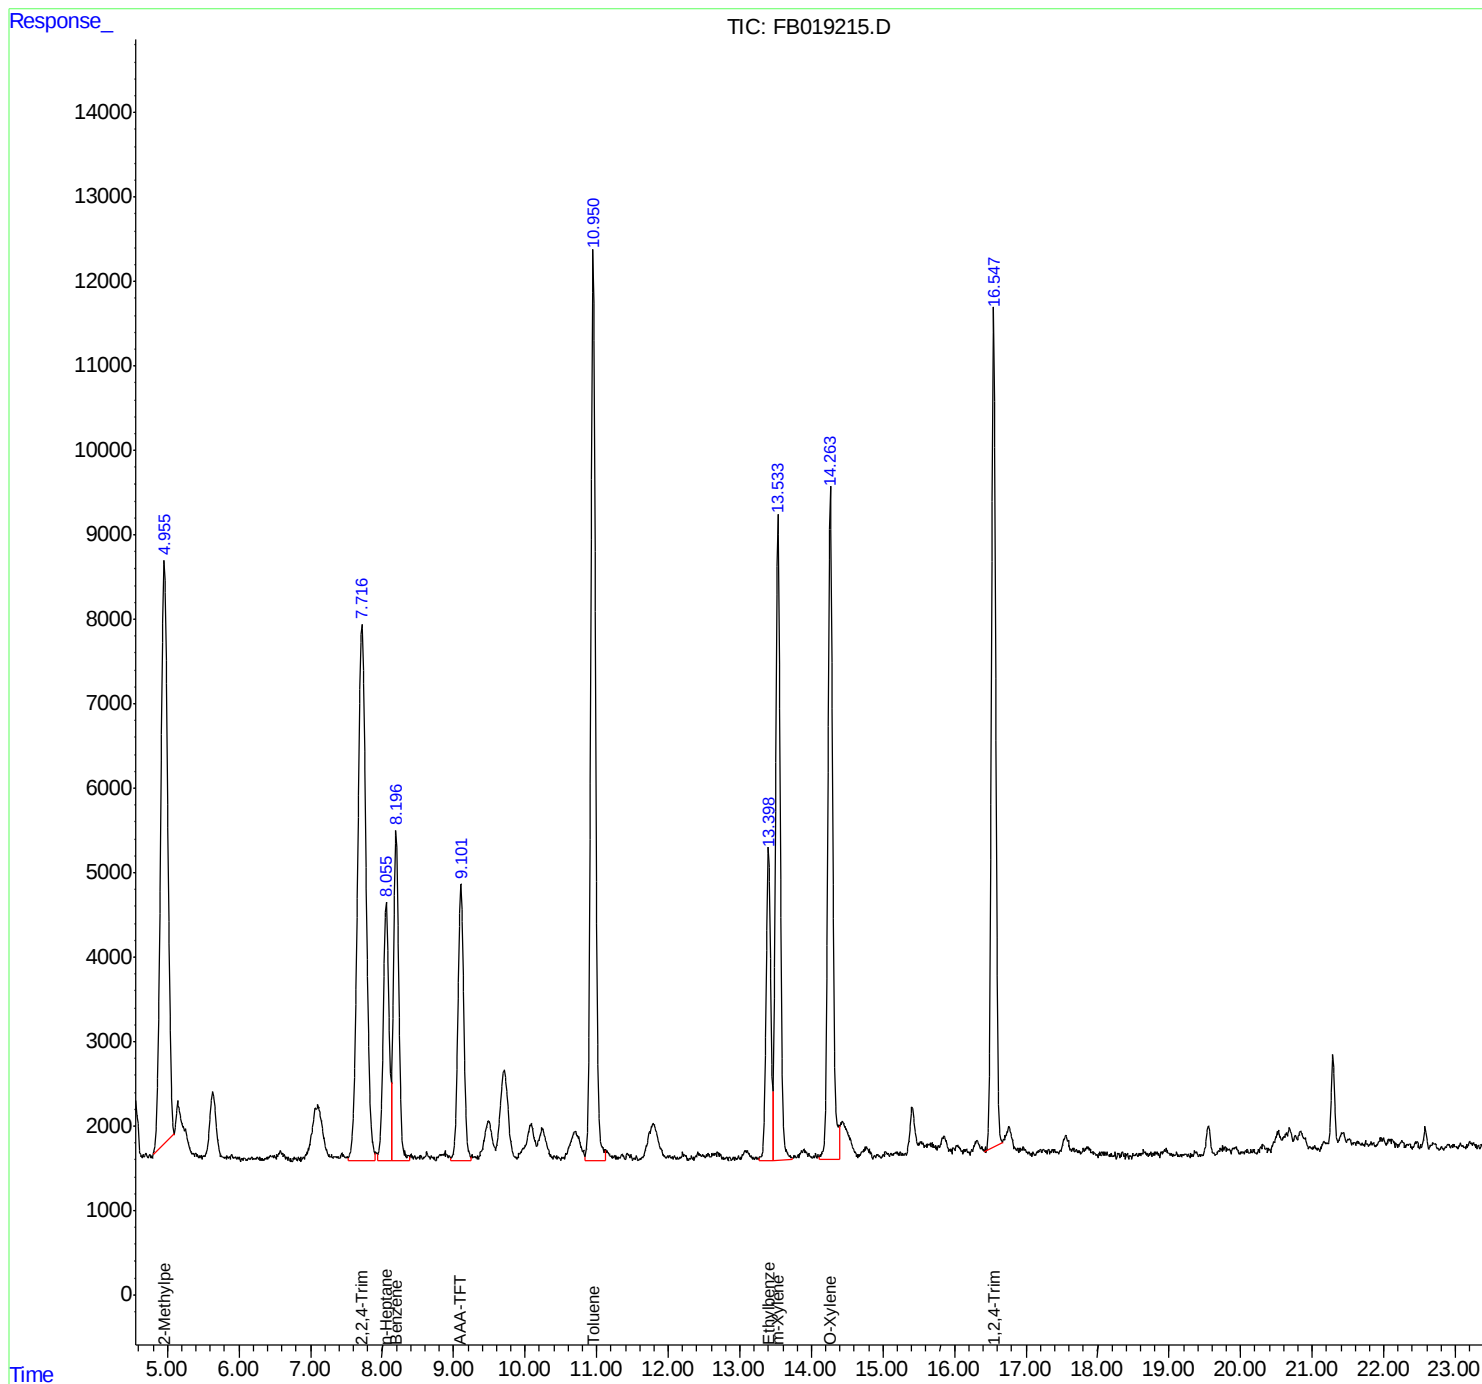


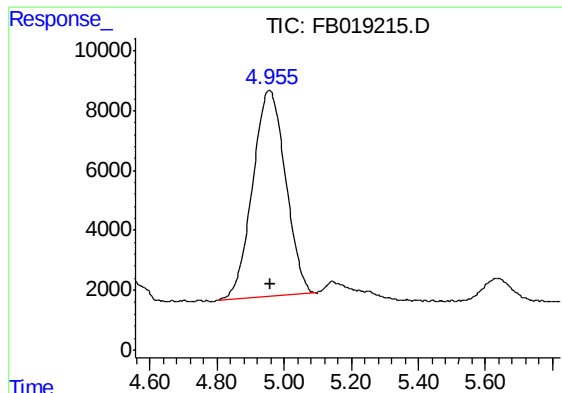

#1 2-Methylpentane


R.T.: 4.956 min
Delta R.T.: -0.005 min
Response: 470826
Conc: 30.80 ng/ml

Instrument :
FID_B
ClientSampleId :

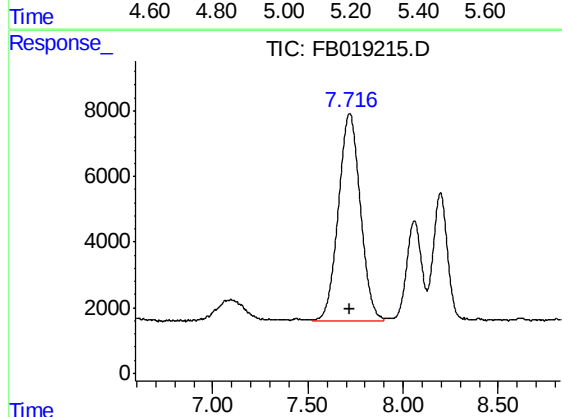


#2 2,2,4-Trimethylpentane

R.T.: 7.718 min
Delta R.T.: -0.005 min
Response: 518694
Conc: 33.67 ng/ml

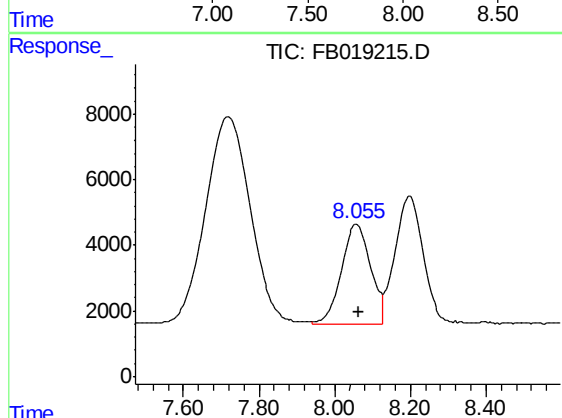


#3 n-Heptane

R.T.: 8.058 min
Delta R.T.: -0.004 min
Response: 167637
Conc: 11.28 ng/ml

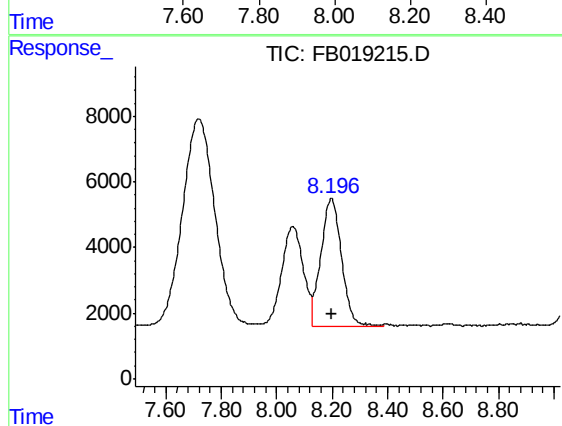

#4 Benzene


R.T.: 8.198 min
Delta R.T.: -0.003 min
Response: 204878
Conc: 11.37 ng/ml

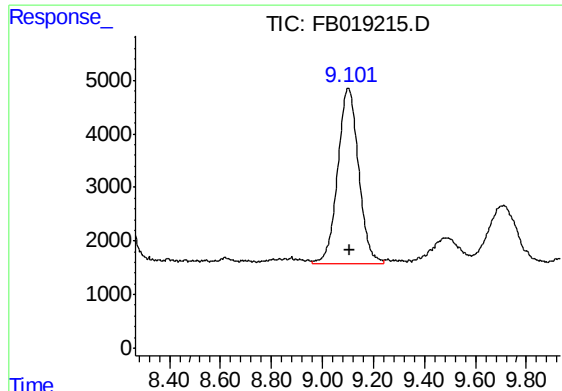

#5 AAA-TFT


R.T.: 9.102 min
Delta R.T.: -0.004 min
Response: 184644
Conc: 21.12 ng/ml

Instrument :
FID_B
ClientSampleId :

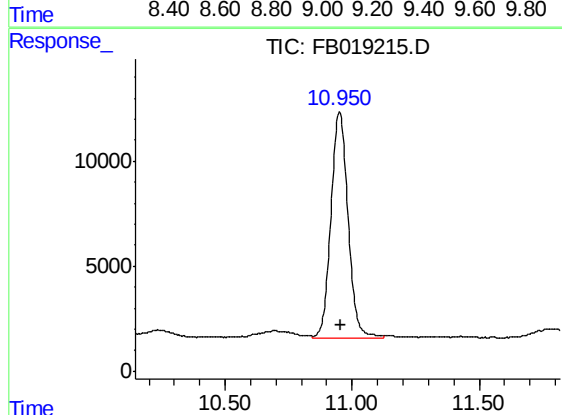


#6 Toluene

R.T.: 10.951 min
Delta R.T.: -0.005 min
Response: 502256
Conc: 33.09 ng/ml

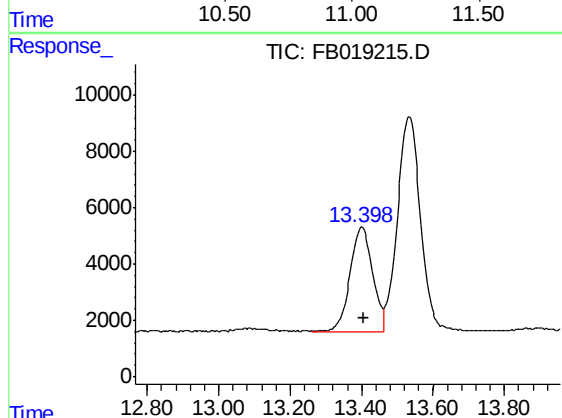


#7 Ethylbenzene

R.T.: 13.401 min
Delta R.T.: -0.005 min
Response: 163100
Conc: 10.50 ng/ml

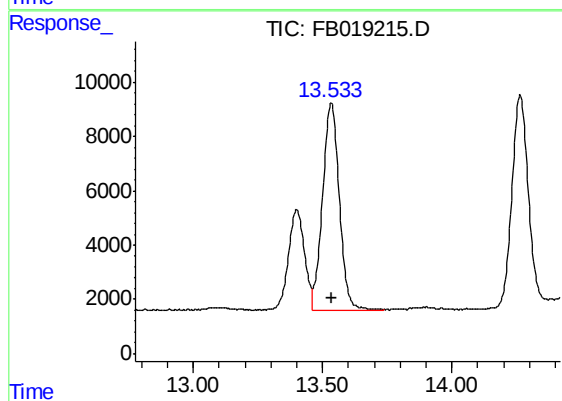

#8 m-Xylene


R.T.: 13.534 min
Delta R.T.: -0.004 min
Response: 344454
Conc: 21.14 ng/ml

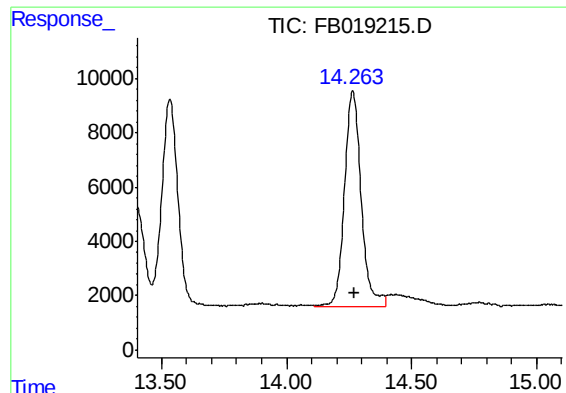

#9 O-Xylene

R.T.: 14.265 min
Delta R.T.: -0.005 min
Response: 369036
Conc: 21.83 ng/ml

Instrument :
FID_B
ClientSampleId :

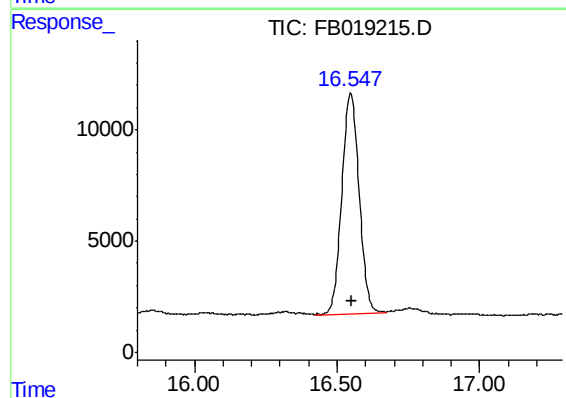

#10 1,2,4-Trimethylbenzene

R.T.: 16.548 min
Delta R.T.: -0.005 min
Response: 413281
Conc: 20.42 ng/ml