

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122719\
 Data File : FB023325.D
 Signal(s) : FID2B.CH
 Acq On : 27 Dec 2019 13:15
 Operator : DD/AJ
 Sample : K6437-05MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 27 21:49:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	427468	18.026 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	768540	24.832 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	780099	23.352 ng/ml
3) t n-Heptane	7.756	245461	7.441 ng/ml
4) t Benzene	7.890	368884	9.238 ng/ml
6) t Toluene	10.628	1027153	26.677 ng/ml
7) t Ethylbenzene	13.068	320466	8.829 ng/ml
8) t m-Xylene	13.200	610177	17.578 ng/ml
9) t O-Xylene	13.928	593882	17.632 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	473177	16.864 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122719\
 Data File : FB023325.D
 Signal(s) : FID2B.CH
 Acq On : 27 Dec 2019 13:15
 Operator : DD/AJ
 Sample : K6437-05MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampled :

Integration File: Calibration.e
 Quant Time: Dec 27 21:49:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

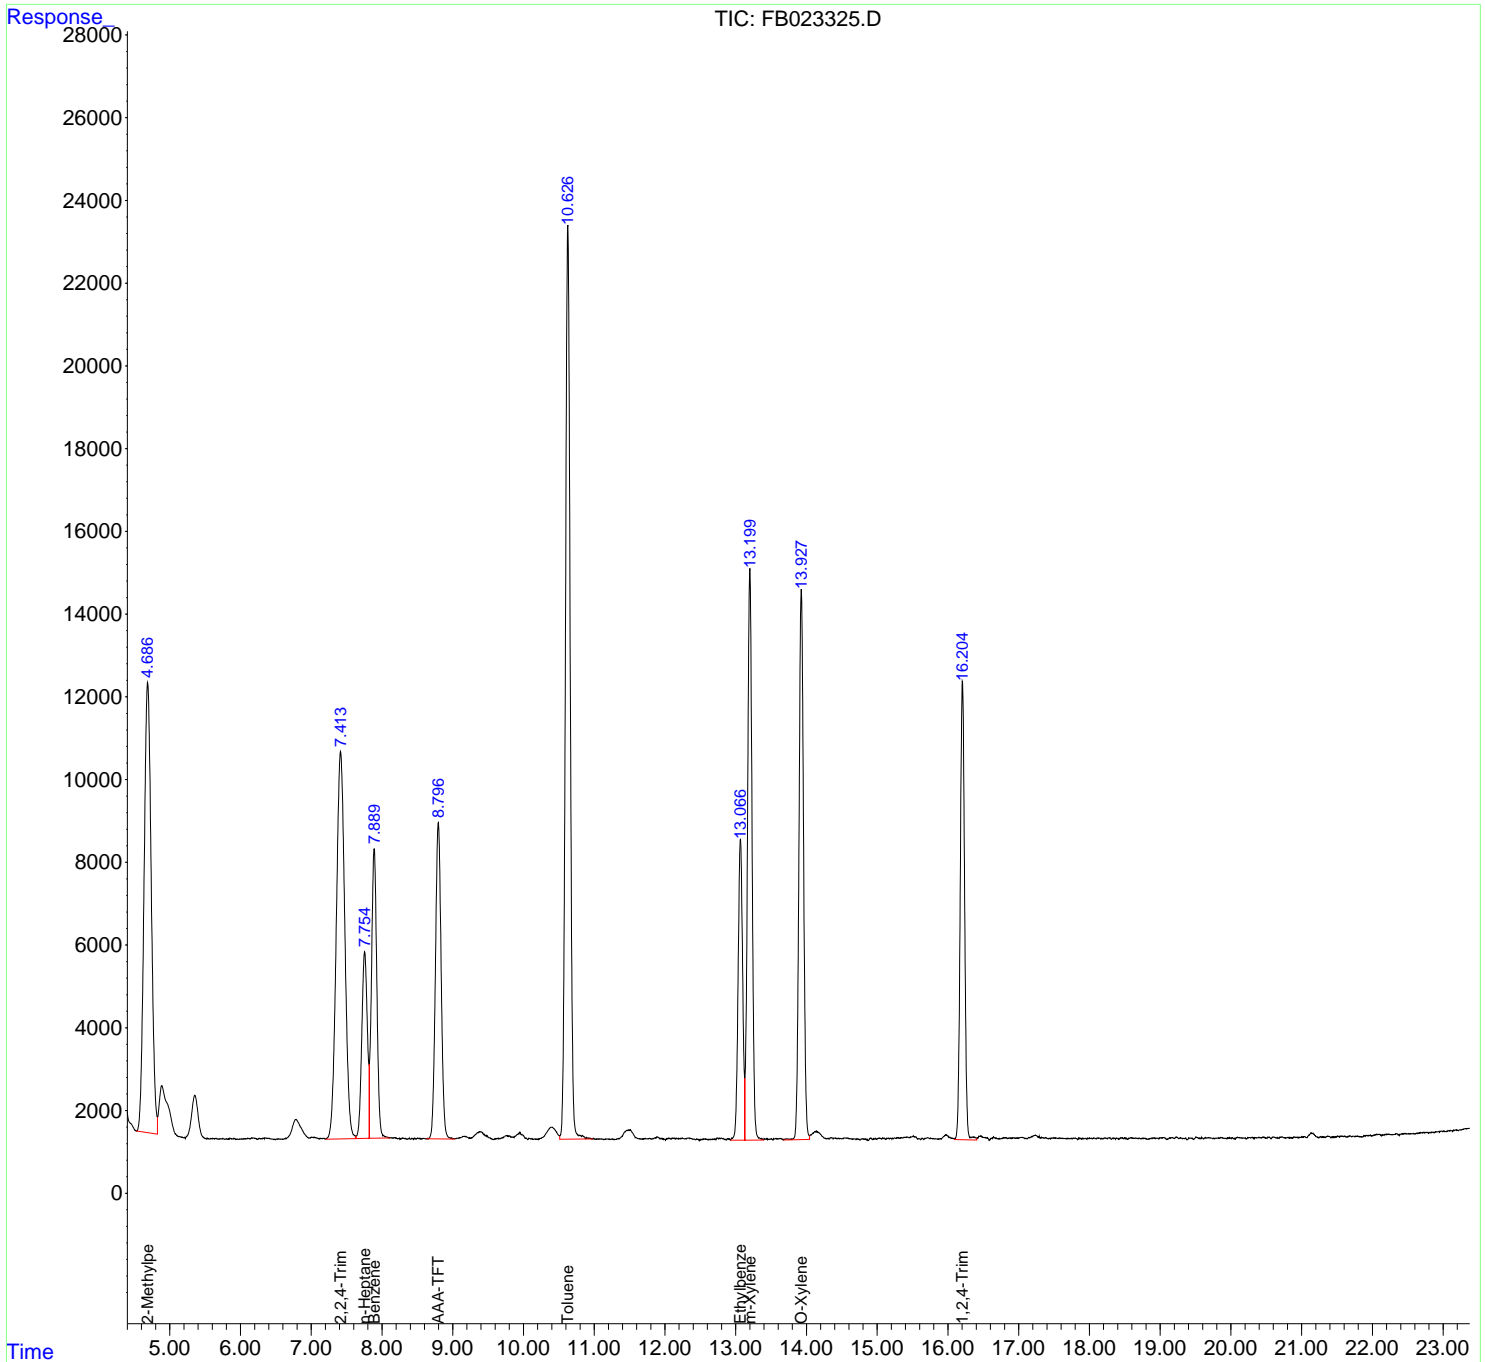

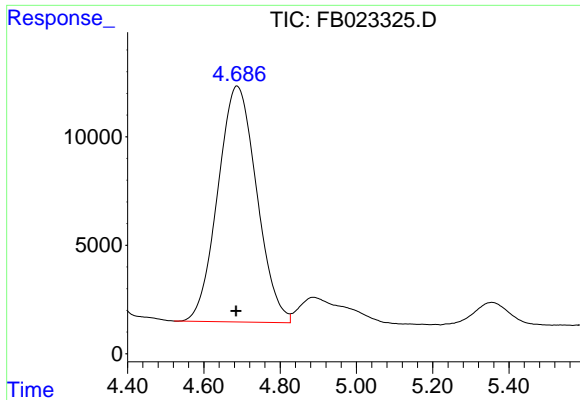


#1 2-Methylpentane
 R.T.: 4.687 min
 Delta R.T.: 0.003 min
 Response: 768540
 Conc: 24.83 ng/ml


Instrument :
 FID_B
 ClientSampled :

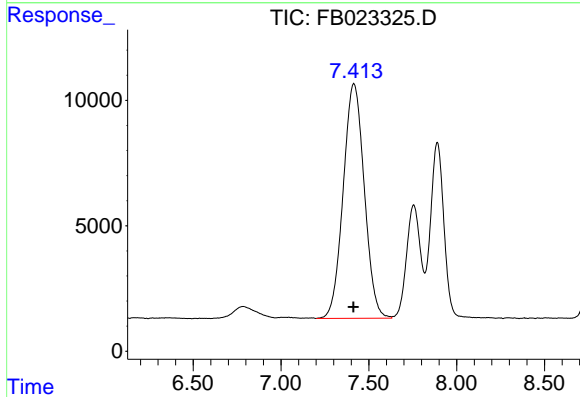


#2 2,2,4-Trimethylpentane
 R.T.: 7.415 min
 Delta R.T.: 0.003 min
 Response: 780099
 Conc: 23.35 ng/ml

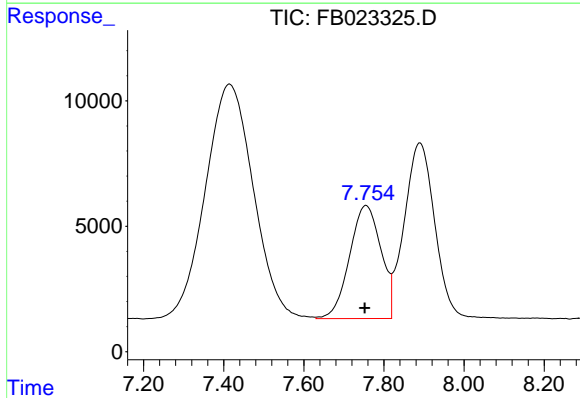

#3 n-Heptane
 R.T.: 7.756 min
 Delta R.T.: 0.004 min
 Response: 245461
 Conc: 7.44 ng/ml

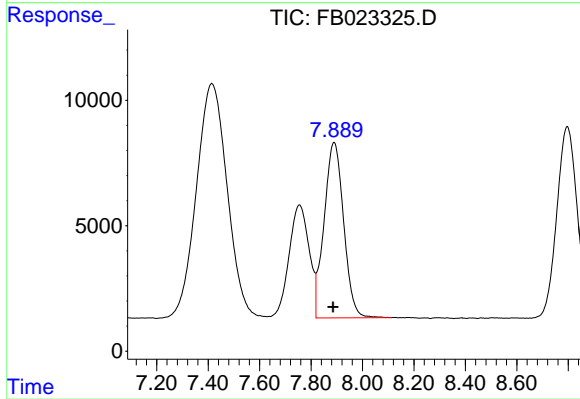


#4 Benzene
 R.T.: 7.890 min
 Delta R.T.: 0.004 min
 Response: 368884
 Conc: 9.24 ng/ml

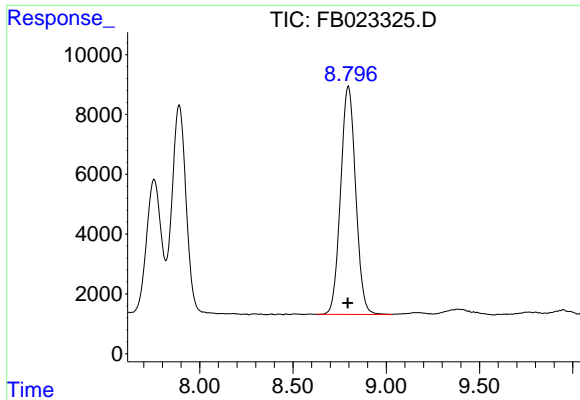


#5 AAA-TFT
 R.T.: 8.797 min
 Delta R.T.: 0.004 min
 Response: 427468
 Conc: 18.03 ng/ml


Instrument :
 FID_B
 ClientSampleId :

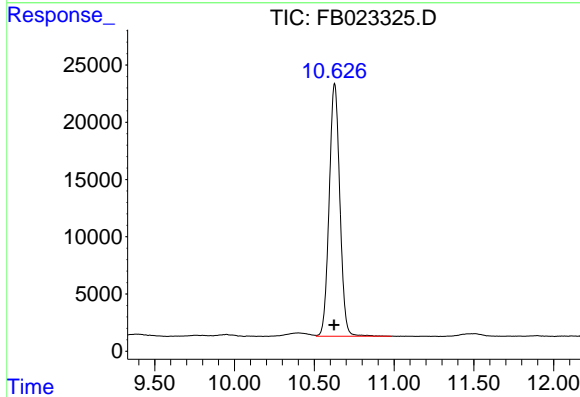


#6 Toluene
 R.T.: 10.628 min
 Delta R.T.: 0.004 min
 Response: 1027153
 Conc: 26.68 ng/ml

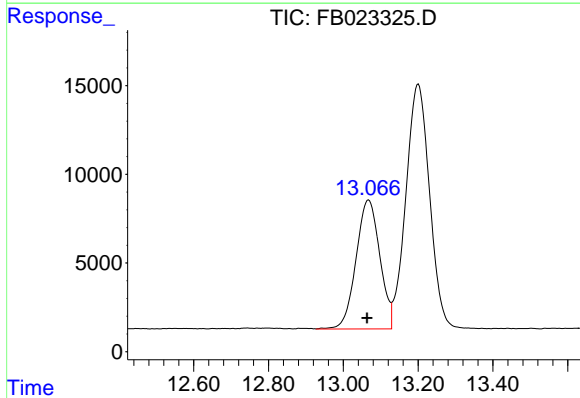

#7 Ethylbenzene
 R.T.: 13.068 min
 Delta R.T.: 0.004 min
 Response: 320466
 Conc: 8.83 ng/ml

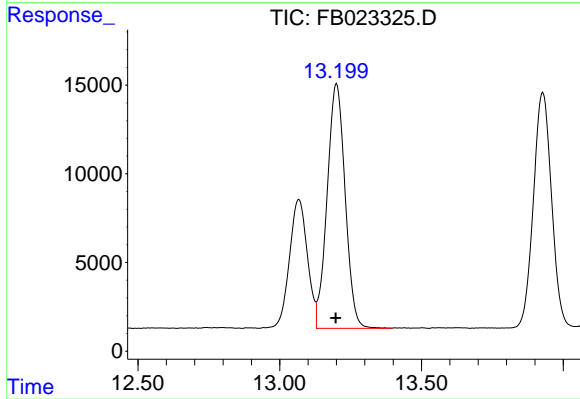


#8 m-Xylene
 R.T.: 13.200 min
 Delta R.T.: 0.003 min
 Response: 610177
 Conc: 17.58 ng/ml

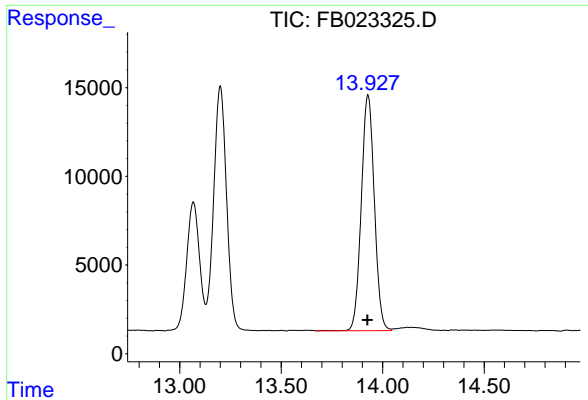

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: 0.003 min
Response: 593882
Conc: 17.63 ng/ml

Instrument :
FID_B
ClientSampleId :

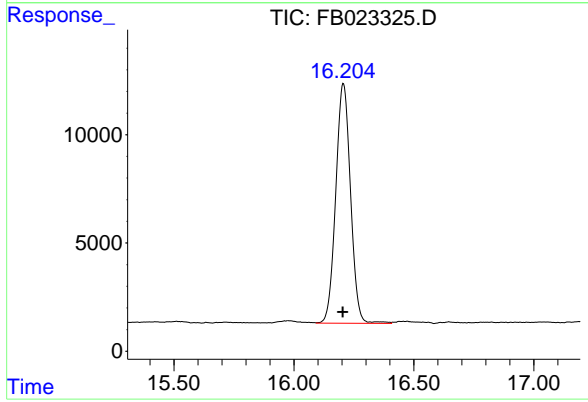

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: 0.003 min
Response: 473177
Conc: 16.86 ng/ml