

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB122719\  
 Data File : FB023326.D  
 Signal(s) : FID2B.CH  
 Acq On : 27 Dec 2019 14:18  
 Operator : DD/AJ  
 Sample : K6437-05MSD  
 Misc : 5.00g/5.00ml DI WATER  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Dec 27 21:49:30 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB121919.M  
 Quant Title :  
 QLast Update : Thu Dec 19 12:43:06 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
5) s AAA-TFT	8.795	460500	19.419 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	838835	27.103 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	919249	27.518 ng/ml
3) t n-Heptane	7.755	299953	9.093 ng/ml
4) t Benzene	7.889	377179	9.445 ng/ml
6) t Toluene	10.627	1094217	28.419 ng/ml
7) t Ethylbenzene	13.067	334453	9.215 ng/ml
8) t m-Xylene	13.200	640579	18.454 ng/ml
9) t O-Xylene	13.928	619927	18.405 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	526262	18.756 ng/ml
-----			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB122719\  
Data File : FB023326.D  
Signal(s) : FID2B.CH  
Acq On : 27 Dec 2019 14:18  
Operator : DD/AJ  
Sample : K6437-05MSD  
Misc : 5.00g/5.00ml DI WATER  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampled :

Integration File: Calibration.e  
Quant Time: Dec 27 21:49:30 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB121919.M  
Quant Title :  
QLast Update : Thu Dec 19 12:43:06 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

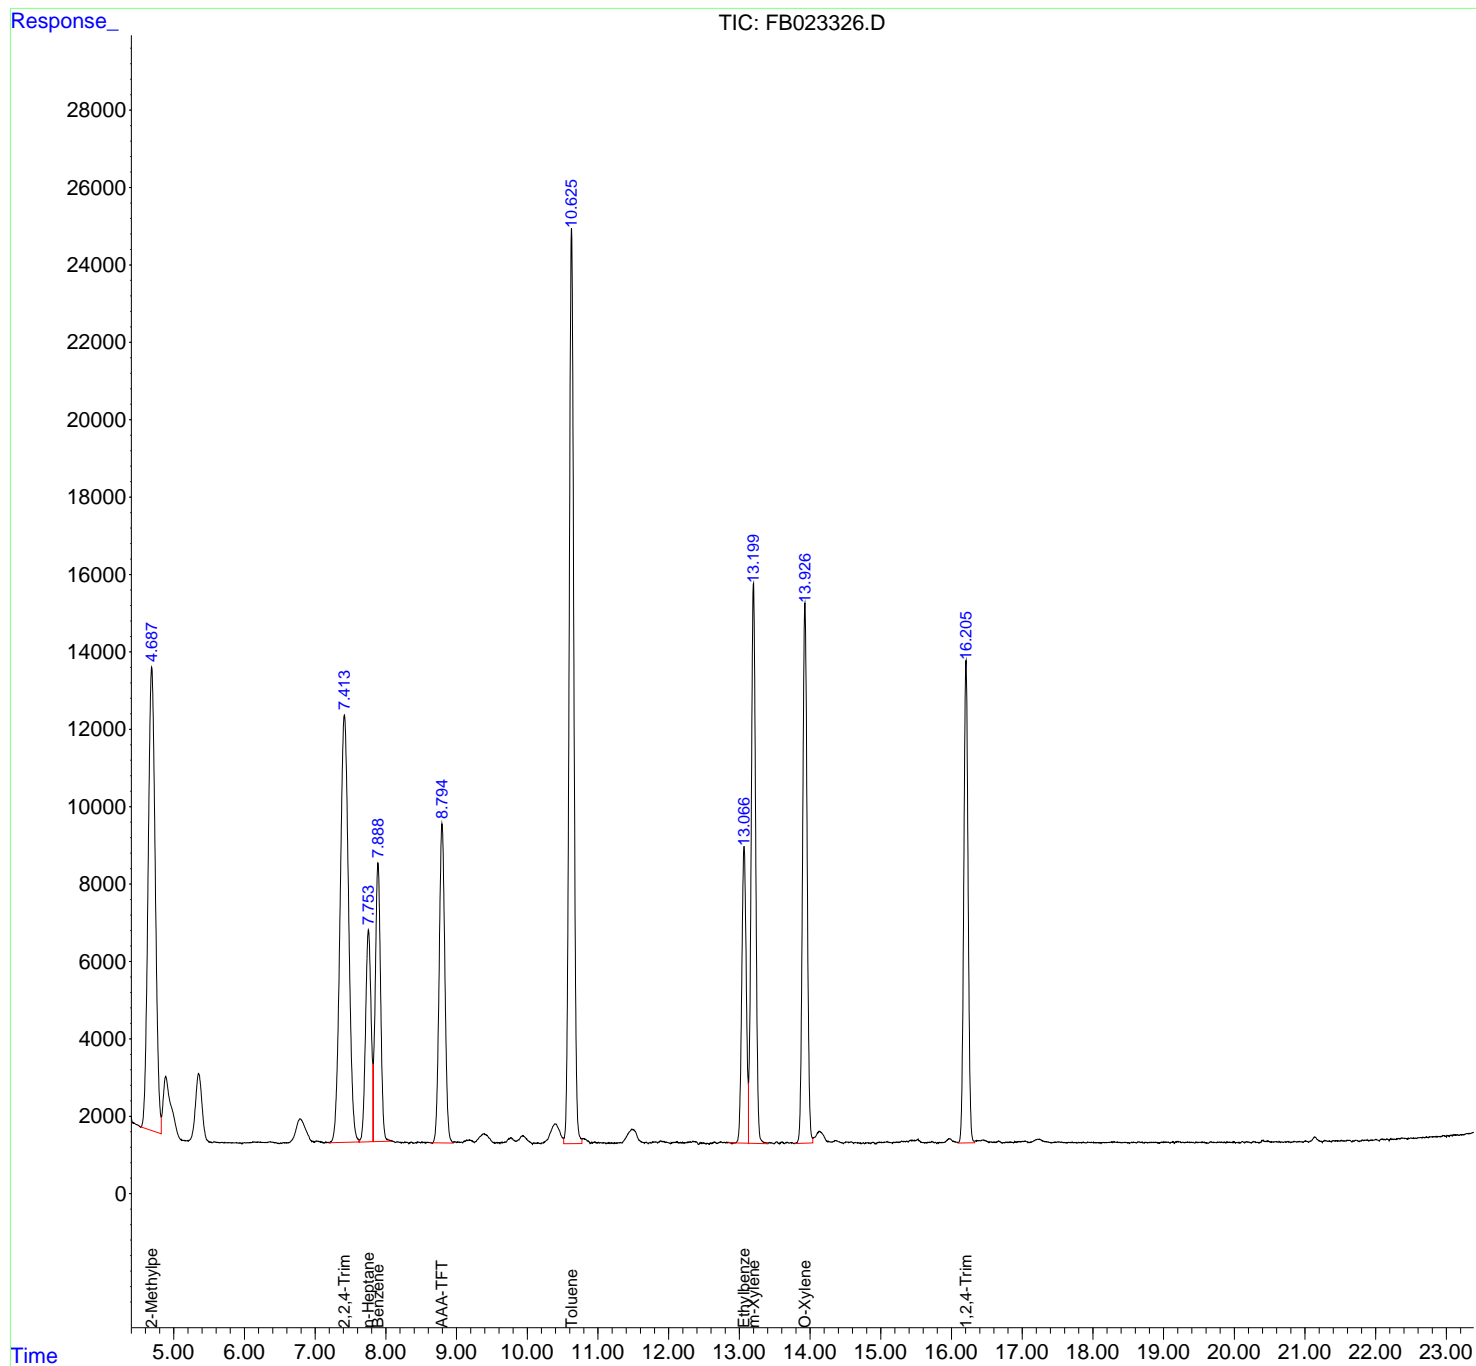


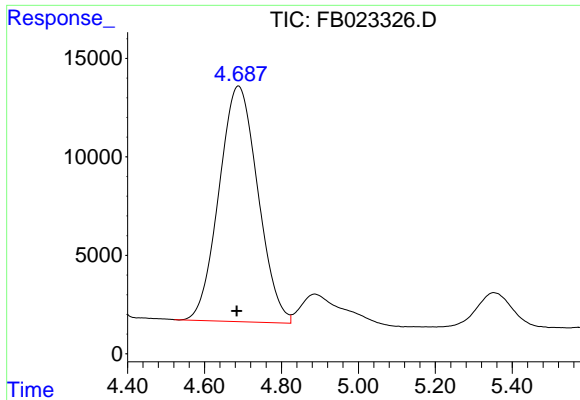

#1 2-Methylpentane


R.T.: 4.689 min  
 Delta R.T.: 0.005 min  
 Response: 838835  
 Conc: 27.10 ng/ml

Instrument :  
 FID\_B  
 ClientSampleId :

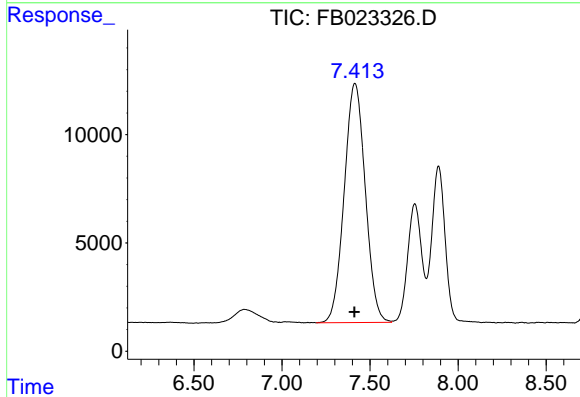


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min  
 Delta R.T.: 0.003 min  
 Response: 919249  
 Conc: 27.52 ng/ml

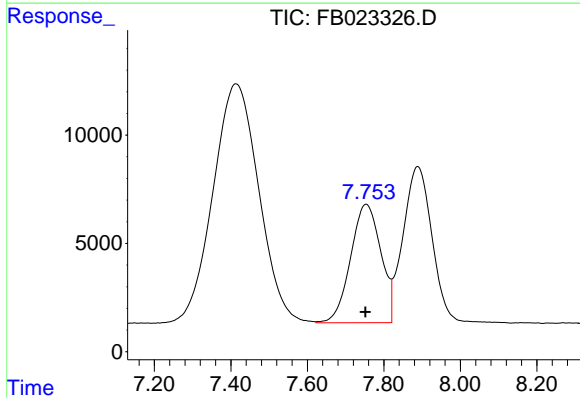


#3 n-Heptane

R.T.: 7.755 min  
 Delta R.T.: 0.003 min  
 Response: 299953  
 Conc: 9.09 ng/ml

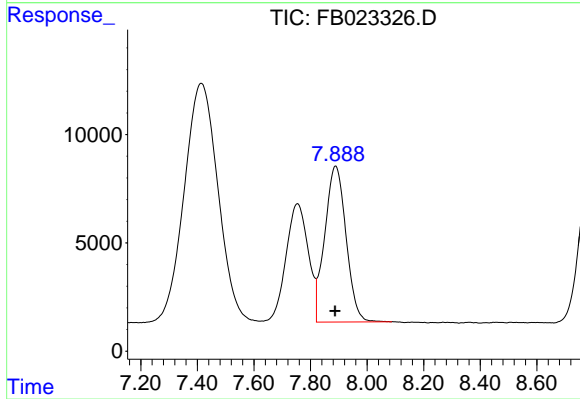


#4 Benzene

R.T.: 7.889 min  
 Delta R.T.: 0.003 min  
 Response: 377179  
 Conc: 9.45 ng/ml

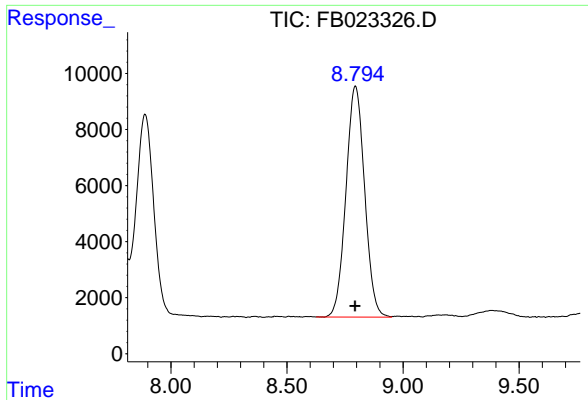


#5 AAA-TFT  
 R.T.: 8.795 min  
 Delta R.T.: 0.002 min  
 Response: 460500  
 Conc: 19.42 ng/ml


Instrument :  
 FID\_B  
 ClientSampled :

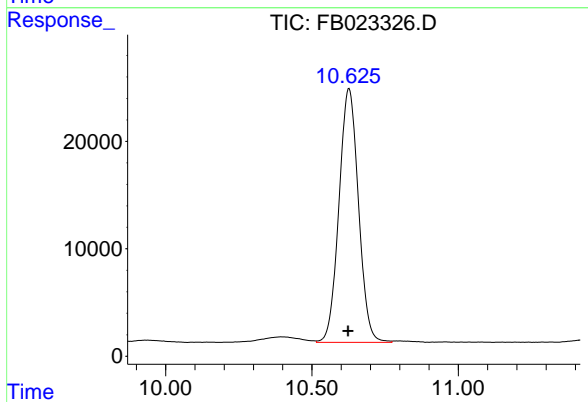


#6 Toluene  
 R.T.: 10.627 min  
 Delta R.T.: 0.003 min  
 Response: 1094217  
 Conc: 28.42 ng/ml

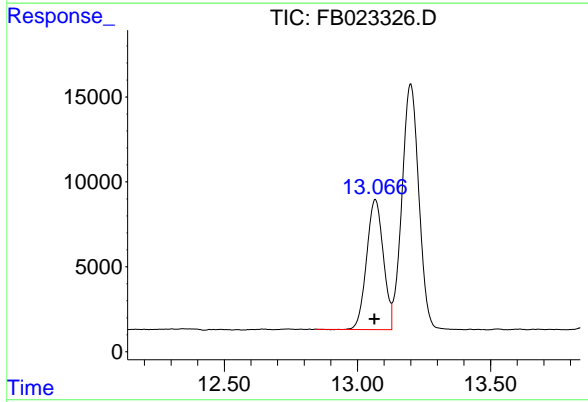

#7 Ethylbenzene  
 R.T.: 13.067 min  
 Delta R.T.: 0.004 min  
 Response: 334453  
 Conc: 9.21 ng/ml

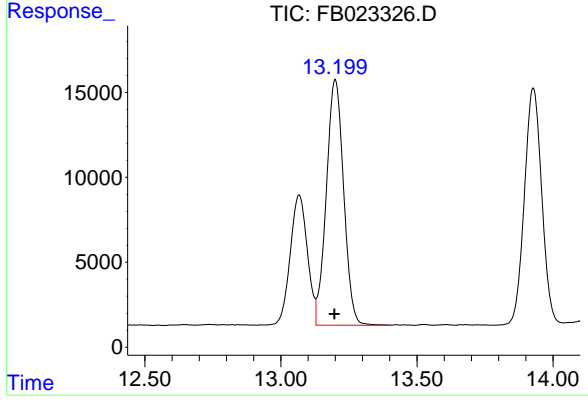


#8 m-Xylene  
 R.T.: 13.200 min  
 Delta R.T.: 0.003 min  
 Response: 640579  
 Conc: 18.45 ng/ml

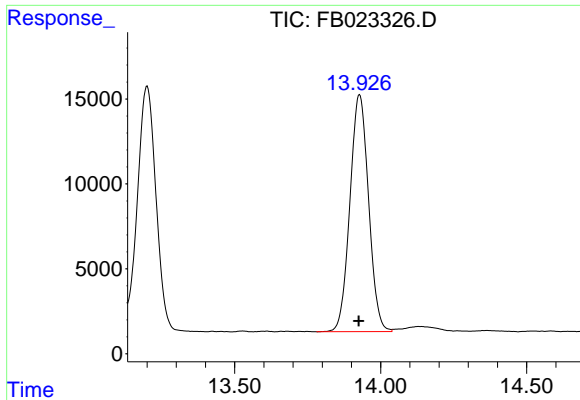

#9 O-Xylene

R.T.: 13.928 min  
Delta R.T.: 0.003 min  
Response: 619927  
Conc: 18.40 ng/ml

Instrument :  
FID\_B  
ClientSampled :

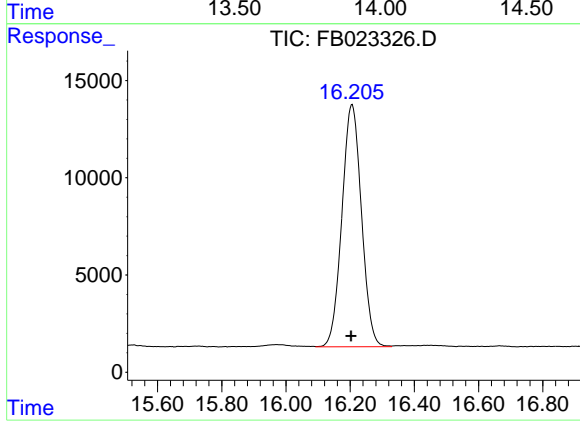

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min  
Delta R.T.: 0.003 min  
Response: 526262  
Conc: 18.76 ng/ml