

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122719\
 Data File : FB023326.D
 Signal(s) : FID2B.CH
 Acq On : 27 Dec 2019 14:18
 Operator : DD/AJ
 Sample : K6437-05MSD
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 GP-3-(1-3)MSD

Integration File: Calibration.e
 Quant Time: Dec 27 21:49:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	460500	19.419 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	838835	27.103 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	919249	27.518 ng/ml
3) t n-Heptane	7.755	299953	9.093 ng/ml
4) t Benzene	7.889	377179	9.445 ng/ml
6) t Toluene	10.627	1094217	28.419 ng/ml
7) t Ethylbenzene	13.067	334453	9.215 ng/ml
8) t m-Xylene	13.200	640579	18.454 ng/ml
9) t O-Xylene	13.928	619927	18.405 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	526262	18.756 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122719\
Data File : FB023326.D
Signal(s) : FID2B.CH
Acq On : 27 Dec 2019 14:18
Operator : DD/AJ
Sample : K6437-05MSD
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
GP-3-(1-3)MSD

Integration File: Calibration.e
Quant Time: Dec 27 21:49:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

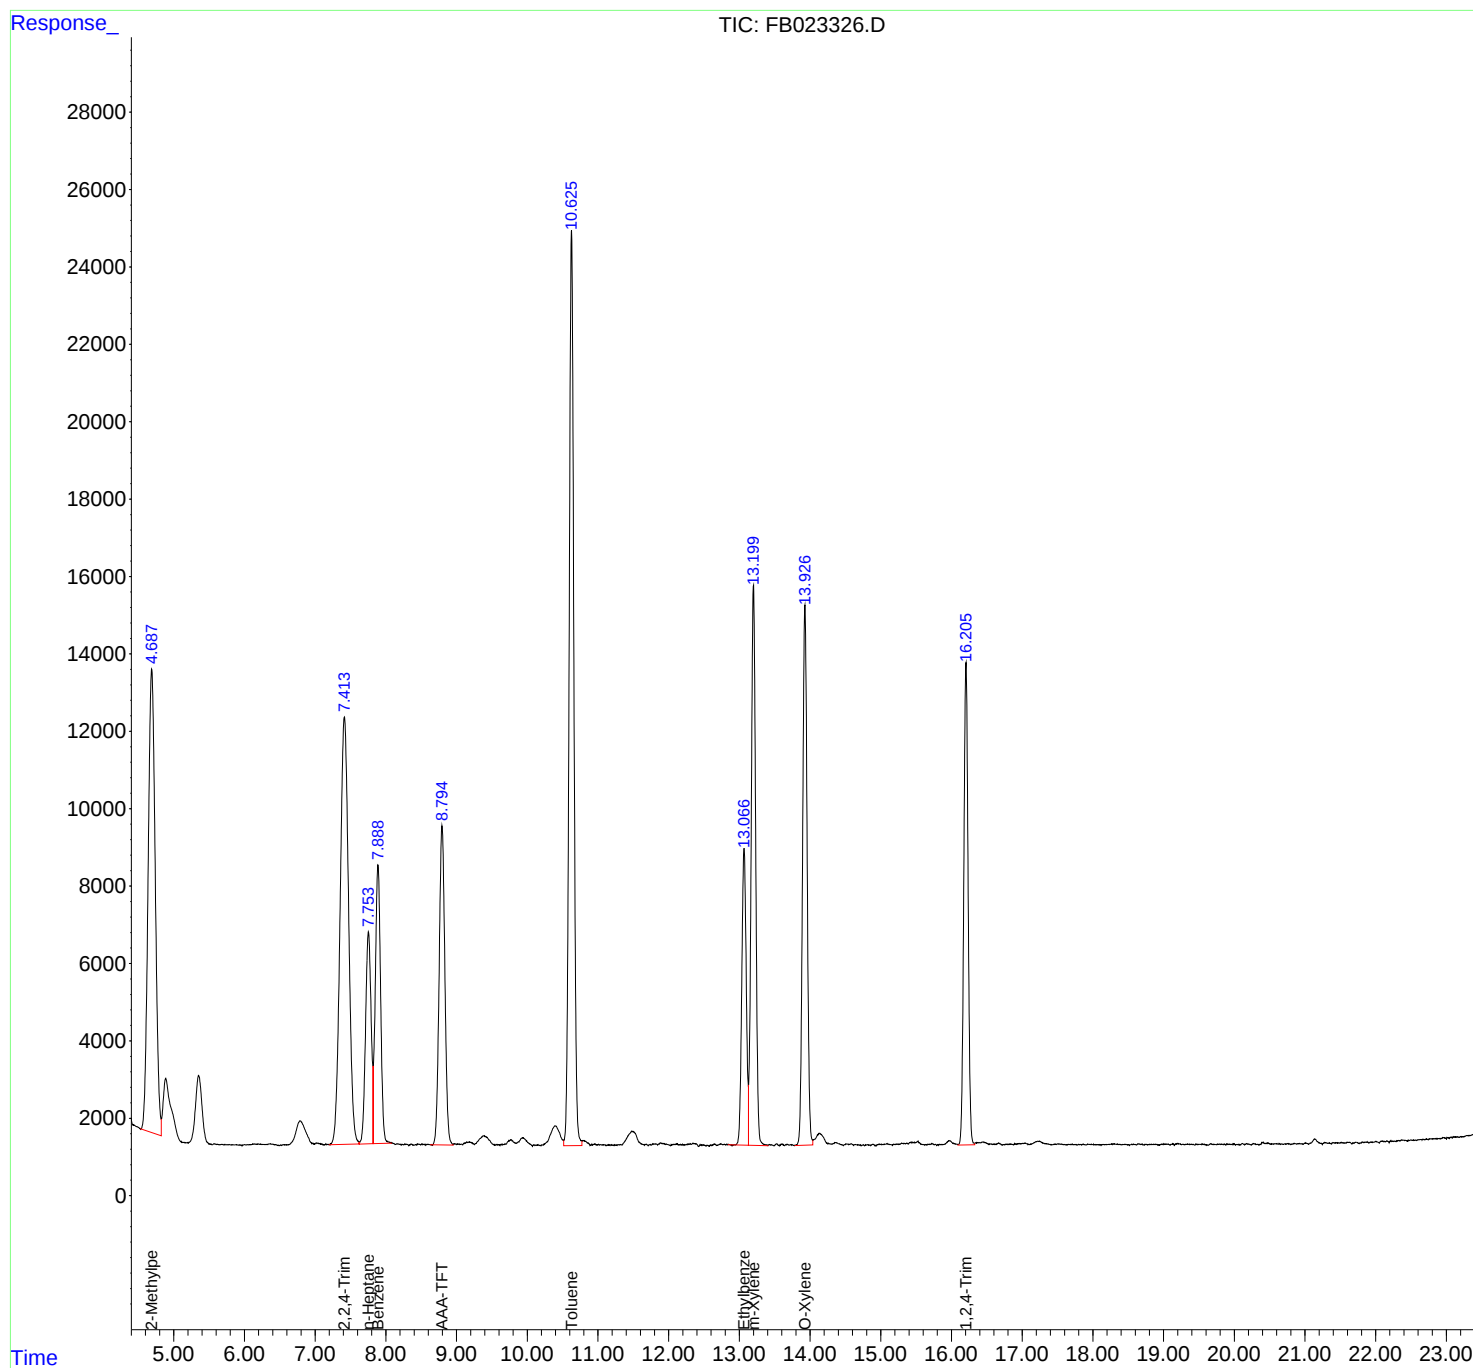


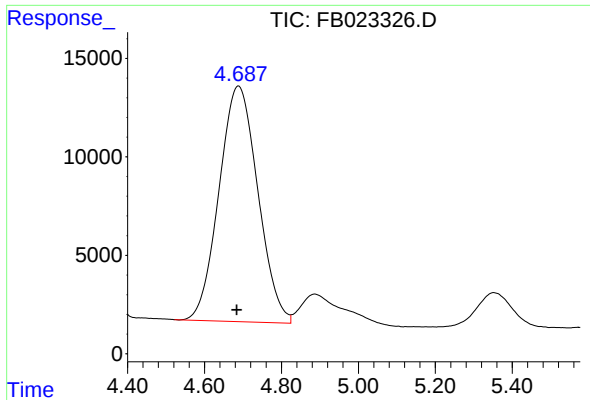

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.005 min
Response: 838835
Conc: 27.10 ng/ml

Instrument :
FID_B
ClientSampleId :
GP-3-(1-3)MSD

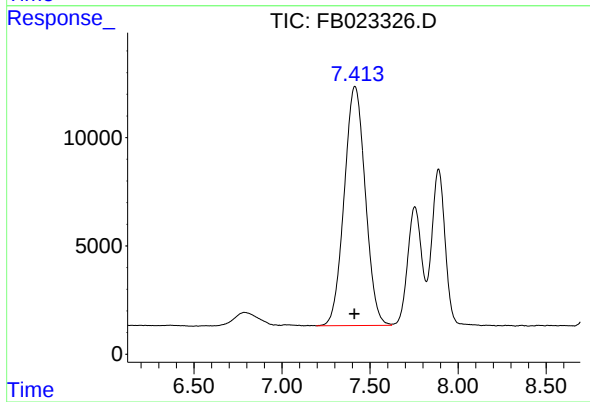


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: 0.003 min
Response: 919249
Conc: 27.52 ng/ml

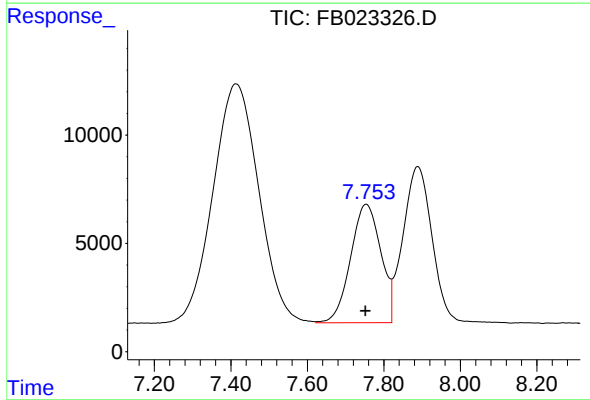


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.003 min
Response: 299953
Conc: 9.09 ng/ml

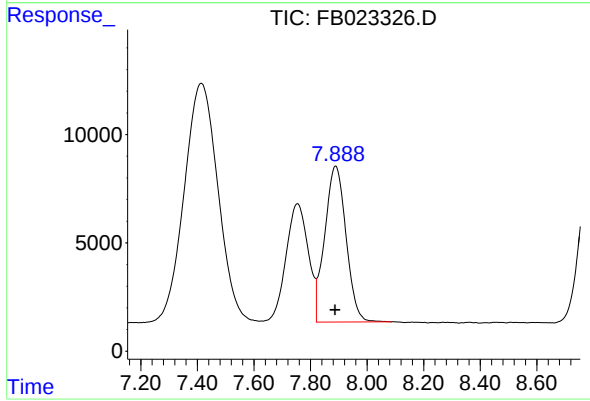

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.003 min
Response: 377179
Conc: 9.45 ng/ml

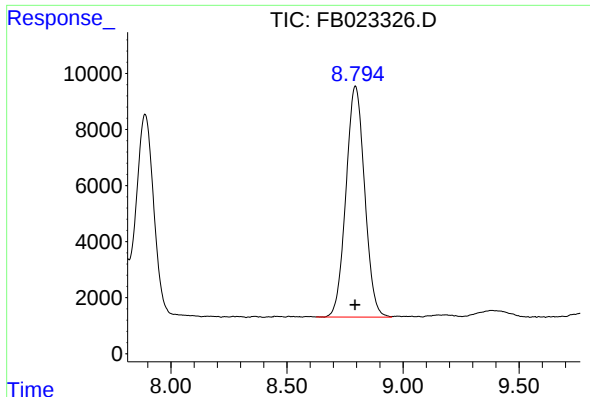

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.002 min
Response: 460500
Conc: 19.42 ng/ml

Instrument :
FID_B
ClientSampleId :
GP-3-(1-3)MSD

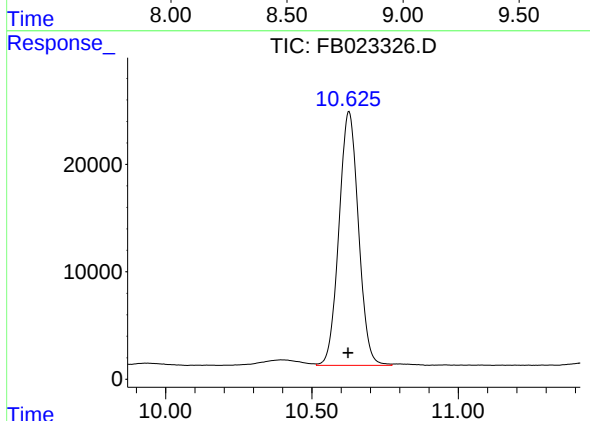


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.003 min
Response: 1094217
Conc: 28.42 ng/ml

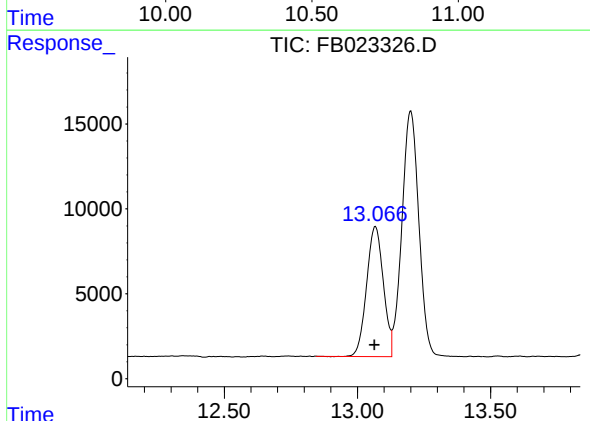


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: 0.004 min
Response: 334453
Conc: 9.21 ng/ml

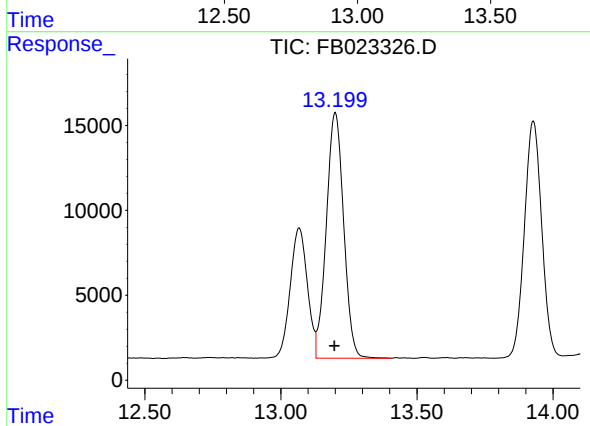

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: 0.003 min
Response: 640579
Conc: 18.45 ng/ml

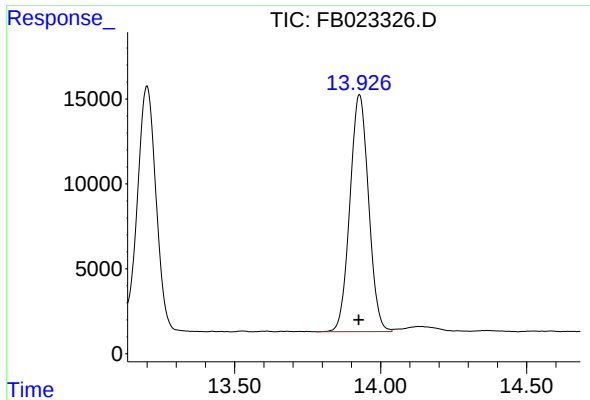

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: 0.003 min
Response: 619927
Conc: 18.40 ng/ml

Instrument :
FID_B
ClientSampleId :
GP-3-(1-3)MSD

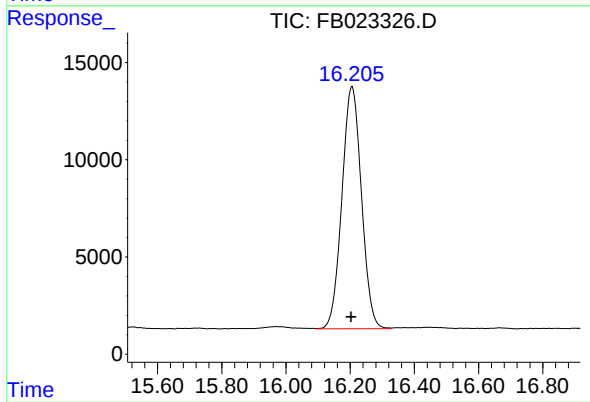

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: 0.003 min
Response: 526262
Conc: 18.76 ng/ml