

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122719\
 Data File : FB023328.D
 Signal(s) : FID2B.CH
 Acq On : 27 Dec 2019 15:44
 Operator : DD/AJ
 Sample : K6113-12
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 OR-03-122619

Integration File: Calibration.e
 Quant Time: Dec 27 21:49:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	417715	17.615 ng/ml
Target Compounds			
6) t Toluene	10.625	7285	0.189 ng/ml
7) t Ethylbenzene	13.052	2355	0.065 ng/ml
8) t m-Xylene	13.200	8555	0.246 ng/ml
9) t O-Xylene	13.937	9972	0.296 ng/ml
10) t 1,2,4-Trimethylbenzene	16.203	9727	0.347 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122719\
Data File : FB023328.D
Signal(s) : FID2B.CH
Acq On : 27 Dec 2019 15:44
Operator : DD/AJ
Sample : K6113-12
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
OR-03-122619

Integration File: Calibration.e
Quant Time: Dec 27 21:49:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

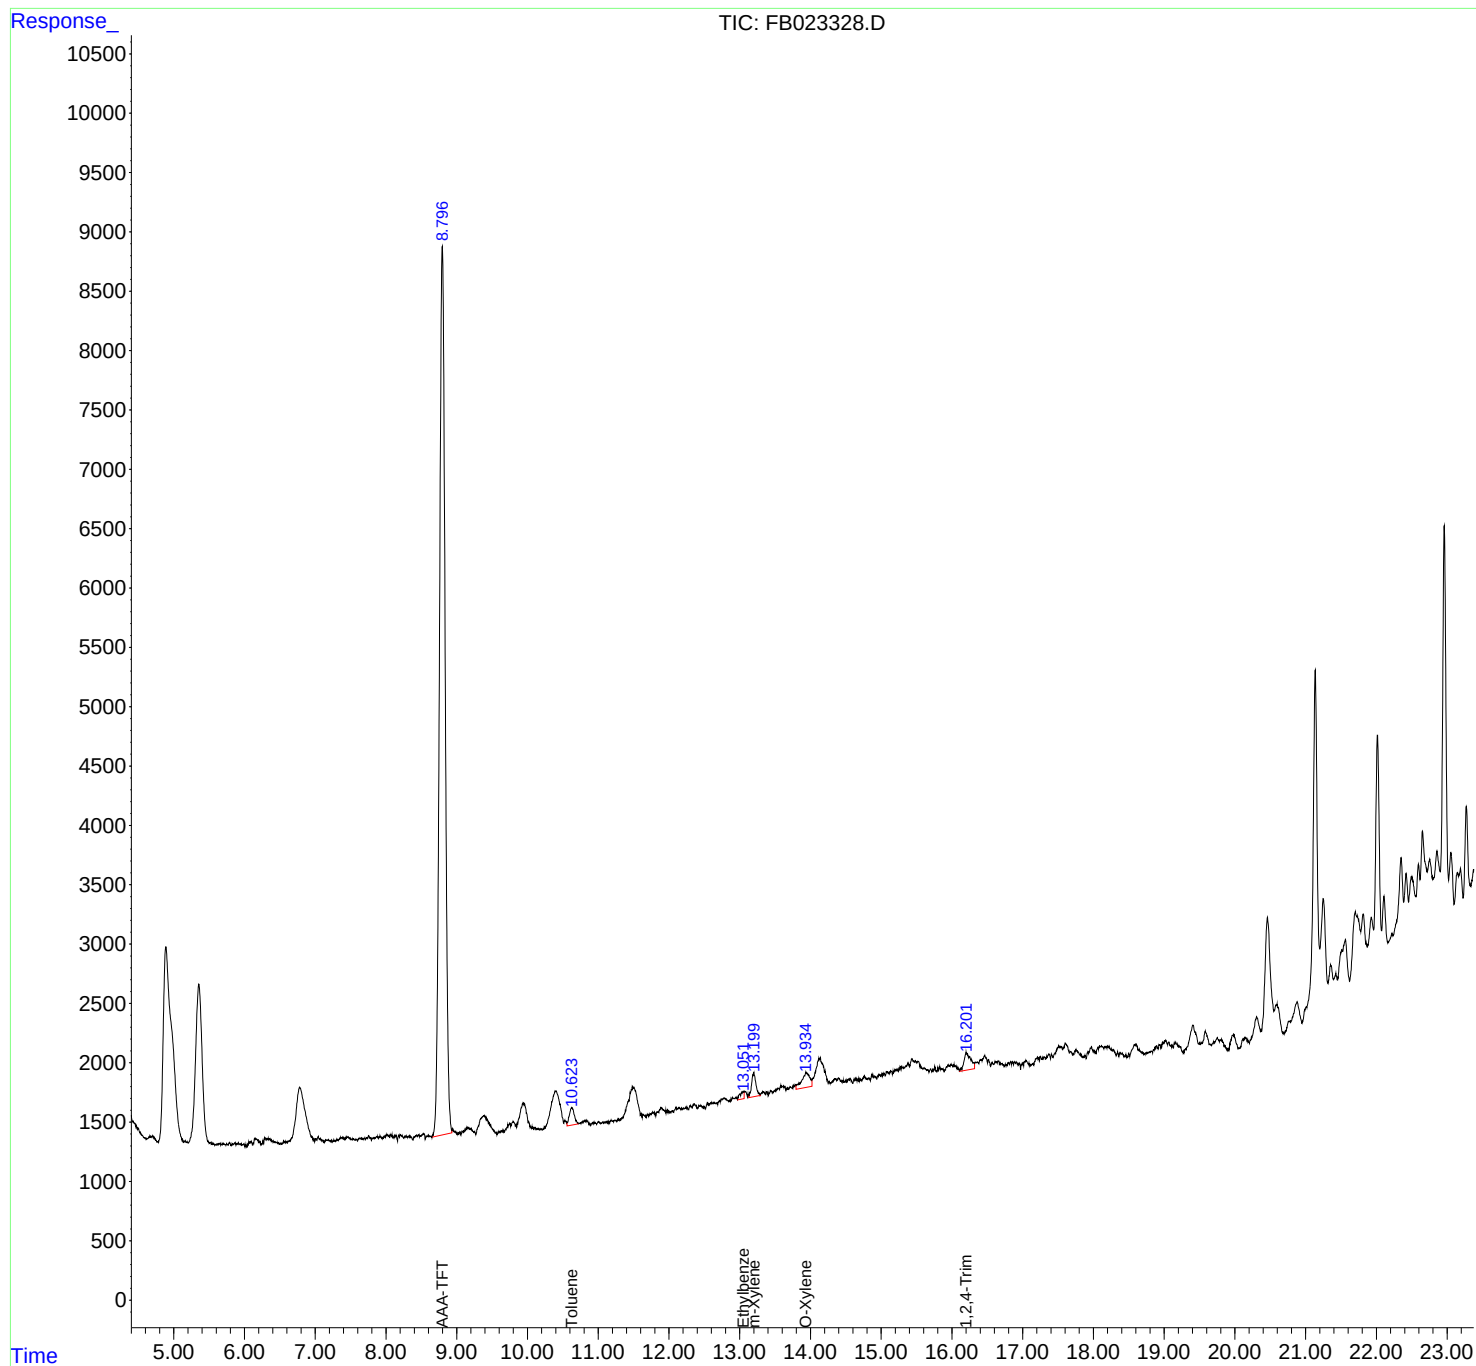


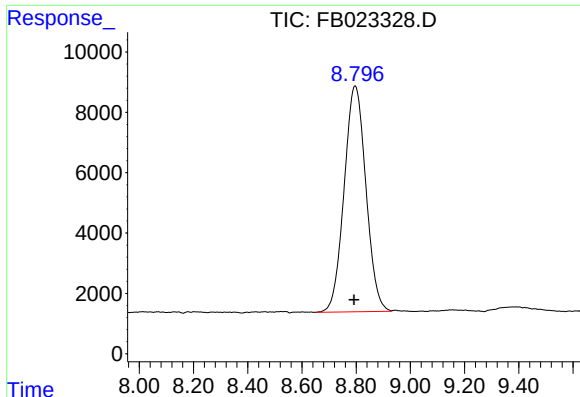

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.004 min
Response: 417715
Conc: 17.61 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-03-122619

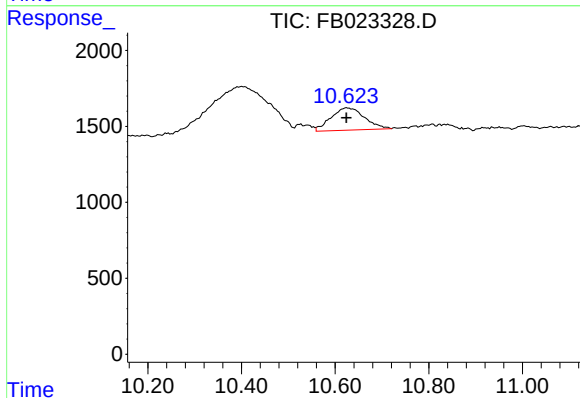


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.001 min
Response: 7285
Conc: 0.19 ng/ml

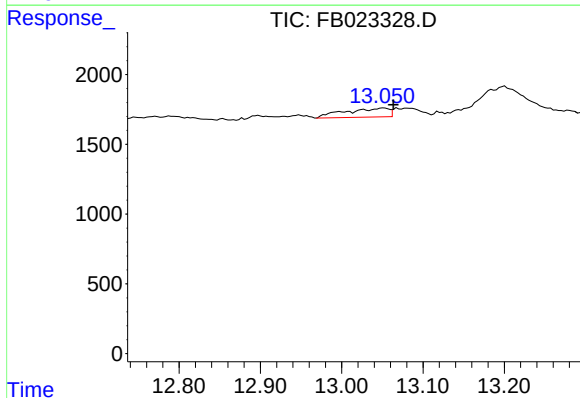


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.012 min
Response: 2355
Conc: 0.06 ng/ml

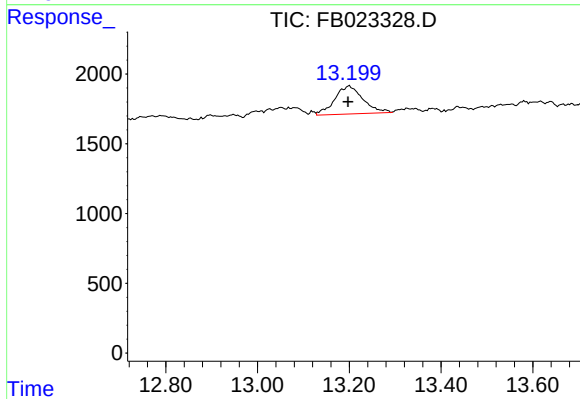

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: 0.003 min
Response: 8555
Conc: 0.25 ng/ml

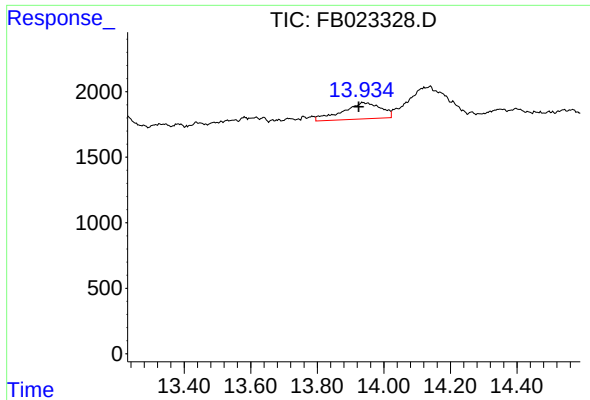

#9 O-Xylene

R.T.: 13.937 min
Delta R.T.: 0.012 min
Response: 9972
Conc: 0.30 ng/ml

Instrument :
FID_B
ClientSampleId :
OR-03-122619

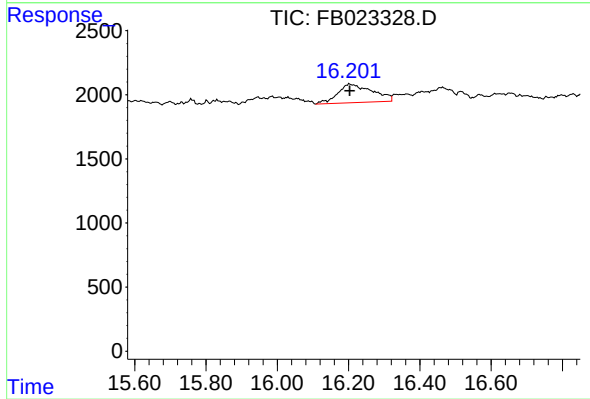

#10 1,2,4-Trimethylbenzene

R.T.: 16.203 min
Delta R.T.: 0.000 min
Response: 9727
Conc: 0.35 ng/ml