

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122719\
Data File : FB023330.D
Signal(s) : FID2B.CH
Acq On : 27 Dec 2019 16:56
Operator : DD/AJ
Sample : K6441-06
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
K321-WC-01

Integration File: Calibration.e
Quant Time: Dec 27 21:50:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	273587	11.537 ng/ml
Target Compounds			
6) t Toluene	10.621	1171	0.030 ng/ml
7) t Ethylbenzene	13.048	1508	0.042 ng/ml
8) t m-Xylene	13.199	8312	0.239 ng/ml
9) t O-Xylene	13.922	2782	0.083 ng/ml
10) t 1,2,4-Trimethylbenzene	16.218	2190	0.078 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122719\
Data File : FB023330.D
Signal(s) : FID2B.CH
Acq On : 27 Dec 2019 16:56
Operator : DD/AJ
Sample : K6441-06
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
K321-WC-01

Integration File: Calibration.e
Quant Time: Dec 27 21:50:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

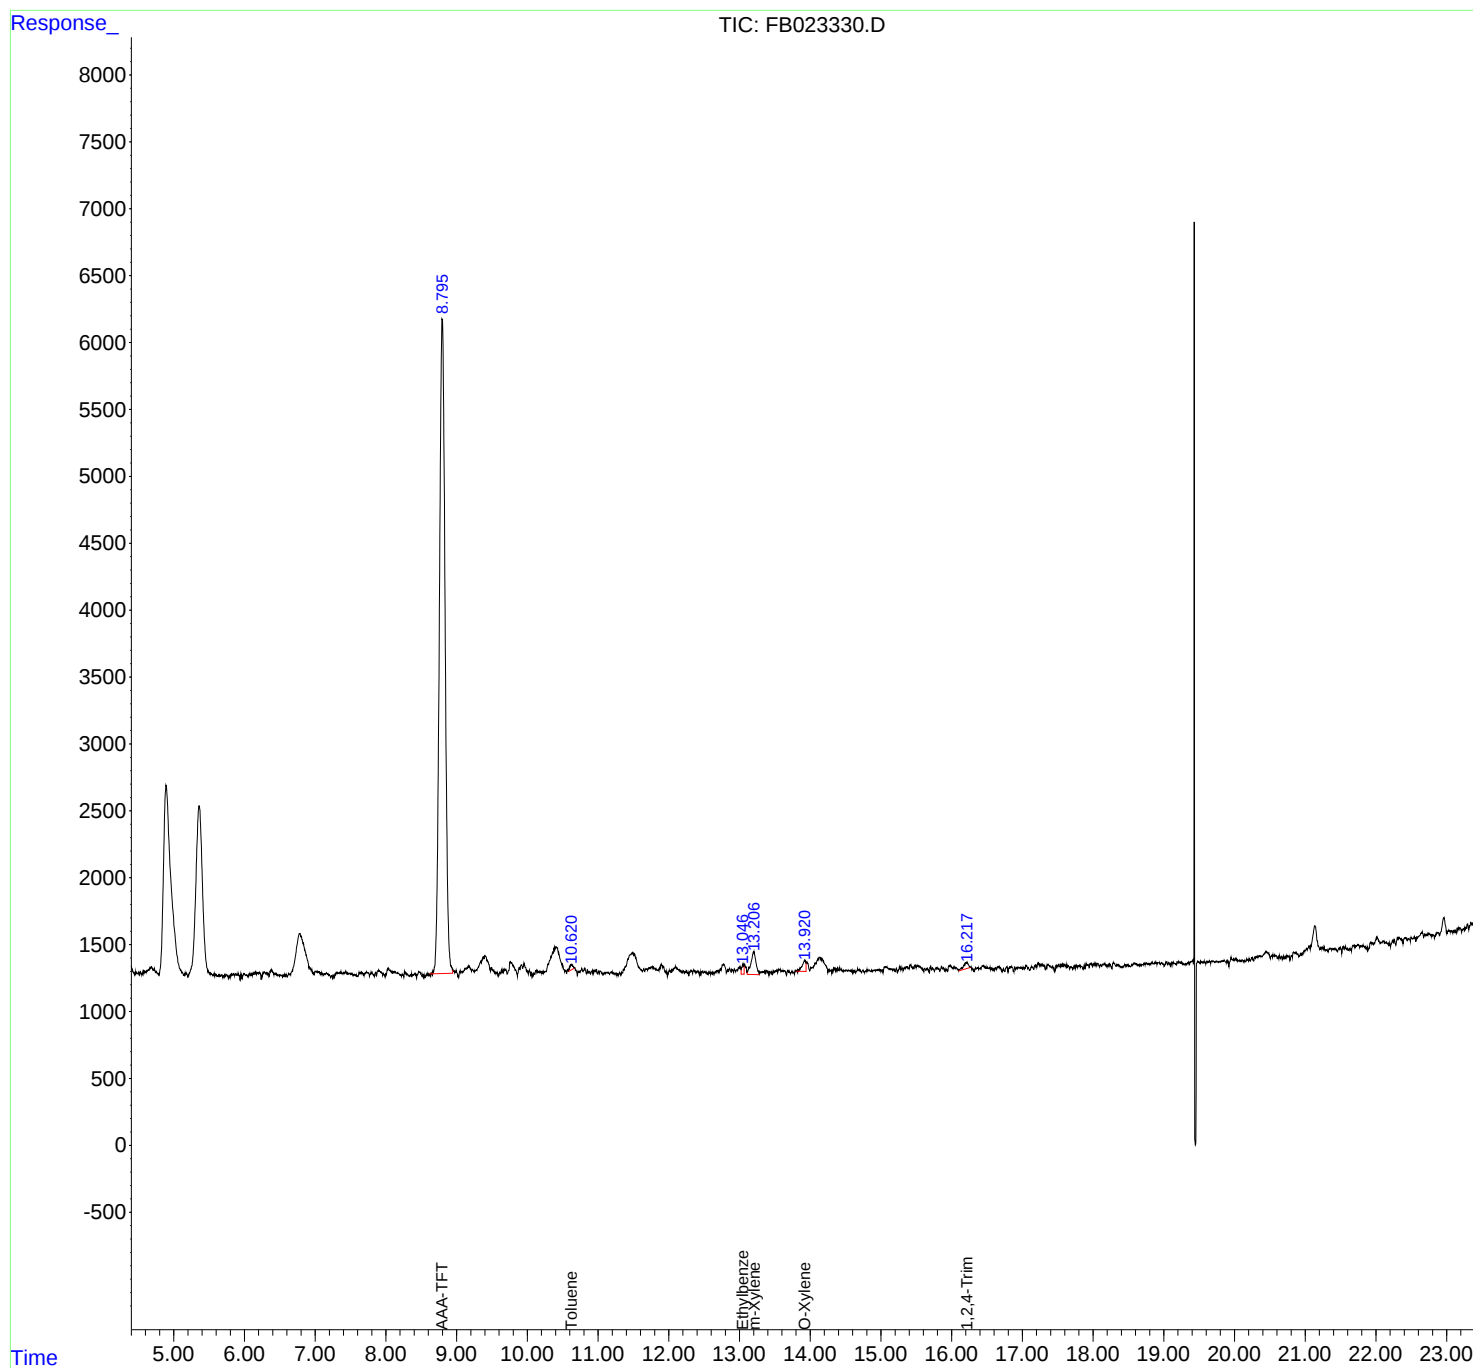


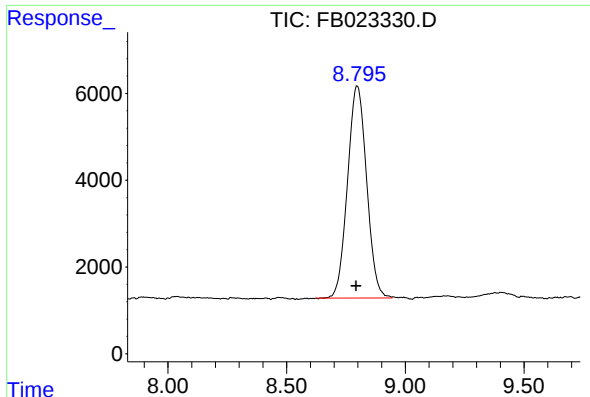

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: 0.004 min
Response: 273587
Conc: 11.54 ng/ml

Instrument :
FID_B
ClientSampleId :
K321-WC-01

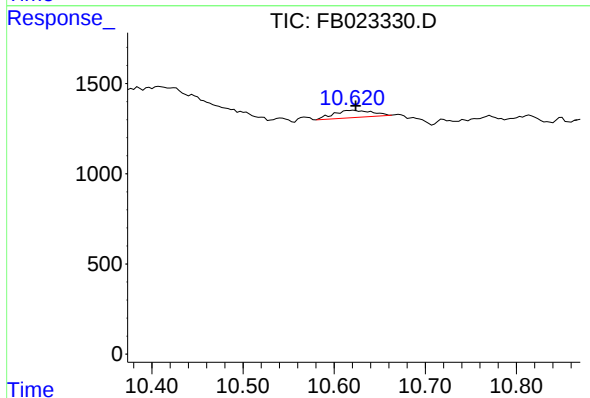


#6 Toluene

R.T.: 10.621 min
Delta R.T.: -0.002 min
Response: 1171
Conc: 0.03 ng/ml

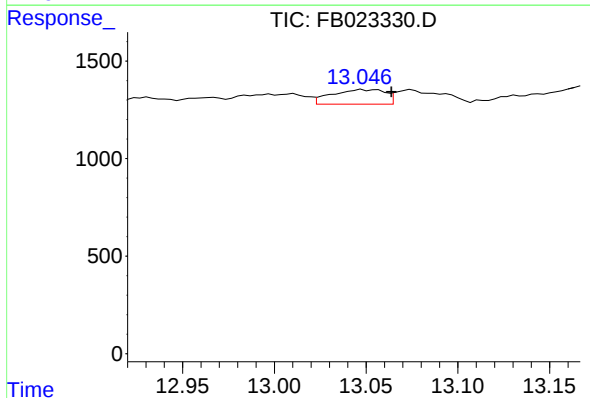


#7 Ethylbenzene

R.T.: 13.048 min
Delta R.T.: -0.015 min
Response: 1508
Conc: 0.04 ng/ml

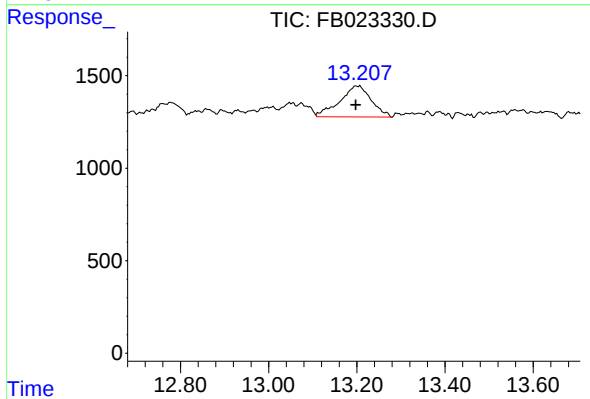

#8 m-Xylene


R.T.: 13.199 min
Delta R.T.: 0.002 min
Response: 8312
Conc: 0.24 ng/ml

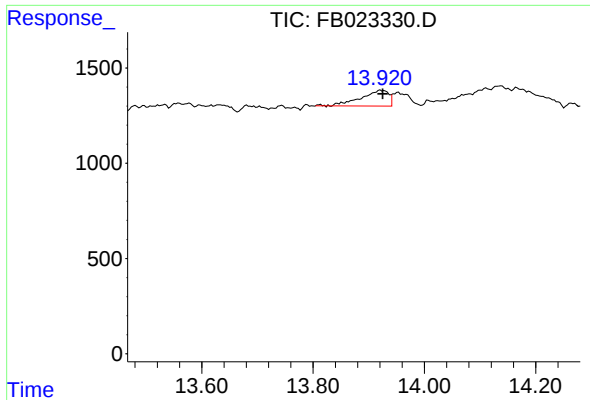

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: -0.003 min
Response: 2782
Conc: 0.08 ng/ml

Instrument :
FID_B
ClientSampleId :
K321-WC-01

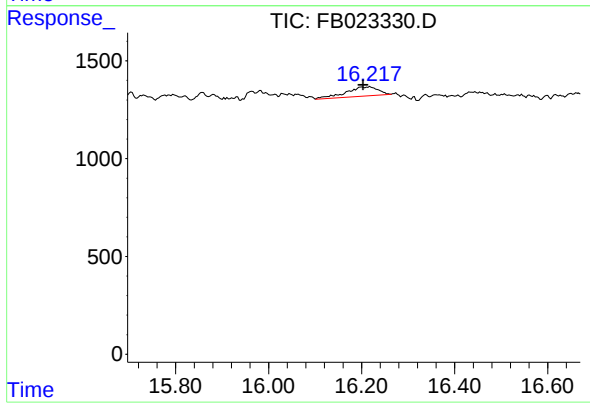

#10 1,2,4-Trimethylbenzene

R.T.: 16.218 min
Delta R.T.: 0.015 min
Response: 2190
Conc: 0.08 ng/ml