

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122719\
Data File : FB023331.D
Signal(s) : FID2B.CH
Acq On : 27 Dec 2019 17:27
Operator : DD/AJ
Sample : K6441-07
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
K321-WC-02

Integration File: Calibration.e
Quant Time: Dec 27 21:50:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
9) t O-Xylene	13.865	909	0.027 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122719\
Data File : FB023331.D
Signal(s) : FID2B.CH
Acq On : 27 Dec 2019 17:27
Operator : DD/AJ
Sample : K6441-07
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
K321-WC-02

Integration File: Calibration.e
Quant Time: Dec 27 21:50:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

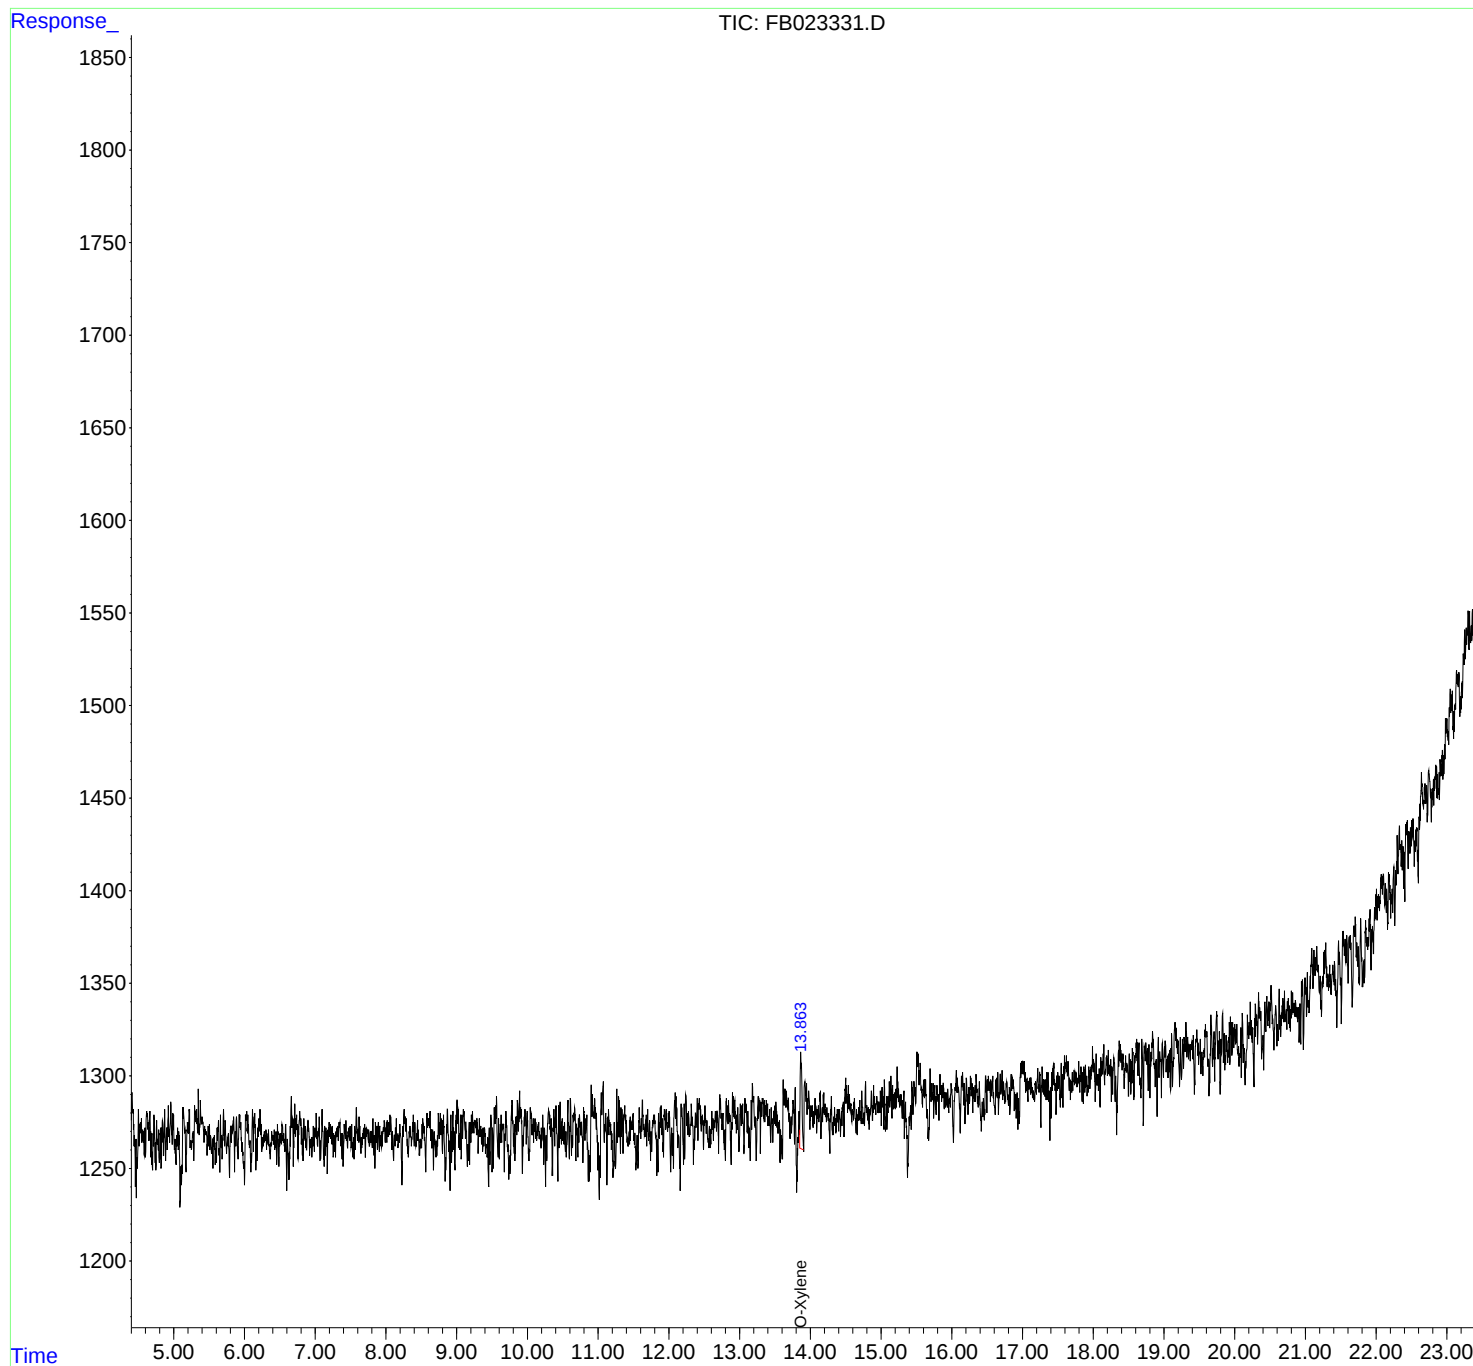


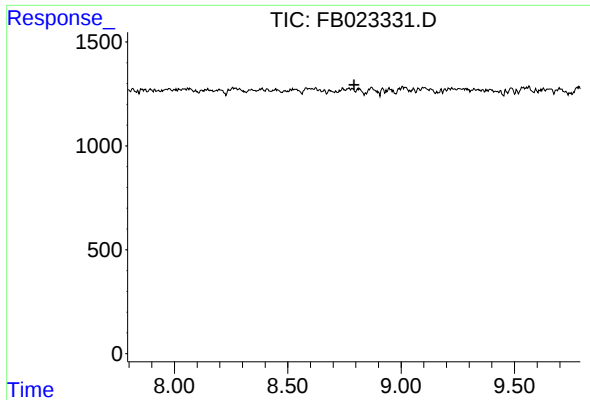

#5 AAA-TFT

R.T.: 0.000 min
Exp R.T. : 8.793 min
Response: 0
Conc: N.D.

Instrument :
FID_B
ClientSampleId :
K321-WC-02

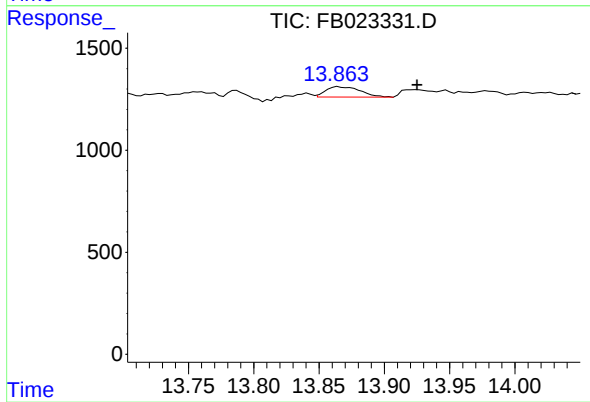

#9 O-Xylene

R.T.: 13.865 min
Delta R.T.: -0.060 min
Response: 909
Conc: 0.03 ng/ml