

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122719\
 Data File : FB023333.D
 Signal(s) : FID2B.CH
 Acq On : 27 Dec 2019 18:28
 Operator : DD/AJ
 Sample : K6114-03
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 27 21:50:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	405153	17.085 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.672	3328	0.108 ng/ml
2) t 2,2,4-Trimethylpentane	7.402	2690	0.081 ng/ml
3) t n-Heptane	7.749	468	0.014 ng/ml
4) t Benzene	7.899	5150	0.129 ng/ml
6) t Toluene	10.632	12147	0.315 ng/ml
7) t Ethylbenzene	13.055	8563	0.236 ng/ml
8) t m-Xylene	13.203	23565	0.679 ng/ml
9) t O-Xylene	13.934	21013	0.624 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	64979	2.316 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122719\
Data File : FB023333.D
Signal(s) : FID2B.CH
Acq On : 27 Dec 2019 18:28
Operator : DD/AJ
Sample : K6114-03
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 27 21:50:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

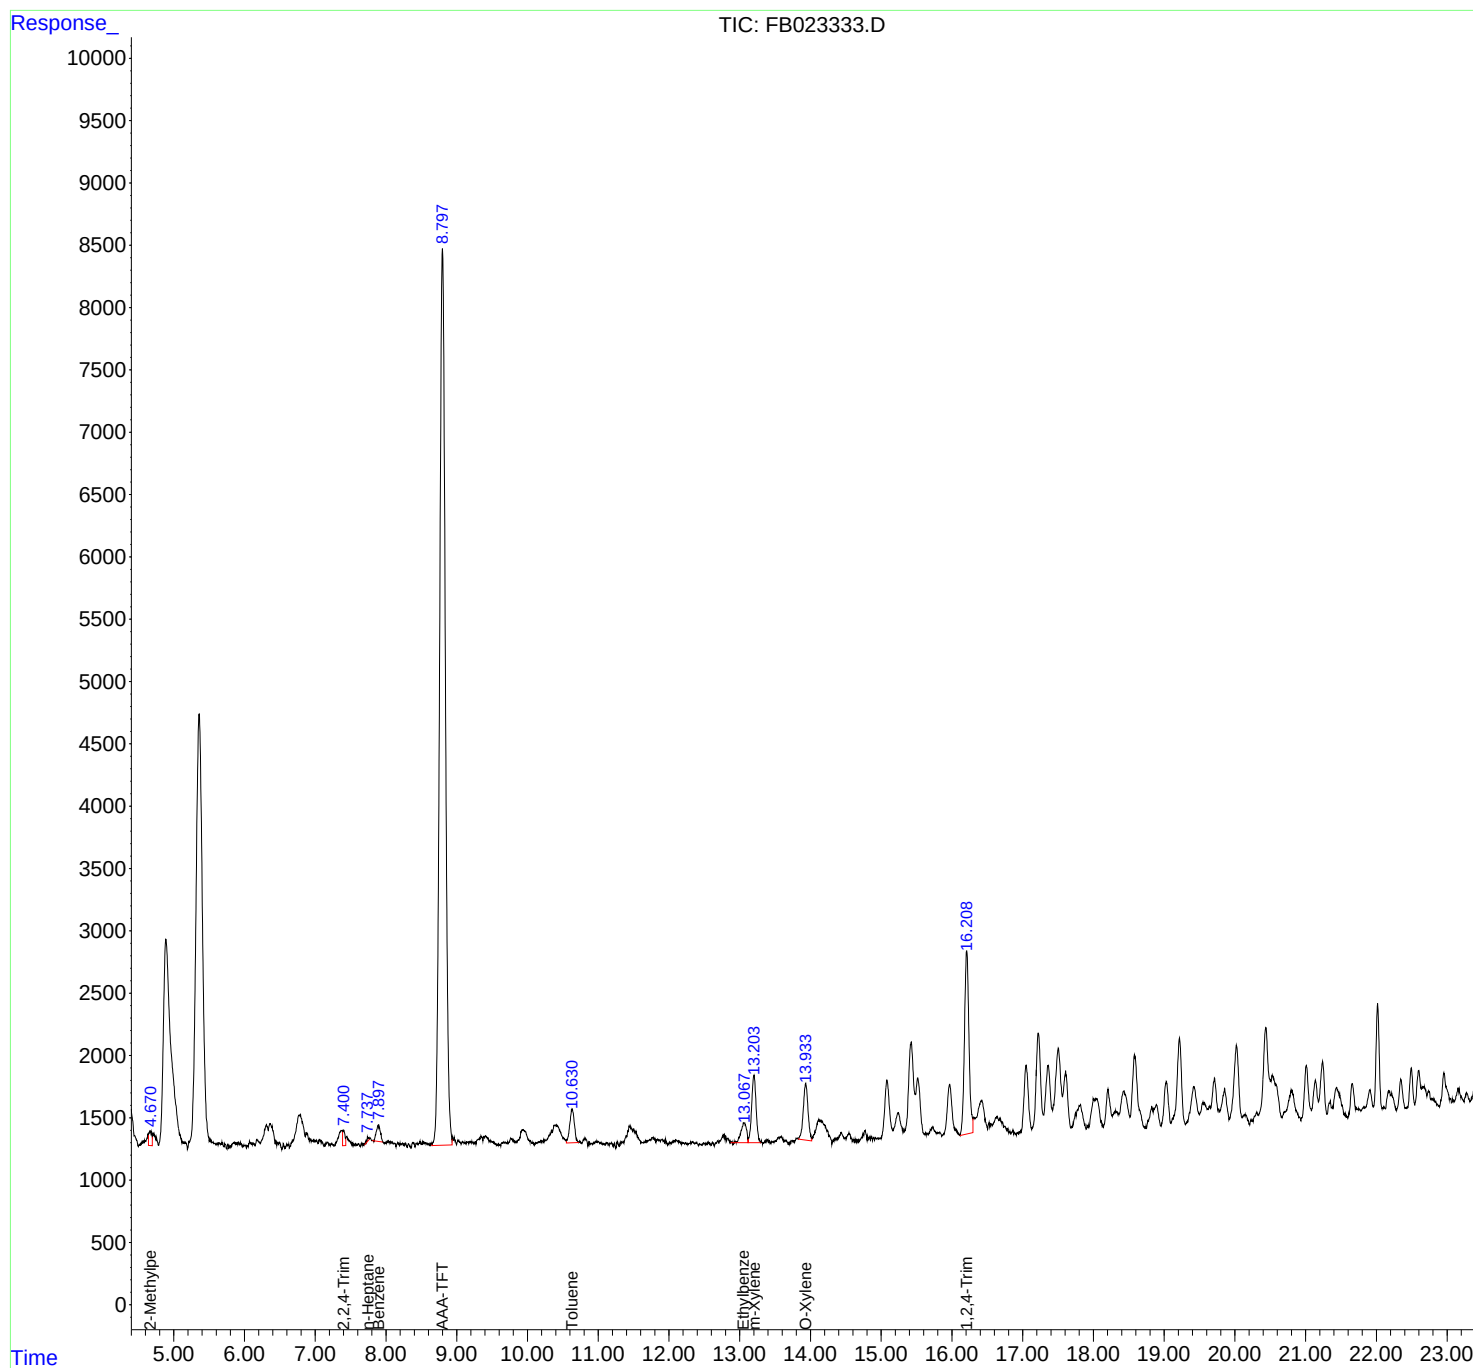


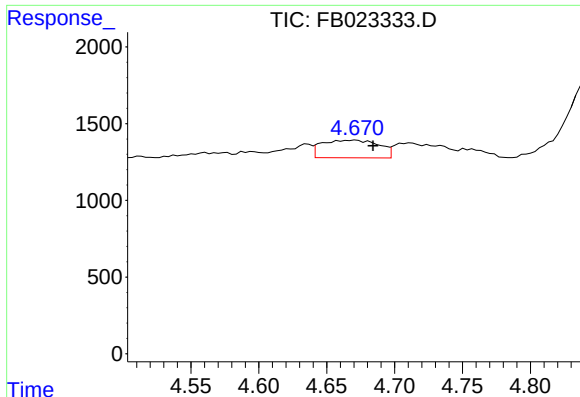

#1 2-Methylpentane


R.T.: 4.672 min
Delta R.T.: -0.012 min
Response: 3328
Conc: 0.11 ng/ml

Instrument :
FID_B
ClientSampleId :

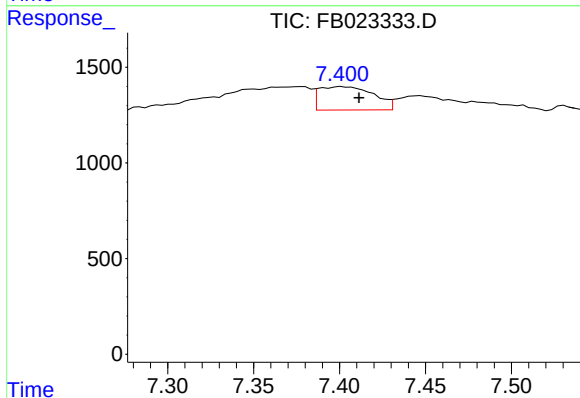


#2 2,2,4-Trimethylpentane

R.T.: 7.402 min
Delta R.T.: -0.010 min
Response: 2690
Conc: 0.08 ng/ml

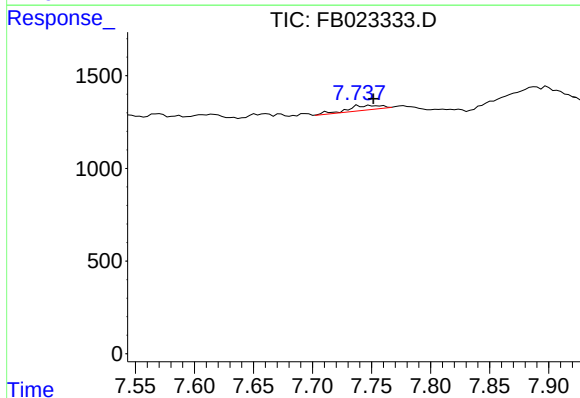


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.003 min
Response: 468
Conc: 0.01 ng/ml

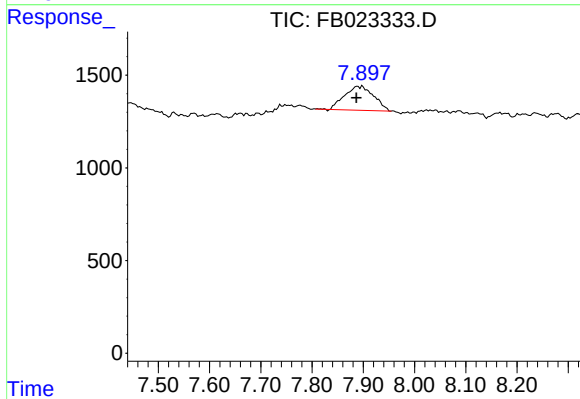

#4 Benzene


R.T.: 7.899 min
Delta R.T.: 0.012 min
Response: 5150
Conc: 0.13 ng/ml

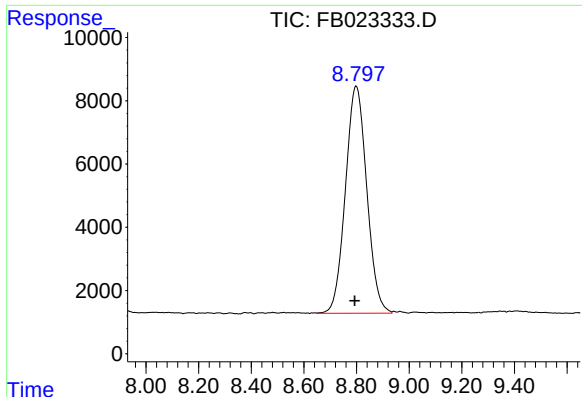

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.006 min
Response: 405153
Conc: 17.09 ng/ml

Instrument :
FID_B
ClientSampleId :

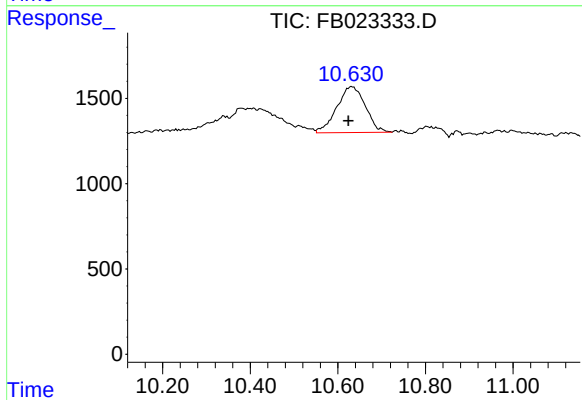


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.008 min
Response: 12147
Conc: 0.32 ng/ml

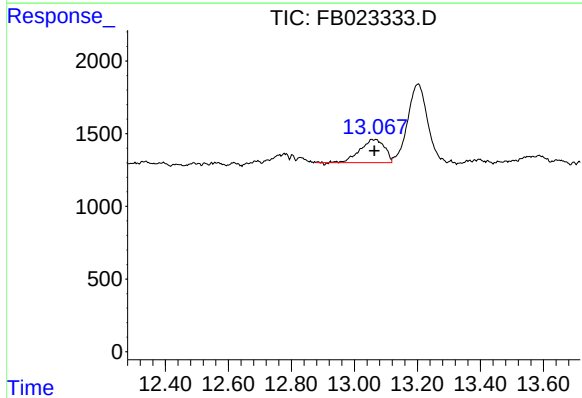


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.008 min
Response: 8563
Conc: 0.24 ng/ml

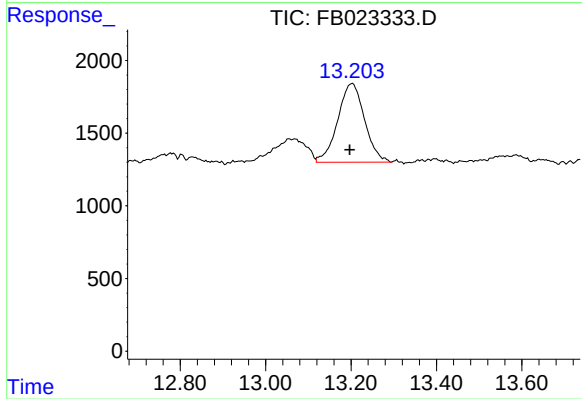

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: 0.006 min
Response: 23565
Conc: 0.68 ng/ml

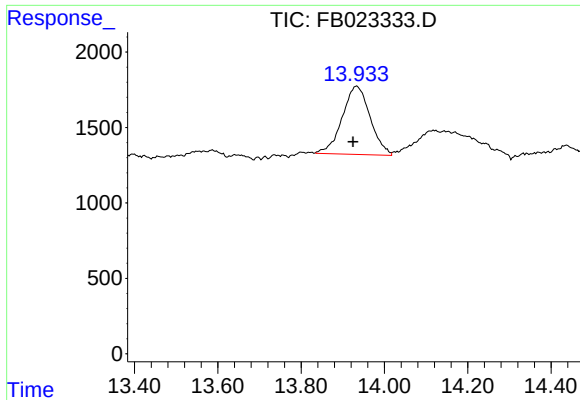

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.009 min
Response: 21013
Conc: 0.62 ng/ml

Instrument :
FID_B
ClientSampleId :

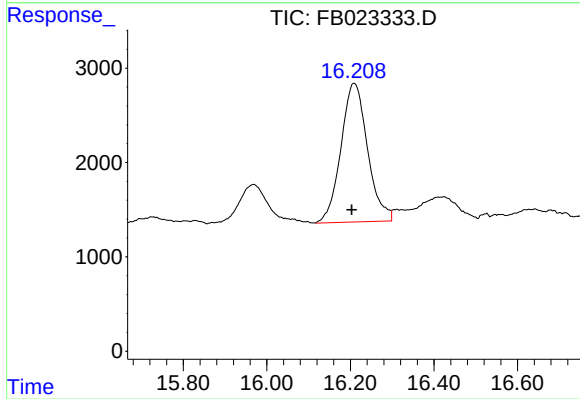

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.006 min
Response: 64979
Conc: 2.32 ng/ml