

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122719\
 Data File : FB023335.D
 Signal(s) : FID2B.CH
 Acq On : 27 Dec 2019 19:29
 Operator : DD/AJ
 Sample : K6456-06
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Dec 27 21:50:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	395780	16.690 ng/ml
Target Compounds			
6) t Toluene	10.627	2318	0.060 ng/ml
9) t O-Xylene	13.939	1639	0.049 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	2310	0.082 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122719\
Data File : FB023335.D
Signal(s) : FID2B.CH
Acq On : 27 Dec 2019 19:29
Operator : DD/AJ
Sample : K6456-06
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Dec 27 21:50:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

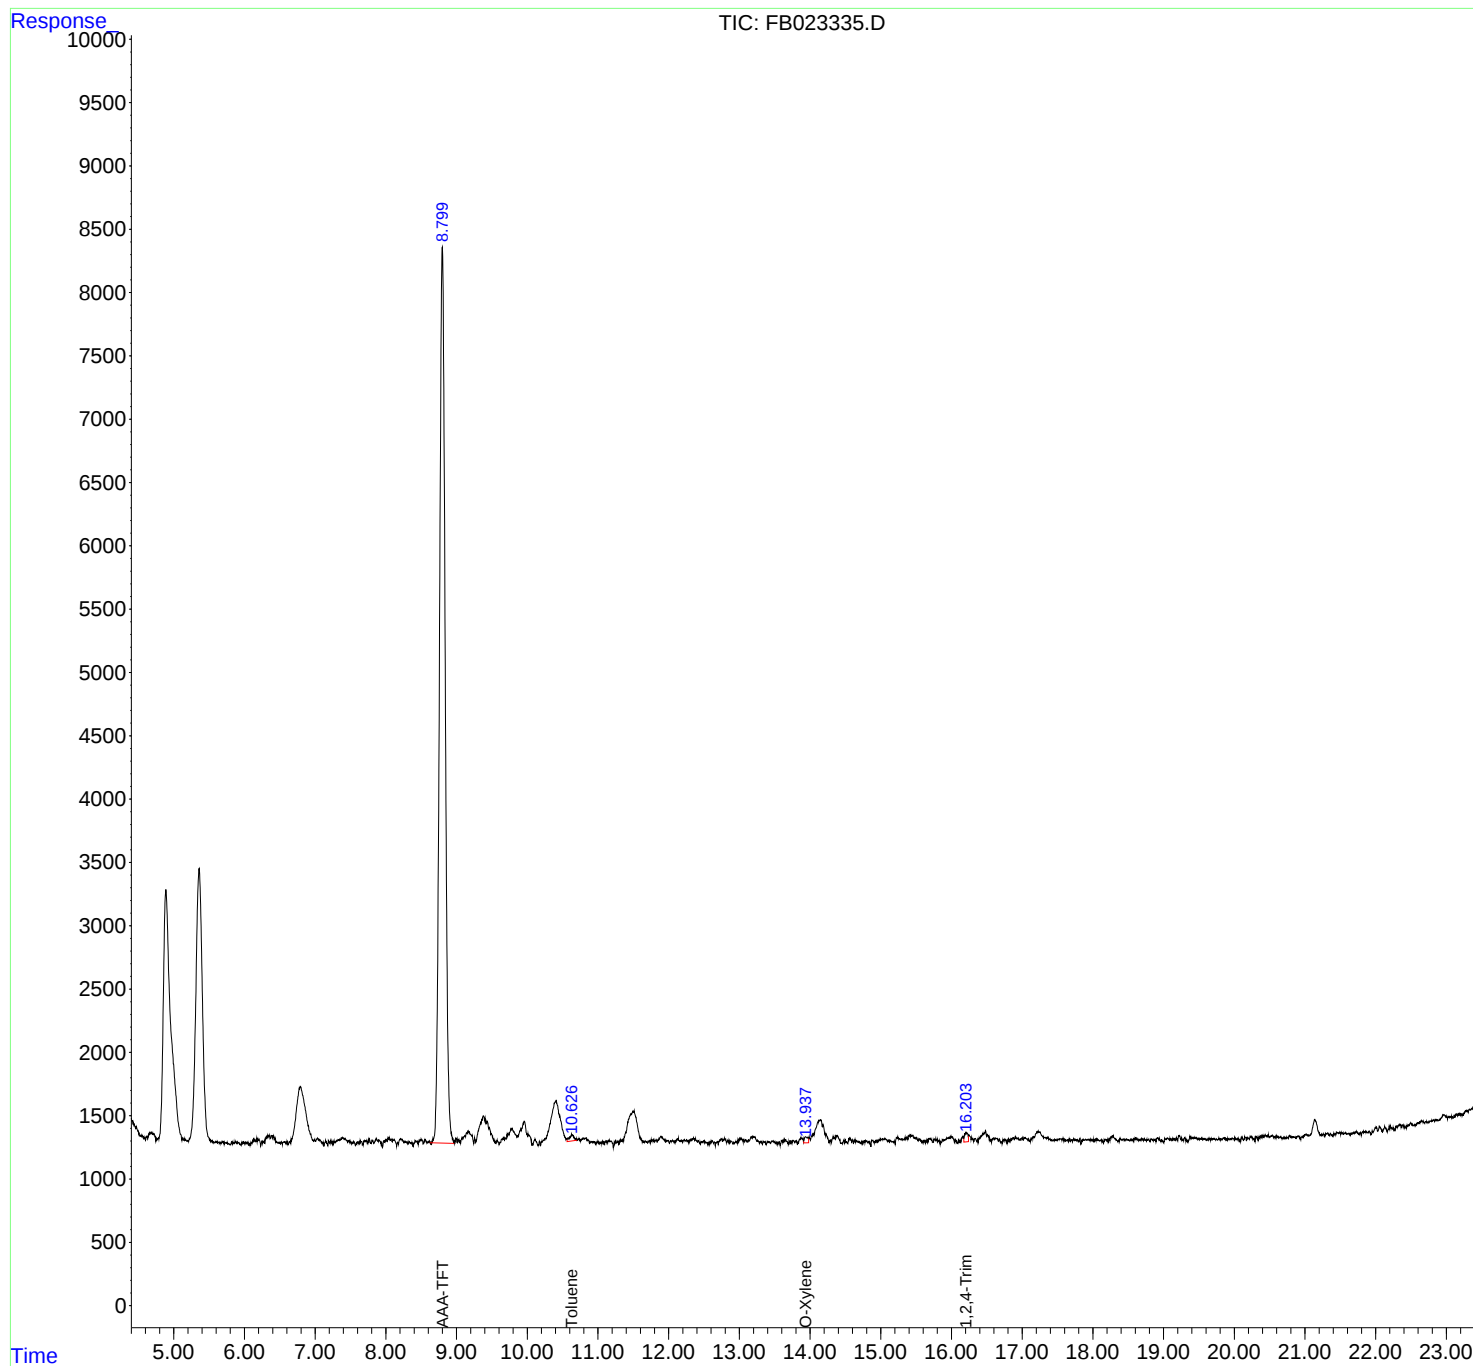


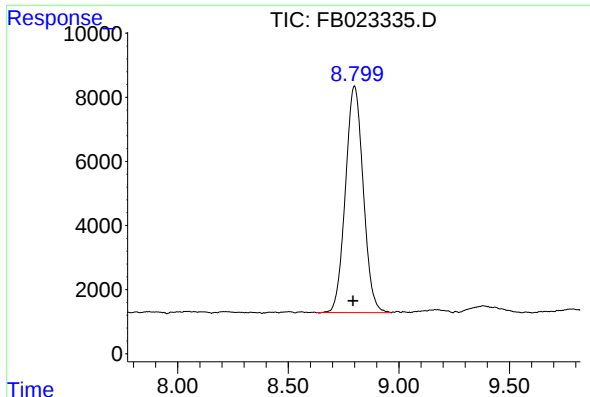

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.007 min
Response: 395780
Conc: 16.69 ng/ml

Instrument :
FID_B
ClientSampleId :

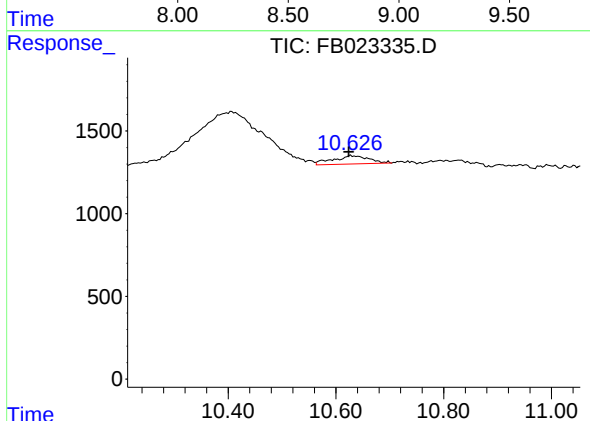


#6 Toluene

R.T.: 10.627 min
Delta R.T.: 0.004 min
Response: 2318
Conc: 0.06 ng/ml

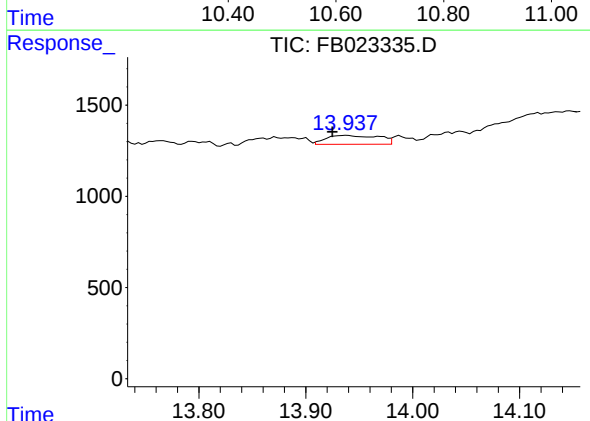

#9 O-Xylene

R.T.: 13.939 min
Delta R.T.: 0.014 min
Response: 1639
Conc: 0.05 ng/ml

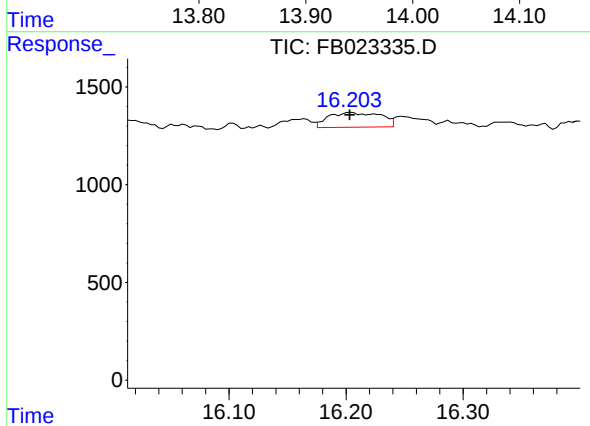

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: 0.001 min
Response: 2310
Conc: 0.08 ng/ml