

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122719\
 Data File : FF006097.D
 Signal(s) : FID2B.ch
 Acq On : 27 Dec 2019 17:04
 Operator : DD\AJ
 Sample : K6437-05
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 GP-3-(1-3)

Integration File: autoint1.e
 Quant Time: Dec 27 22:35:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
 Quant Title :
 QLast Update : Fri Dec 06 13:20:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.635	1925244	13.252 ug/ml
Target Compounds			
4) N-TETRADECANE	8.260	470090	2.772 ug/ml
7) N-EICOSANE	12.602	1435993	8.314 ug/ml
8) N-DOCOSANE	13.762	87168	0.512 ug/ml
10) N-TETRACOSANE	14.813	783316	4.693 ug/ml
11) N-HEXACOSANE	15.857	159029	0.987 ug/ml
12) N-OCTACOSANE	16.805	468099	3.051 ug/ml
13) N-TRIACONTANE	17.688	618768	4.265 ug/ml
14) N-DOTRIACONTANE	18.516	511793	3.686 ug/ml
15) N-TETRATRIACONTANE	19.307	425936	3.247 ug/ml
16) N-HEXATRIACONTANE	20.040	324770	2.602 ug/ml
17) N-OCTATRIACONTANE	20.765	460557	3.924 ug/ml
18) N-TETRACONTANE	21.648	415314	3.332 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122719\
Data File : FF006097.D
Signal(s) : FID2B.ch
Acq On : 27 Dec 2019 17:04
Operator : DD\AJ
Sample : K6437-05
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
GP-3-(1-3)

Integration File: autoint1.e
Quant Time: Dec 27 22:35:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
Quant Title :
QLast Update : Fri Dec 06 13:20:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

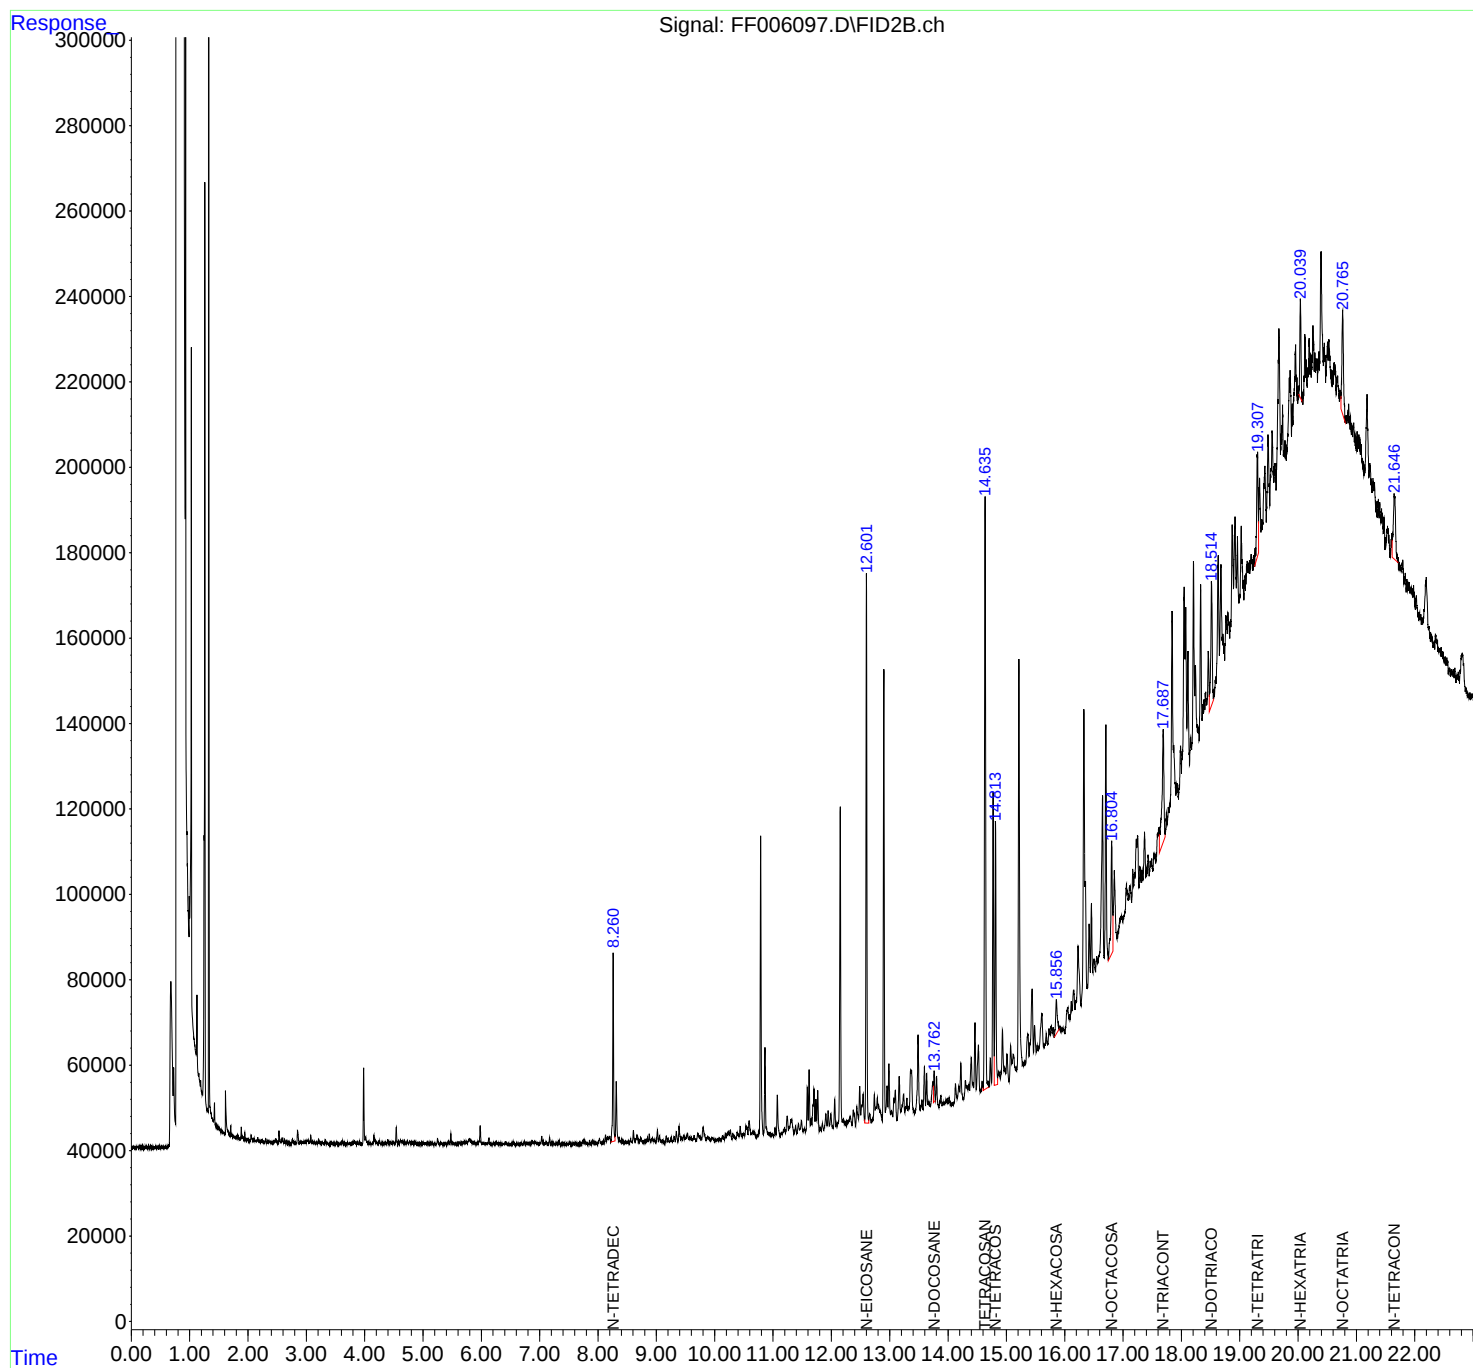


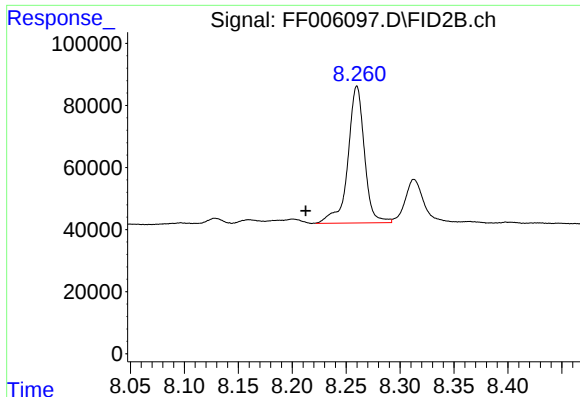

#4 N-TETRADECANE


R.T.: 8.260 min
Delta R.T.: 0.047 min
Response: 470090
Conc: 2.77 ug/ml

Instrument :
FID_B
ClientSampleId :
GP-3-(1-3)

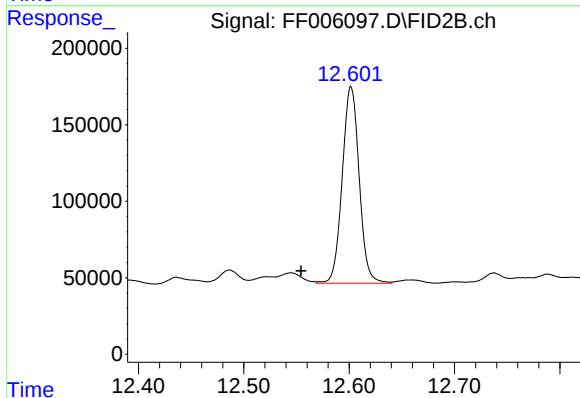


#7 N-EICOSANE

R.T.: 12.602 min
Delta R.T.: 0.047 min
Response: 1435993
Conc: 8.31 ug/ml

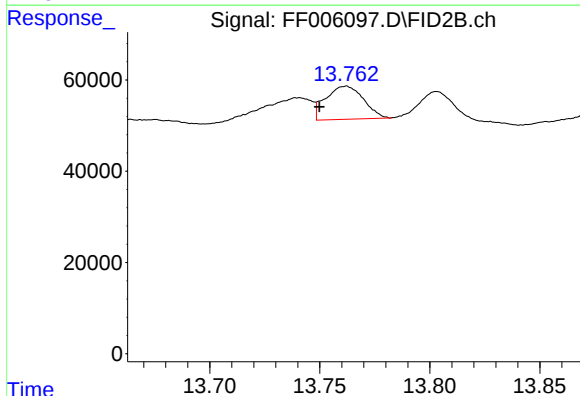


#8 N-DOCOSANE

R.T.: 13.762 min
Delta R.T.: 0.012 min
Response: 87168
Conc: 0.51 ug/ml

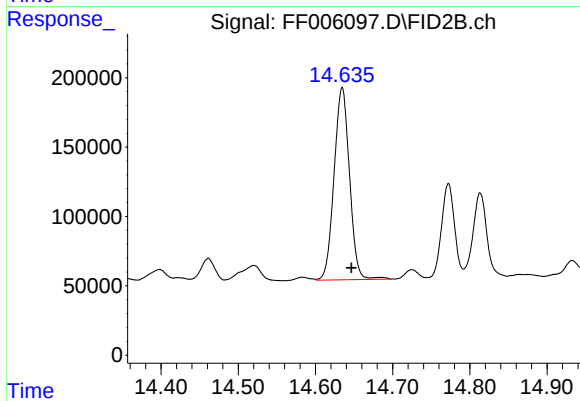

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.635 min
Delta R.T.: -0.012 min
Response: 1925244
Conc: 13.25 ug/ml

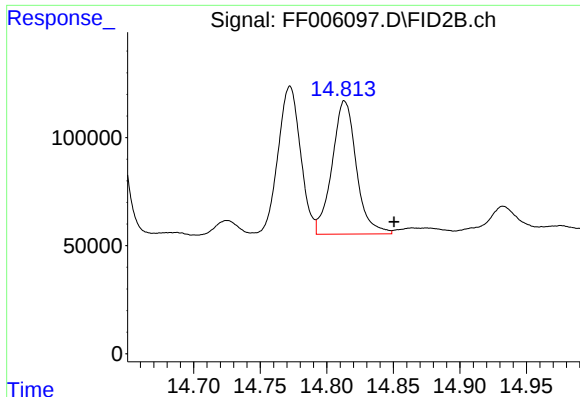

#10 N-TETRACOSANE


R.T.: 14.813 min
Delta R.T.: -0.037 min
Response: 783316
Conc: 4.69 ug/ml

Instrument :
FID_B
ClientSampleId :
GP-3-(1-3)

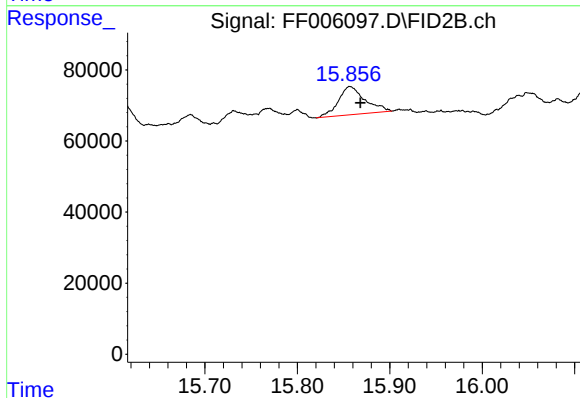


#11 N-HEXACOSANE

R.T.: 15.857 min
Delta R.T.: -0.011 min
Response: 159029
Conc: 0.99 ug/ml

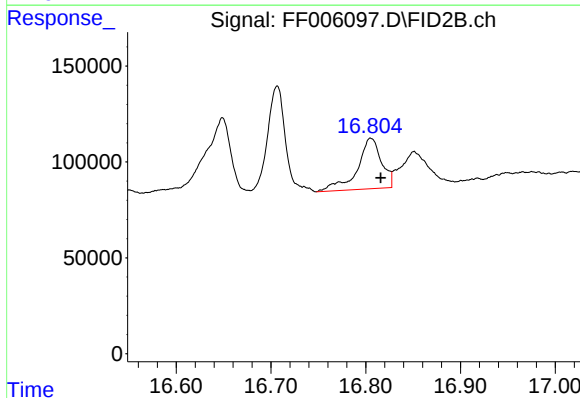


#12 N-OCTACOSANE

R.T.: 16.805 min
Delta R.T.: -0.010 min
Response: 468099
Conc: 3.05 ug/ml

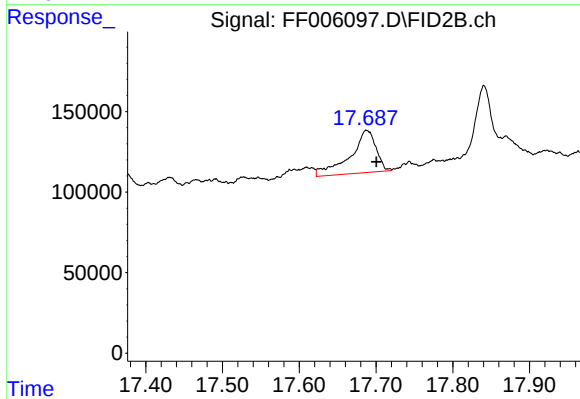

#13 N-TRIACONTANE


R.T.: 17.688 min
Delta R.T.: -0.013 min
Response: 618768
Conc: 4.27 ug/ml

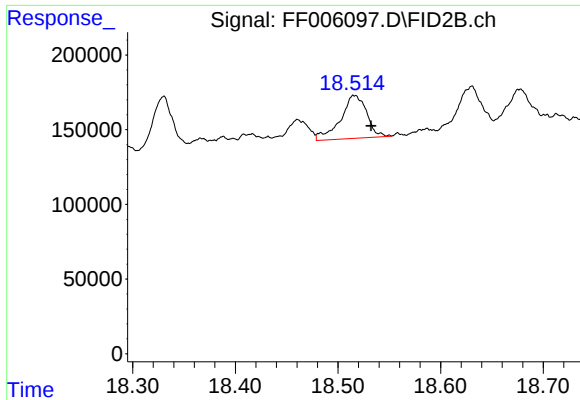

#14 N-DOTRIACONTANE


R.T.: 18.516 min
Delta R.T.: -0.016 min
Response: 511793
Conc: 3.69 ug/ml

Instrument :
FID_B
ClientSampleId :
GP-3-(1-3)

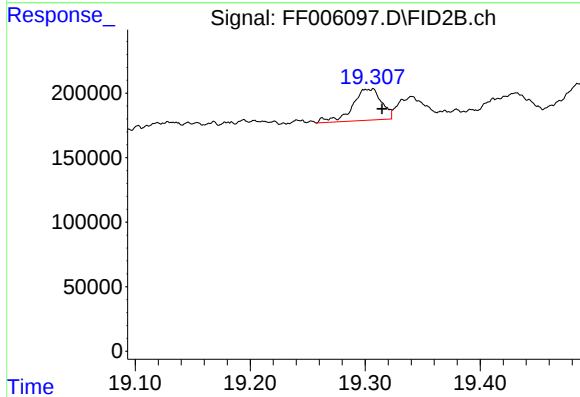


#15 N-TETRATRIACONTANE

R.T.: 19.307 min
Delta R.T.: -0.008 min
Response: 425936
Conc: 3.25 ug/ml

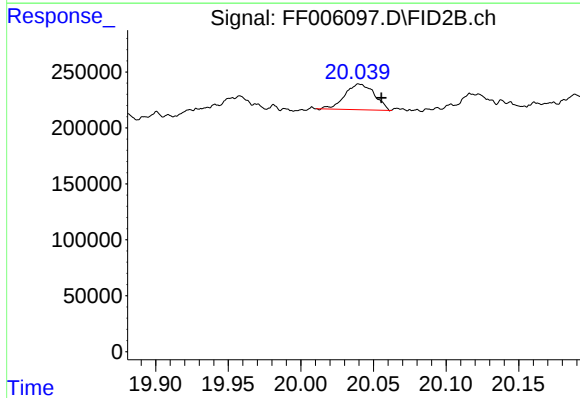


#16 N-HEXATRIACONTANE

R.T.: 20.040 min
Delta R.T.: -0.015 min
Response: 324770
Conc: 2.60 ug/ml

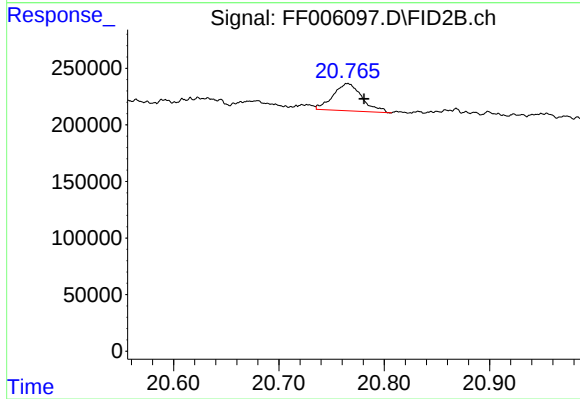

#17 N-OCTATRIACONTANE

R.T.: 20.765 min
Delta R.T.: -0.016 min
Response: 460557
Conc: 3.92 ug/ml

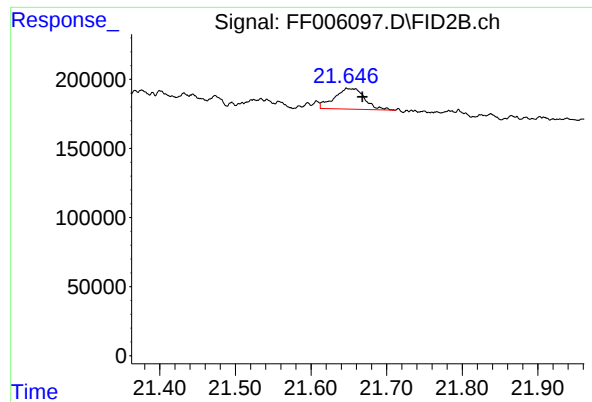

#18 N-TETRACONTANE

R.T.: 21.648 min
Delta R.T.: -0.021 min
Response: 415314
Conc: 3.33 ug/ml

Instrument :
FID_B
ClientSampleId :
GP-3-(1-3)