

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122719\
 Data File : FF006100.D
 Signal(s) : FID2B.ch
 Acq On : 27 Dec 2019 18:36
 Operator : DD\AJ
 Sample : K6442-06
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 K615-WC-1

Integration File: autoint1.e
 Quant Time: Dec 27 22:36:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
 Quant Title :
 QLast Update : Fri Dec 06 13:20:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.634	1618487	11.140 ug/ml
Target Compounds			
4) N-TETRADECANE	8.261	298828	1.762 ug/ml
7) N-EICOSANE	12.602	310197	1.796 ug/ml
10) N-TETRACOSANE	14.814	206585	1.238 ug/ml
11) N-HEXACOSANE	15.855	133708	0.830 ug/ml
12) N-OCTACOSANE	16.803	272454	1.776 ug/ml
13) N-TRIACONTANE	17.685	348523	2.402 ug/ml
14) N-DOTRIACONTANE	18.512	308192	2.219 ug/ml
15) N-TETRATRIACONTANE	19.297	85812	0.654 ug/ml
16) N-HEXATRIACONTANE	20.002f	65958	0.528 ug/ml
17) N-OCTATRIACONTANE	20.762	288716	2.460 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122719\
Data File : FF006100.D
Signal(s) : FID2B.ch
Acq On : 27 Dec 2019 18:36
Operator : DD\AJ
Sample : K6442-06
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
K615-WC-1

Integration File: autoint1.e
Quant Time: Dec 27 22:36:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
Quant Title :
QLast Update : Fri Dec 06 13:20:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

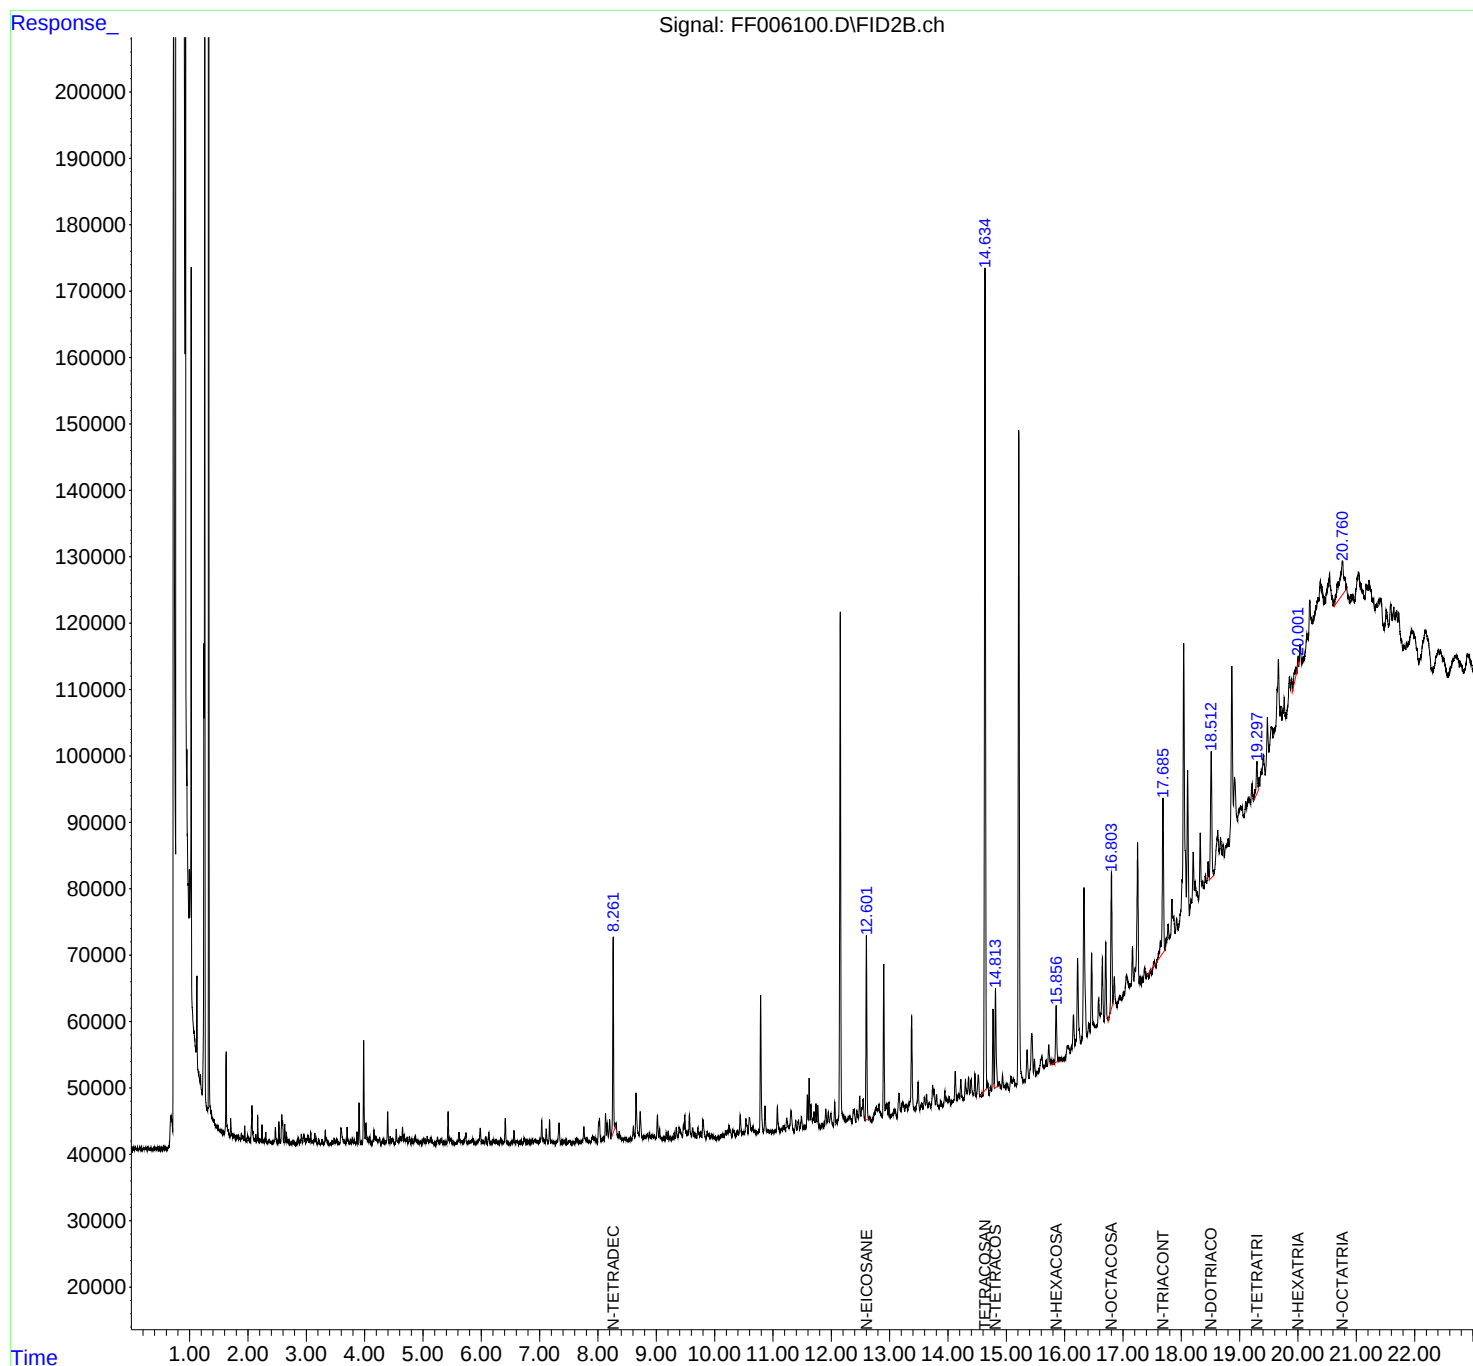


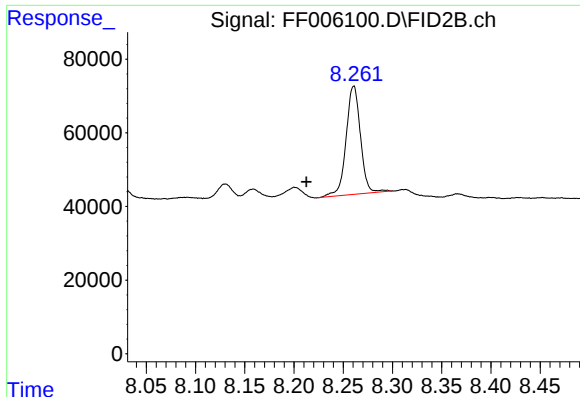

#4 N-TETRADECANE


R.T.: 8.261 min
Delta R.T.: 0.048 min
Response: 298828
Conc: 1.76 ug/ml

Instrument :
FID_B
ClientSampleId :
K615-WC-1

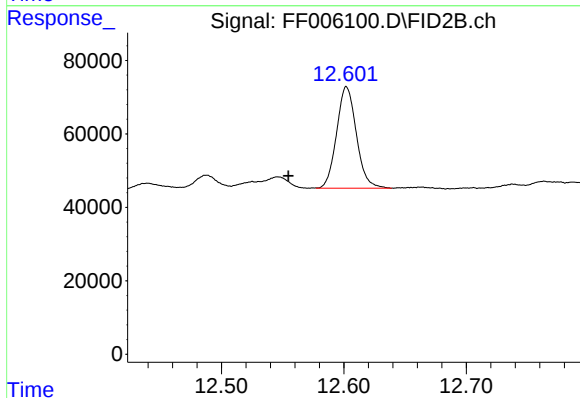


#7 N-EICOSANE

R.T.: 12.602 min
Delta R.T.: 0.048 min
Response: 310197
Conc: 1.80 ug/ml

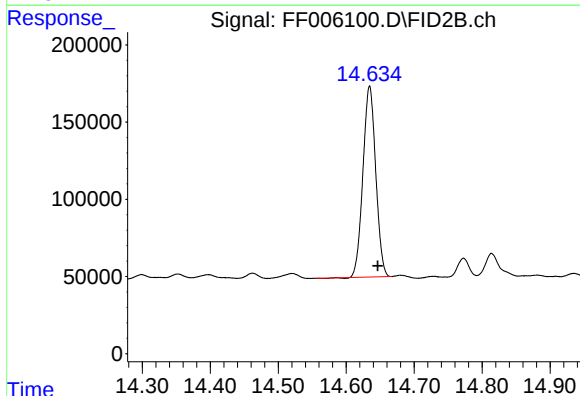


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.634 min
Delta R.T.: -0.012 min
Response: 1618487
Conc: 11.14 ug/ml

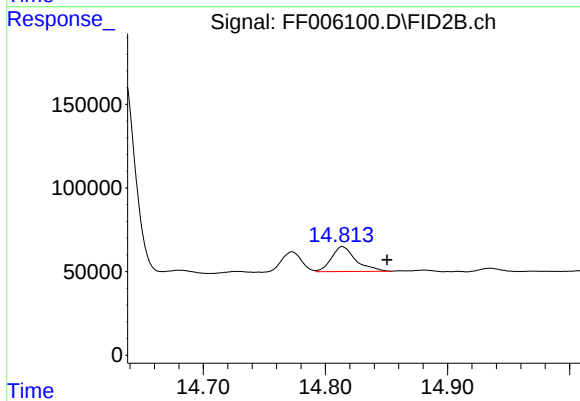

#10 N-TETRACOSANE


R.T.: 14.814 min
Delta R.T.: -0.037 min
Response: 206585
Conc: 1.24 ug/ml

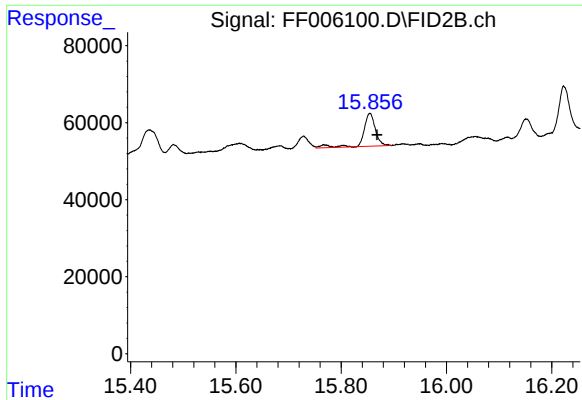

#11 N-HEXACOSANE


R.T.: 15.855 min
Delta R.T.: -0.014 min
Response: 133708
Conc: 0.83 ug/ml

Instrument :
FID_B
ClientSampleId :
K615-WC-1

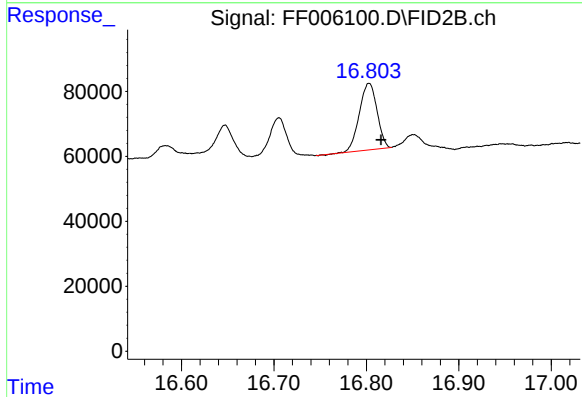


#12 N-OCTACOSANE

R.T.: 16.803 min
Delta R.T.: -0.013 min
Response: 272454
Conc: 1.78 ug/ml

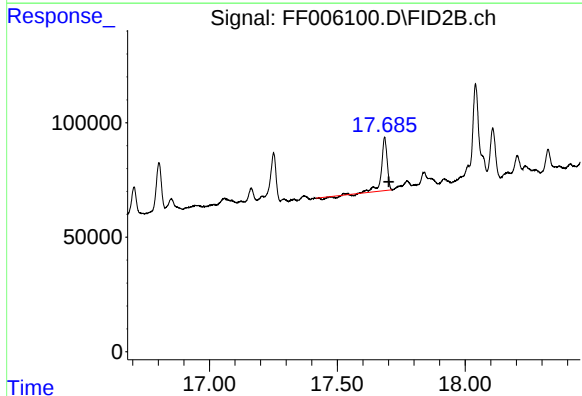


#13 N-TRIACONTANE

R.T.: 17.685 min
Delta R.T.: -0.016 min
Response: 348523
Conc: 2.40 ug/ml

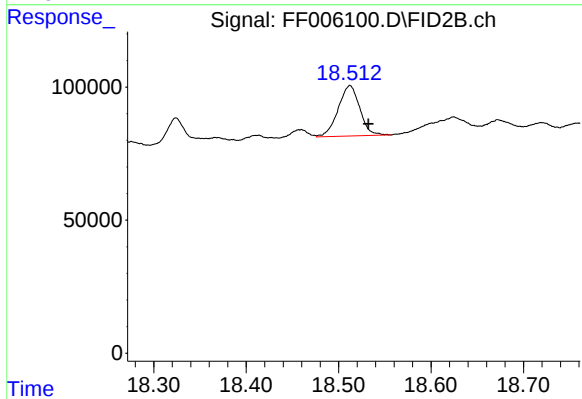

#14 N-DOTRIACONTANE


R.T.: 18.512 min
Delta R.T.: -0.020 min
Response: 308192
Conc: 2.22 ug/ml

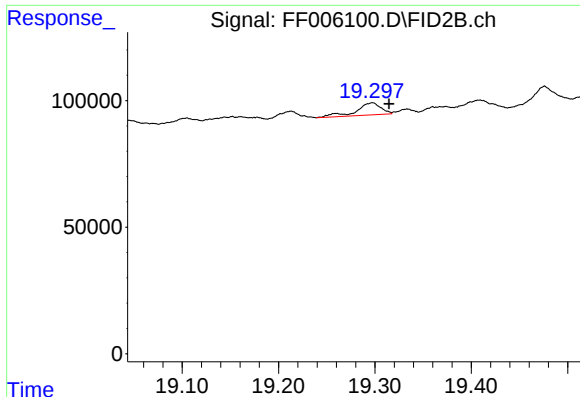

#15 N-TETRATRIACONTANE


R.T.: 19.297 min
Delta R.T.: -0.018 min
Response: 85812
Conc: 0.65 ug/ml

Instrument :
FID_B
ClientSampleId :
K615-WC-1

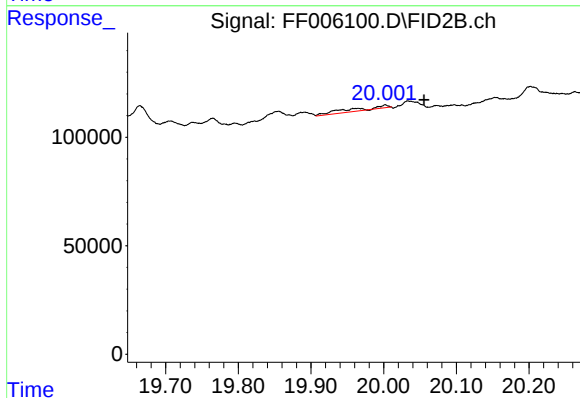

#16 N-HEXATRIACONTANE

R.T.: 20.002 min
Delta R.T.: -0.053 min
Response: 65958
Conc: 0.53 ug/ml

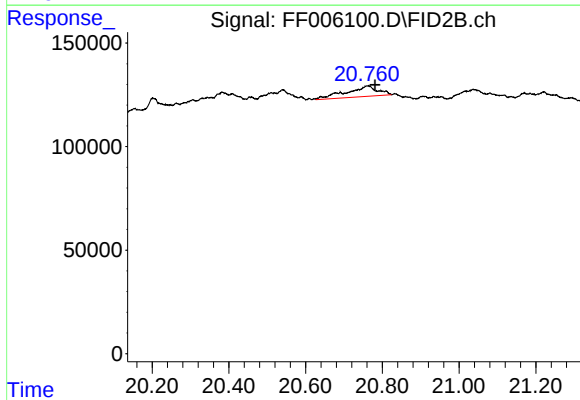

#17 N-OCTATRIACONTANE

R.T.: 20.762 min
Delta R.T.: -0.019 min
Response: 288716
Conc: 2.46 ug/ml