

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF122719\  
Data File : FF006101.D  
Signal(s) : FID2B.ch  
Acq On : 27 Dec 2019 19:06  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
I.BLK

Integration File: autoint1.e  
Quant Time: Dec 27 22:36:42 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF120719.M  
Quant Title :  
QLast Update : Fri Dec 06 13:20:24 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.635 | 2163412  | 14.891 ug/ml |
| Target Compounds              |        |          |              |
| 14) N-DOTRIACONTANE           | 18.513 | 117013   | 0.843 ug/ml  |
| 15) N-TETRATRIACONTANE        | 19.294 | 134466   | 1.025 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF122719\  
Data File : FF006101.D  
Signal(s) : FID2B.ch  
Acq On : 27 Dec 2019 19:06  
Operator : DD\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 52 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampled :  
I.BLK

Integration File: autoint1.e  
Quant Time: Dec 27 22:36:42 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF120719.M  
Quant Title :  
QLast Update : Fri Dec 06 13:20:24 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

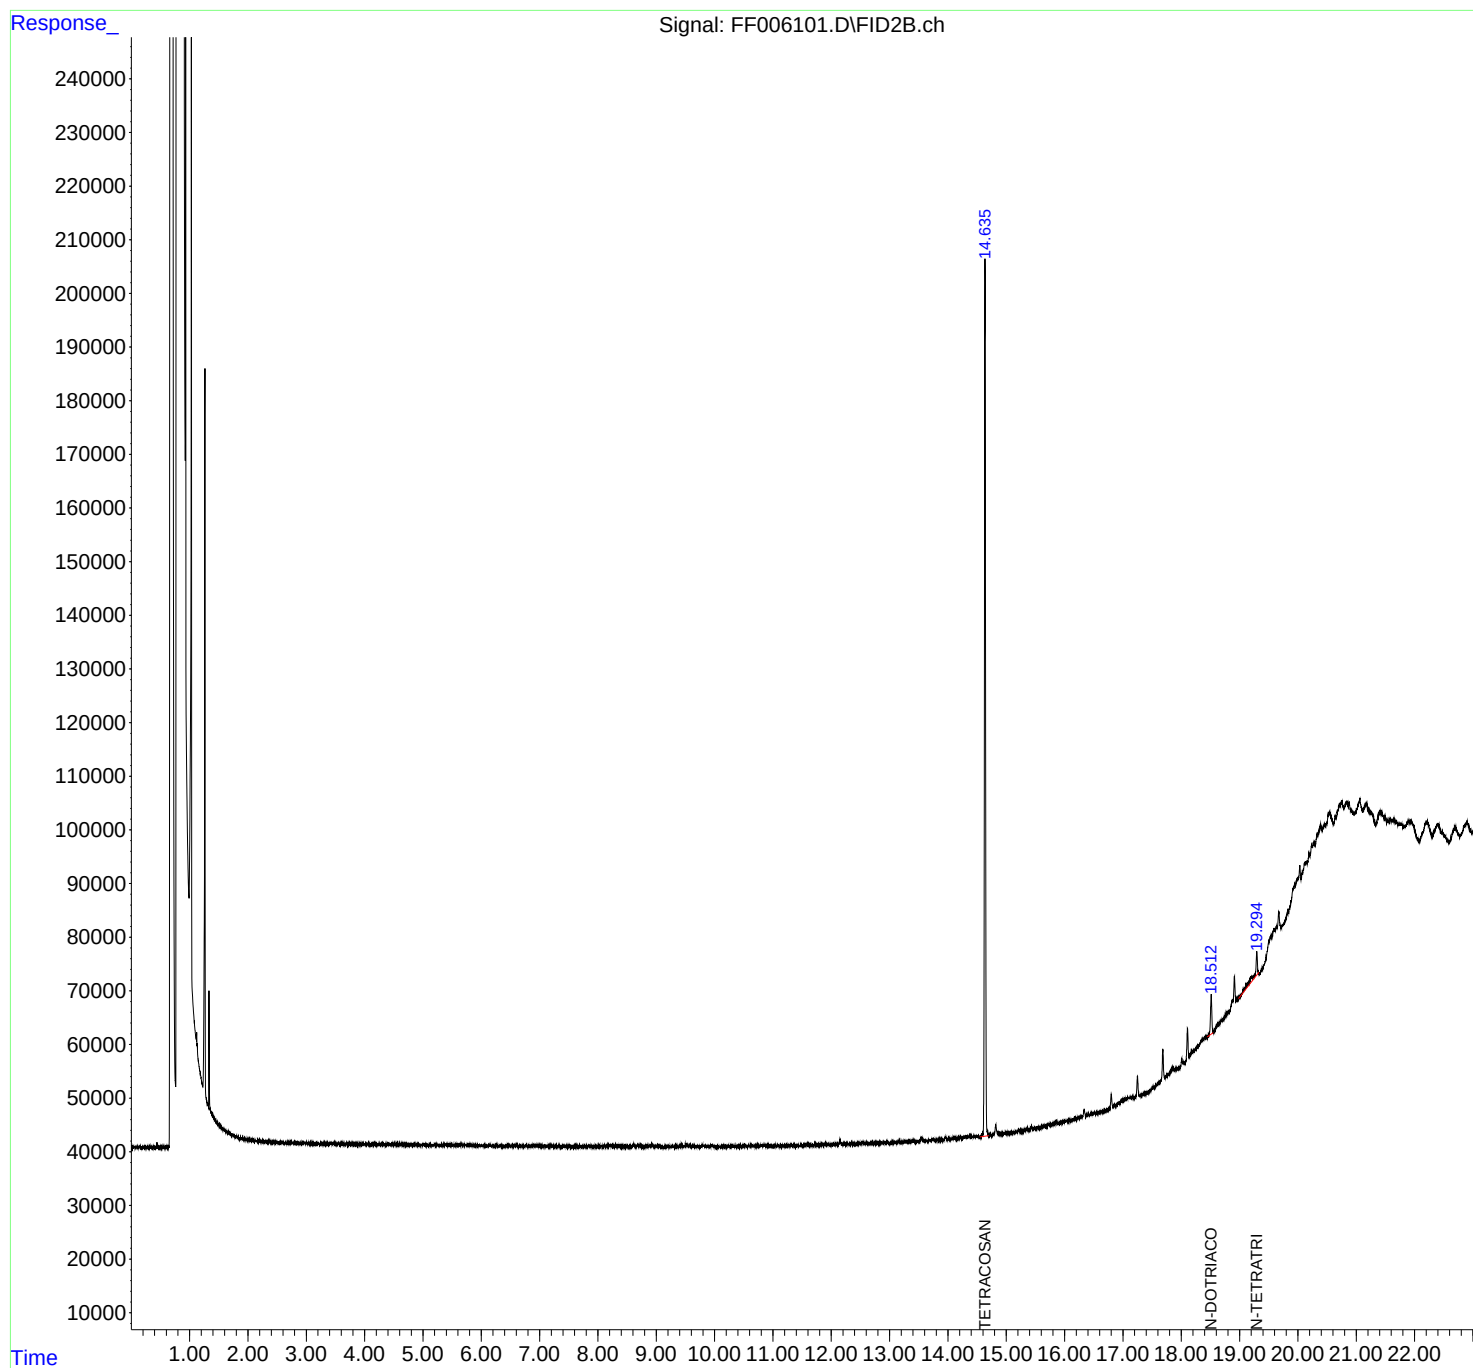


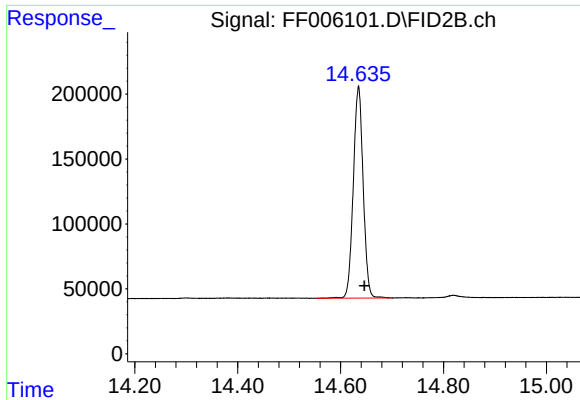

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.635 min  
Delta R.T.: -0.011 min  
Response: 2163412  
Conc: 14.89 ug/ml

Instrument :  
FID\_B  
ClientSampleId :  
I.BLK

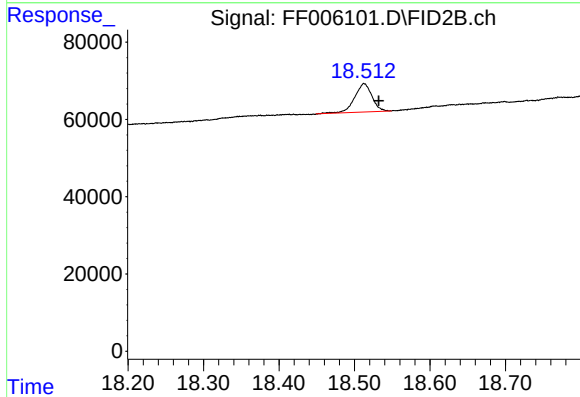

#14 N-DOTRIACONTANE

R.T.: 18.513 min  
Delta R.T.: -0.020 min  
Response: 117013  
Conc: 0.84 ug/ml

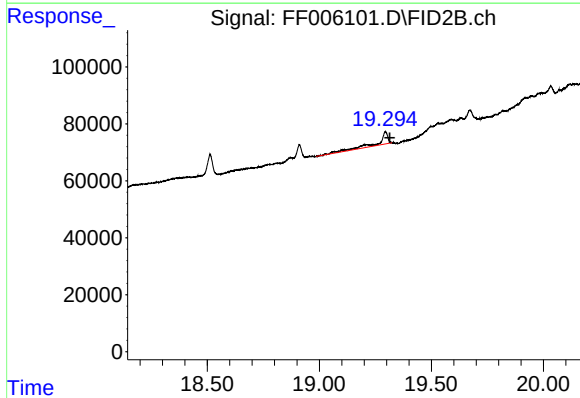

#15 N-TETRATRIACONTANE

R.T.: 19.294 min  
Delta R.T.: -0.020 min  
Response: 134466  
Conc: 1.03 ug/ml