

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122719\
 Data File : FF006104.D
 Signal(s) : FID2B.ch
 Acq On : 27 Dec 2019 20:38
 Operator : DD\AJ
 Sample : K6117-10 5X
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TR-05-122619

Integration File: autoint1.e
 Quant Time: Dec 27 22:37:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
 Quant Title :
 QLast Update : Fri Dec 06 13:20:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.633	492686	3.391 ug/ml
Target Compounds			
4) N-TETRADECANE	8.184	123106	0.726 ug/ml
7) N-EICOSANE	12.547	162471	0.941 ug/ml
8) N-DOCOSANE	13.765	344029	2.021 ug/ml
10) N-TETRACOSANE	14.815	925798	5.547 ug/ml
11) N-HEXACOSANE	15.858	126556	0.786 ug/ml
12) N-OCTACOSANE	16.807	404610	2.638 ug/ml
13) N-TRIACONTANE	17.686	287561	1.982 ug/ml
14) N-DOTRIACONTANE	18.512	183784	1.323 ug/ml
15) N-TETRATRIACONTANE	19.298	122721	0.936 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122719\
Data File : FF006104.D
Signal(s) : FID2B.ch
Acq On : 27 Dec 2019 20:38
Operator : DD\AJ
Sample : K6117-10 5X
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TR-05-122619

Integration File: autoint1.e
Quant Time: Dec 27 22:37:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
Quant Title :
QLast Update : Fri Dec 06 13:20:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

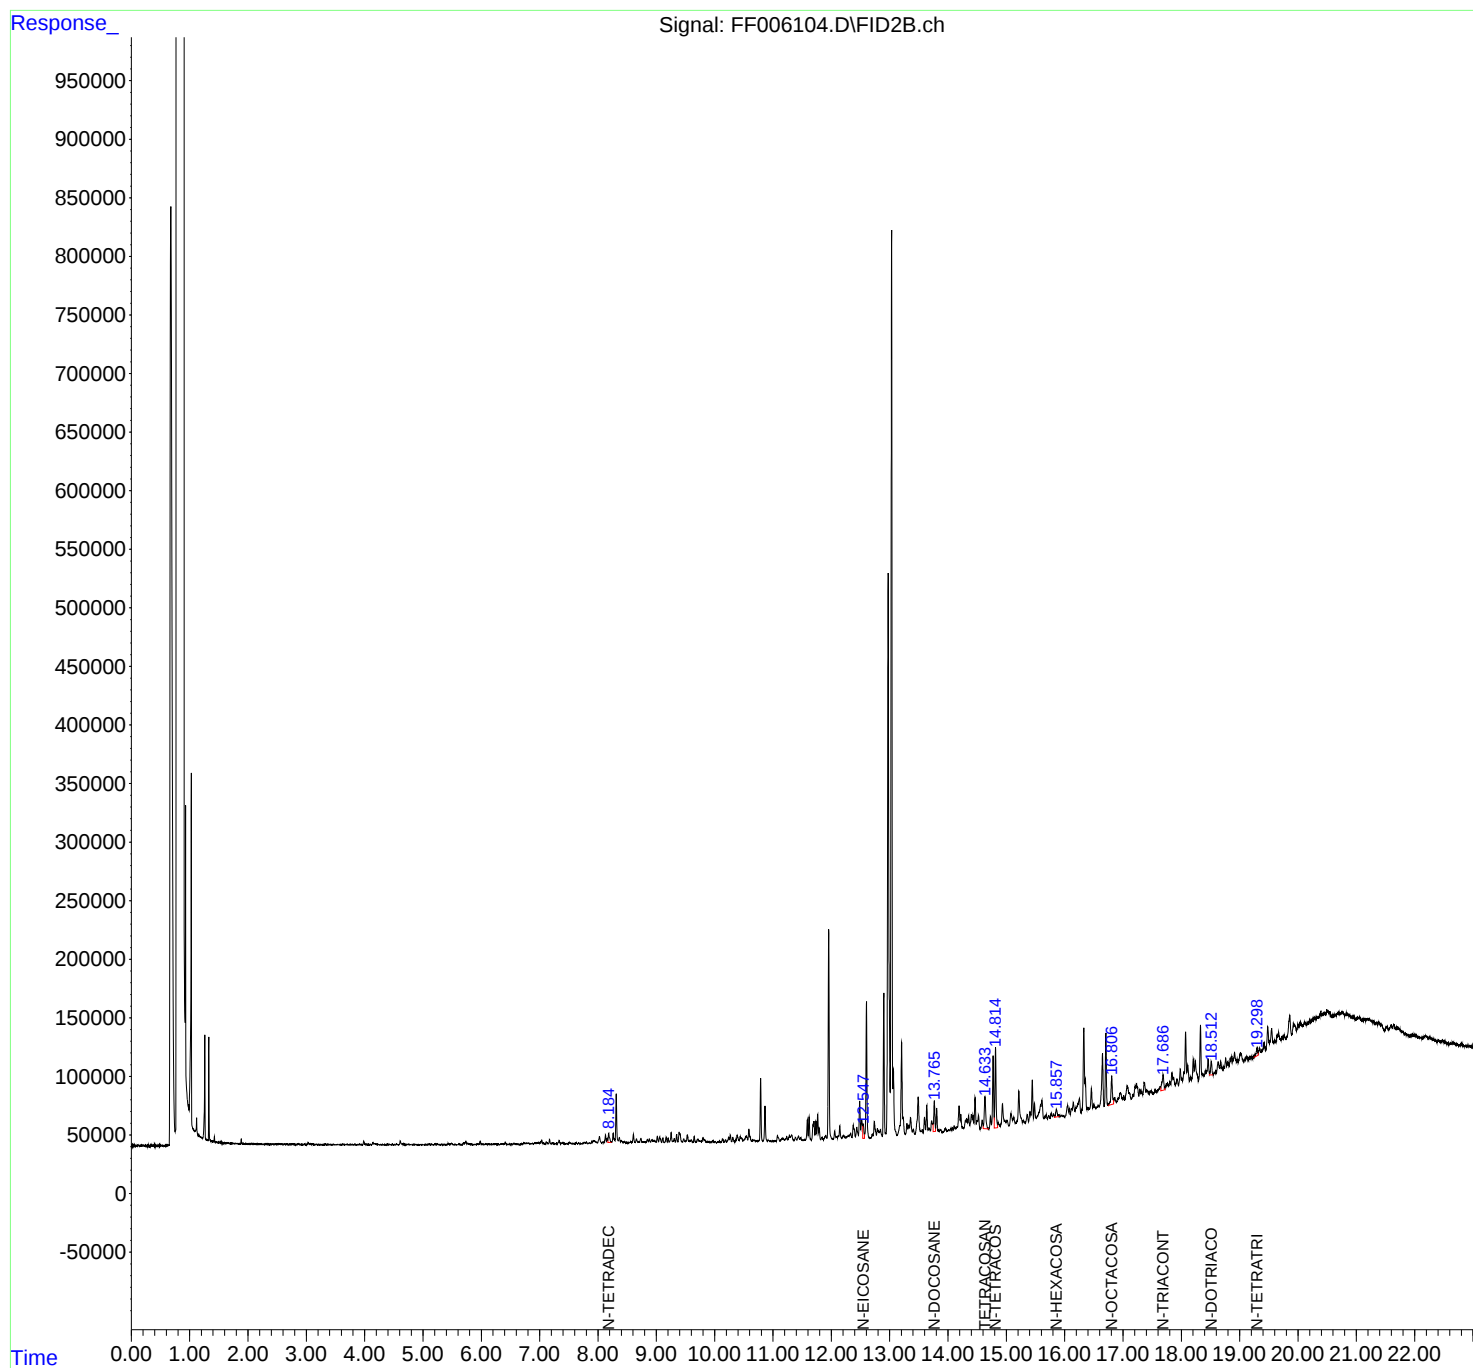


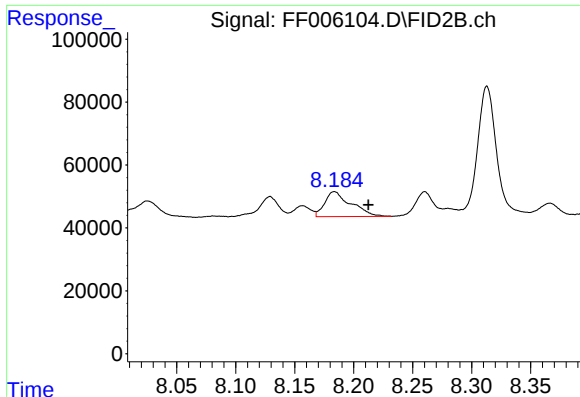

#4 N-TETRADECANE


R.T.: 8.184 min
Delta R.T.: -0.029 min
Response: 123106
Conc: 0.73 ug/ml

Instrument :
FID_B
ClientSampleId :
TR-05-122619

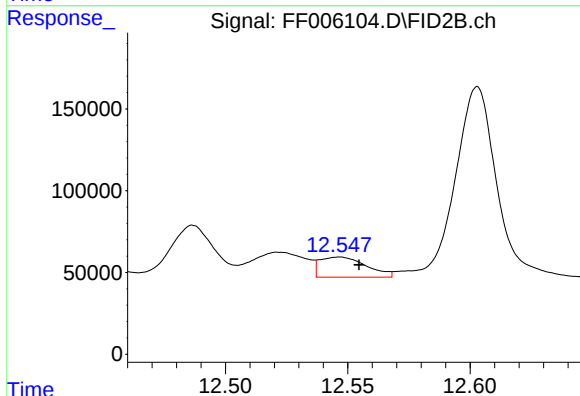


#7 N-EICOSANE

R.T.: 12.547 min
Delta R.T.: -0.008 min
Response: 162471
Conc: 0.94 ug/ml

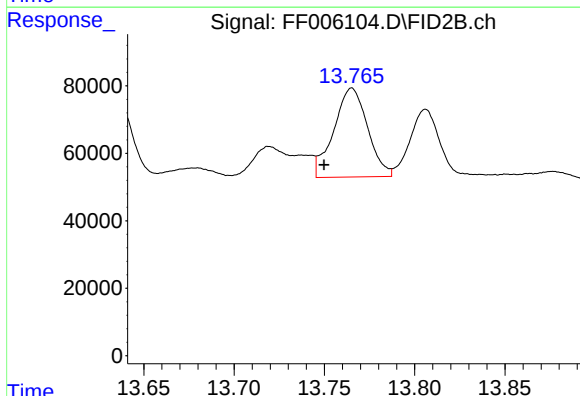


#8 N-DOCOSANE

R.T.: 13.765 min
Delta R.T.: 0.015 min
Response: 344029
Conc: 2.02 ug/ml

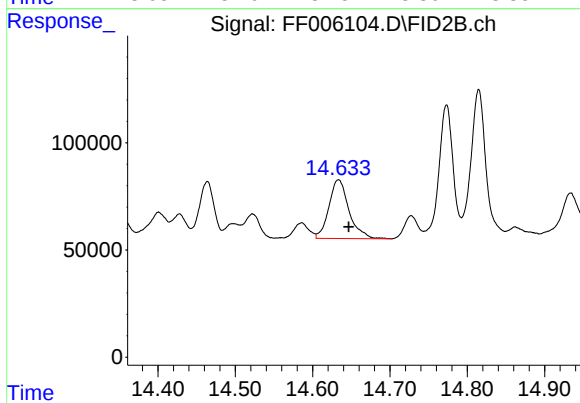

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.633 min
Delta R.T.: -0.013 min
Response: 492686
Conc: 3.39 ug/ml

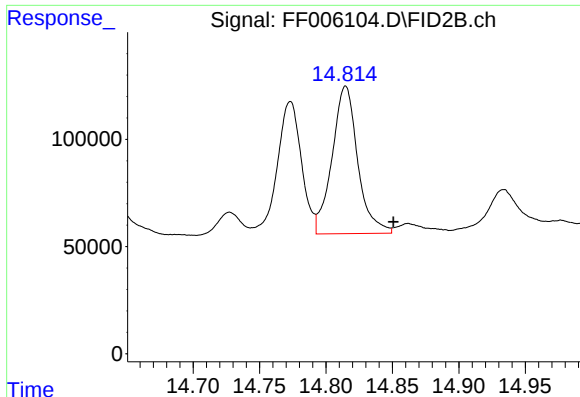

#10 N-TETRACOSANE


R.T.: 14.815 min
Delta R.T.: -0.036 min
Response: 925798
Conc: 5.55 ug/ml

Instrument :
FID_B
ClientSampleId :
TR-05-122619

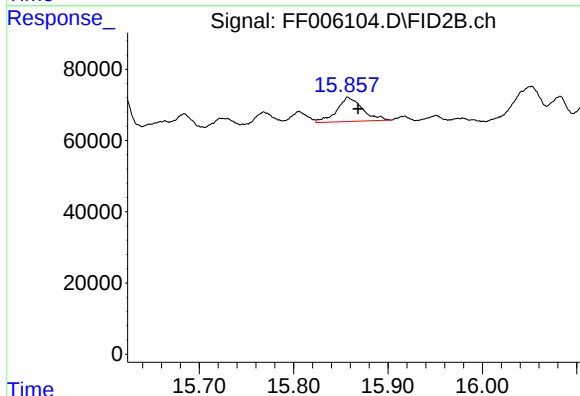


#11 N-HEXACOSANE

R.T.: 15.858 min
Delta R.T.: -0.011 min
Response: 126556
Conc: 0.79 ug/ml

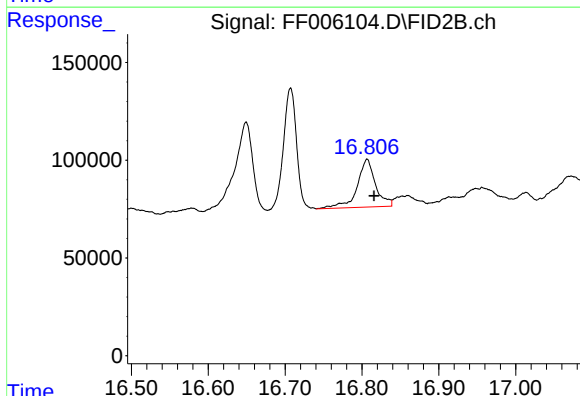


#12 N-OCTACOSANE

R.T.: 16.807 min
Delta R.T.: -0.009 min
Response: 404610
Conc: 2.64 ug/ml

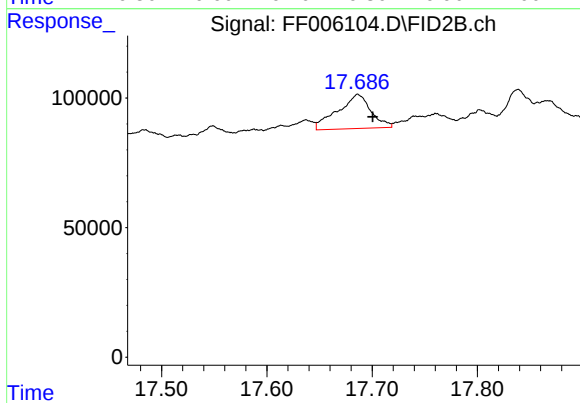

#13 N-TRIACONTANE


R.T.: 17.686 min
Delta R.T.: -0.014 min
Response: 287561
Conc: 1.98 ug/ml

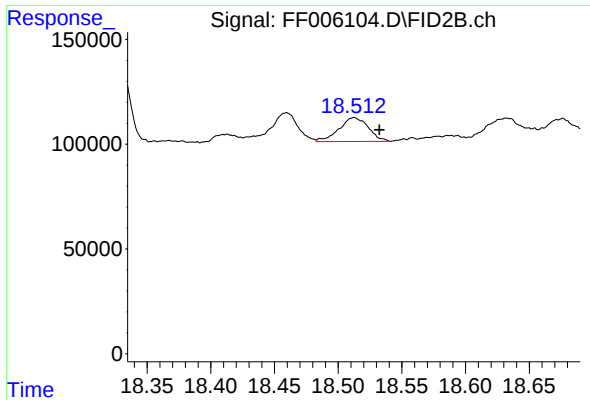

#14 N-DOTRIACONTANE

R.T.: 18.512 min
Delta R.T.: -0.020 min
Response: 183784
Conc: 1.32 ug/ml

Instrument :
FID_B
ClientSampleId :
TR-05-122619

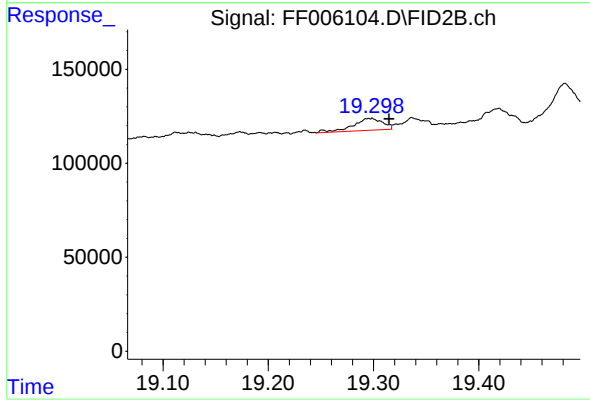

#15 N-TETRATRIACONTANE

R.T.: 19.298 min
Delta R.T.: -0.017 min
Response: 122721
Conc: 0.94 ug/ml