

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122719\
 Data File : FF006105.D
 Signal(s) : FID2B.ch
 Acq On : 27 Dec 2019 21:08
 Operator : DD\AJ
 Sample : K6436-06 5X
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 K009-WC-1

Integration File: autoint1.e
 Quant Time: Dec 27 22:37:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
 Quant Title :
 QLast Update : Fri Dec 06 13:20:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.633	226794	1.561 ug/ml
Target Compounds			
7) N-EICOSANE	12.601	259136	1.500 ug/ml
8) N-DOCOSANE	13.742	112682	0.662 ug/ml
10) N-TETRACOSANE	14.815	73148	0.438 ug/ml
11) N-HEXACOSANE	15.859	103489	0.643 ug/ml
12) N-OCTACOSANE	16.804	350067	2.282 ug/ml
13) N-TRIACONTANE	17.689	627292	4.324 ug/ml
14) N-DOTRIACONTANE	18.518	537536	3.871 ug/ml
15) N-TETRATRIACONTANE	19.301	302437	2.306 ug/ml
16) N-HEXATRIACONTANE	20.069	89184	0.714 ug/ml
17) N-OCTATRIACONTANE	20.769	370966	3.161 ug/ml
18) N-TETRACONTANE	21.654	381002	3.057 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122719\
Data File : FF006105.D
Signal(s) : FID2B.ch
Acq On : 27 Dec 2019 21:08
Operator : DD\AJ
Sample : K6436-06 5X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_B
ClientSampled :
K009-WC-1

Integration File: autoint1.e
Quant Time: Dec 27 22:37:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
Quant Title :
QLast Update : Fri Dec 06 13:20:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

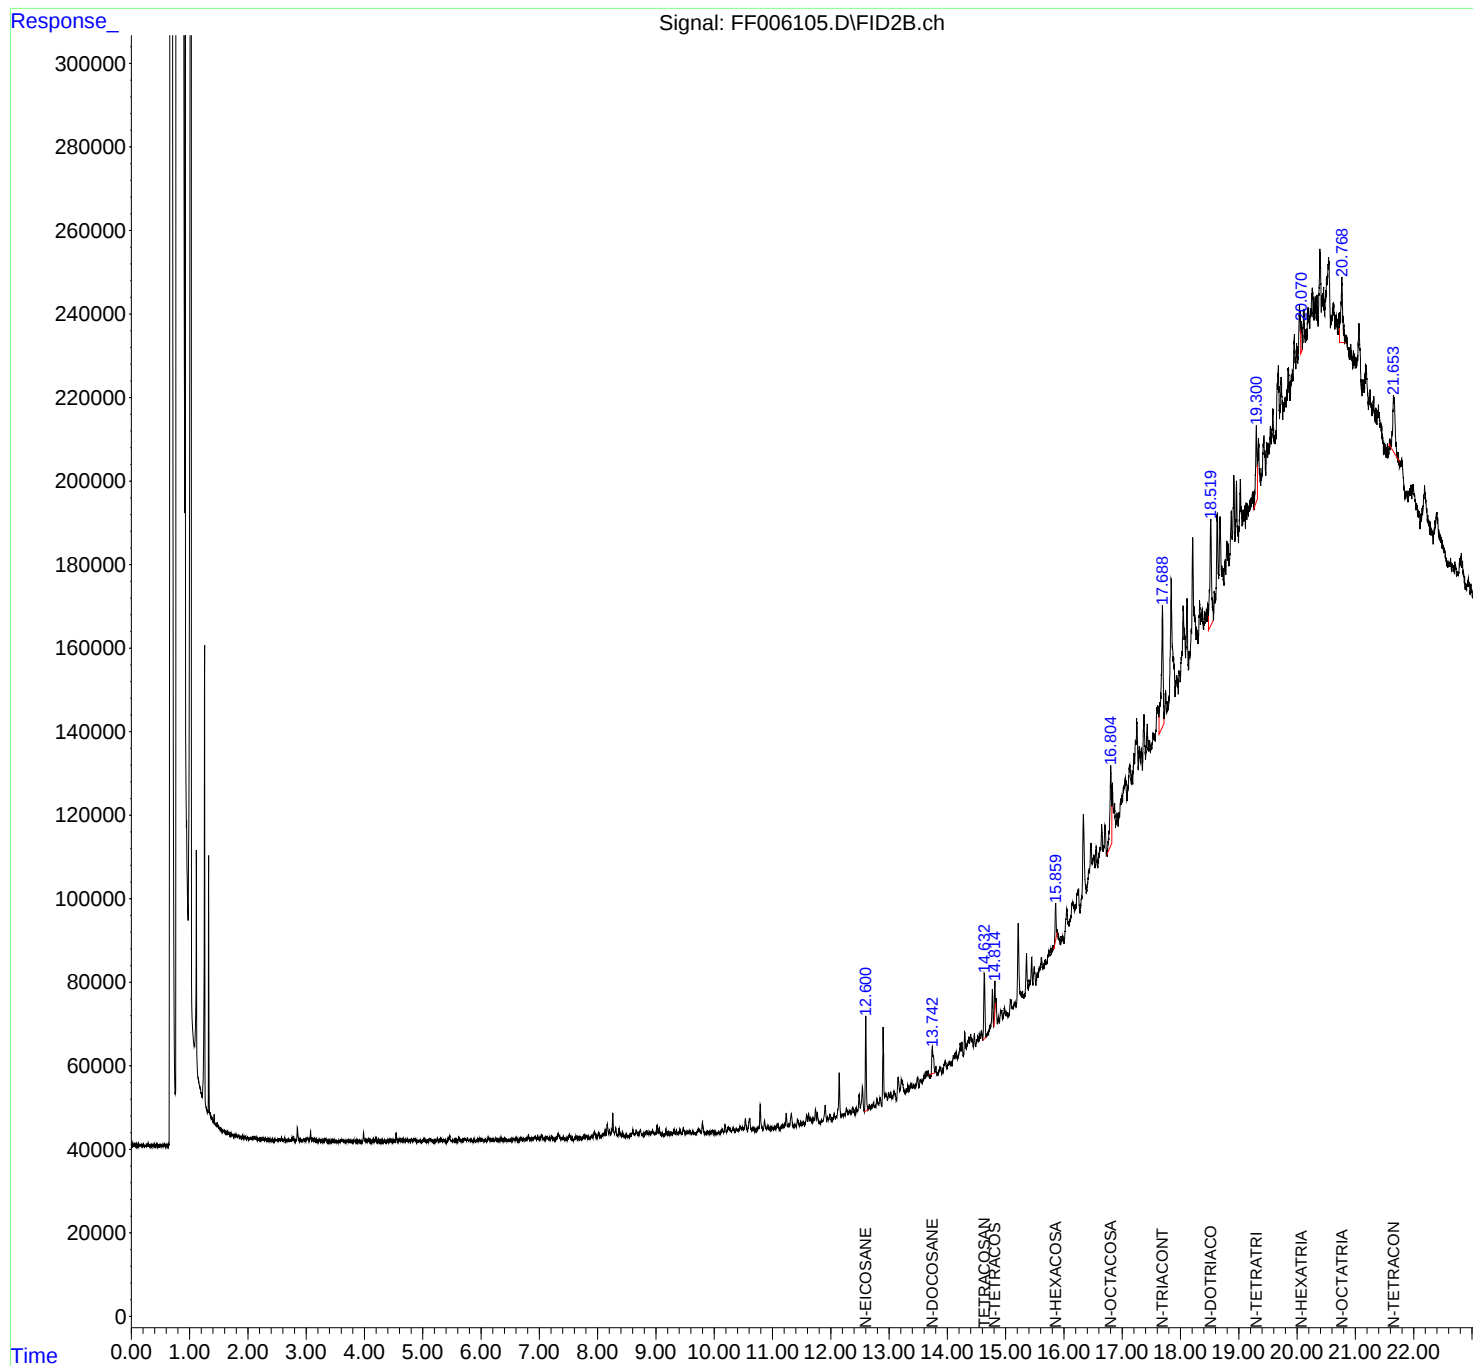


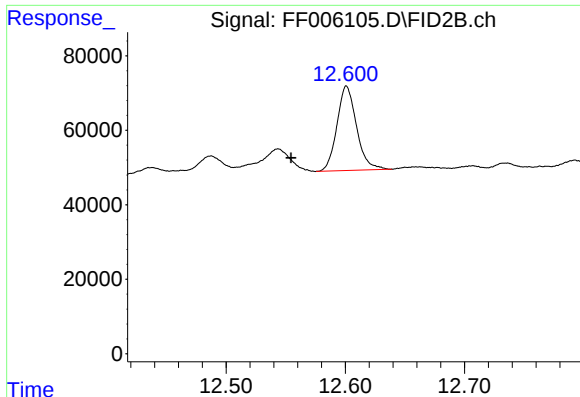

#7 N-EICOSANE


R.T.: 12.601 min
Delta R.T.: 0.046 min
Response: 259136
Conc: 1.50 ug/ml

Instrument :
FID_B
ClientSampleId :
K009-WC-1

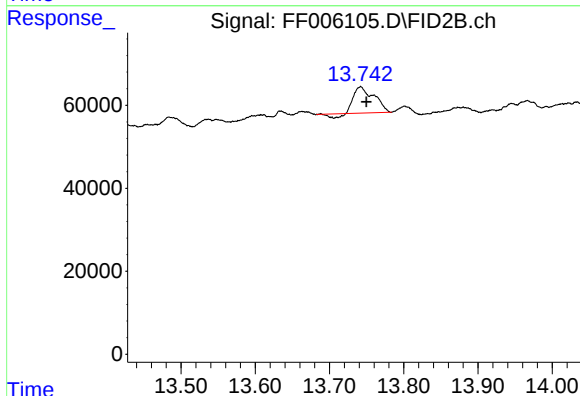


#8 N-DOCOSANE

R.T.: 13.742 min
Delta R.T.: -0.008 min
Response: 112682
Conc: 0.66 ug/ml

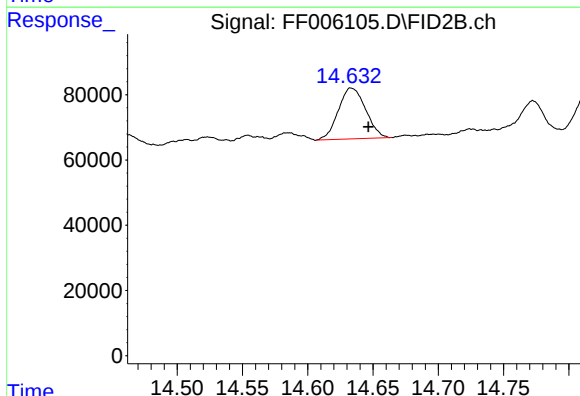


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.633 min
Delta R.T.: -0.013 min
Response: 226794
Conc: 1.56 ug/ml

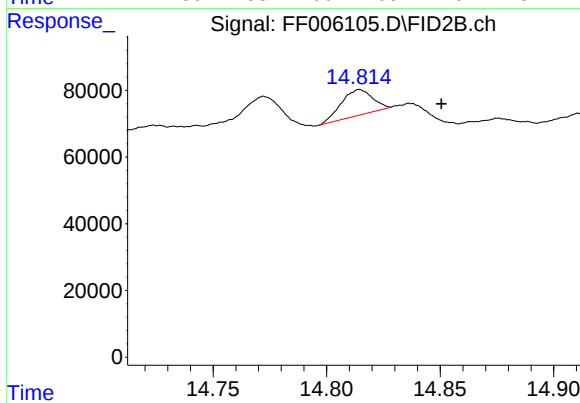

#10 N-TETRACOSANE


R.T.: 14.815 min
Delta R.T.: -0.036 min
Response: 73148
Conc: 0.44 ug/ml

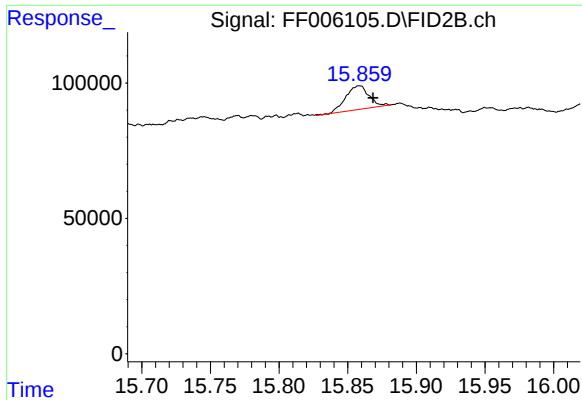

#11 N-HEXACOSANE


R.T.: 15.859 min
Delta R.T.: -0.010 min
Response: 103489
Conc: 0.64 ug/ml

Instrument :
FID_B
ClientSampleId :
K009-WC-1

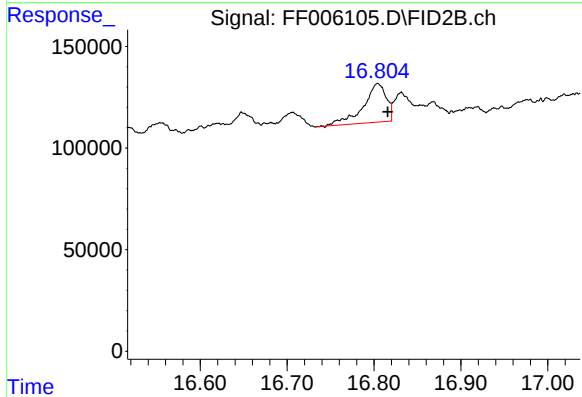


#12 N-OCTACOSANE

R.T.: 16.804 min
Delta R.T.: -0.012 min
Response: 350067
Conc: 2.28 ug/ml

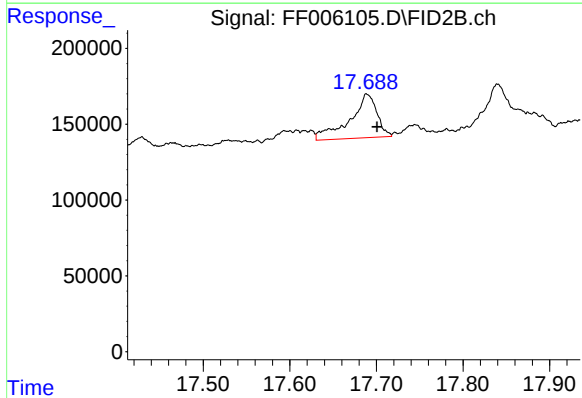


#13 N-TRIACONTANE

R.T.: 17.689 min
Delta R.T.: -0.012 min
Response: 627292
Conc: 4.32 ug/ml

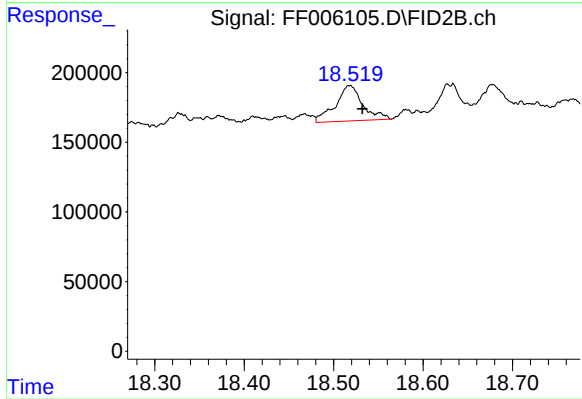

#14 N-DOTRIACONTANE


R.T.: 18.518 min
Delta R.T.: -0.014 min
Response: 537536
Conc: 3.87 ug/ml

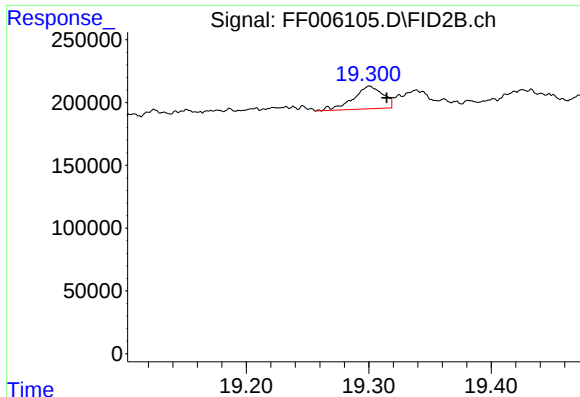

#15 N-TETRATRIACONTANE


R.T.: 19.301 min
Delta R.T.: -0.014 min
Response: 302437
Conc: 2.31 ug/ml

Instrument :
FID_B
ClientSampleId :
K009-WC-1

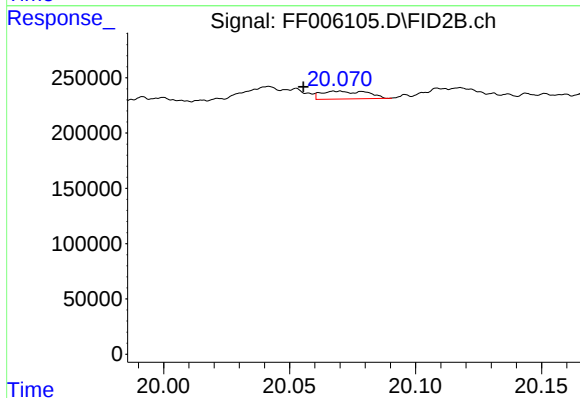


#16 N-HEXATRIACONTANE

R.T.: 20.069 min
Delta R.T.: 0.014 min
Response: 89184
Conc: 0.71 ug/ml

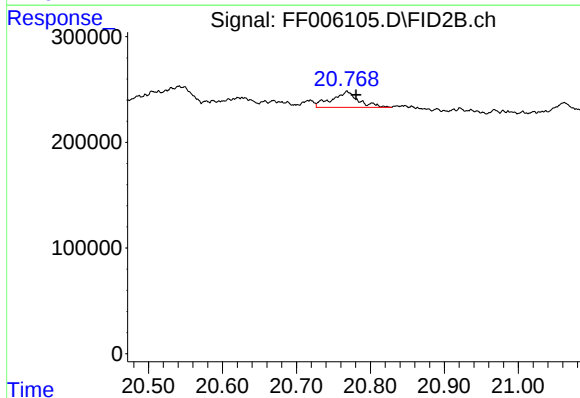

#17 N-OCTATRIACONTANE

R.T.: 20.769 min
Delta R.T.: -0.012 min
Response: 370966
Conc: 3.16 ug/ml

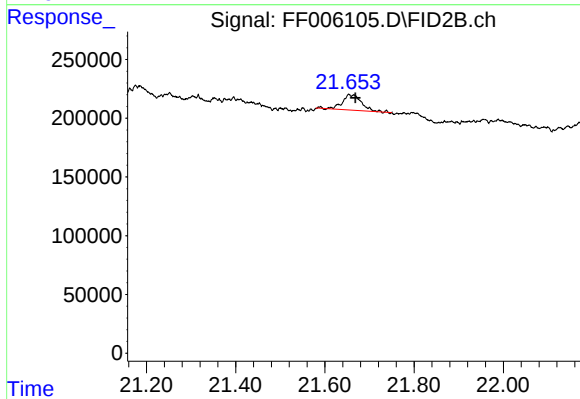

#18 N-TETRACONTANE

R.T.: 21.654 min
Delta R.T.: -0.014 min
Response: 381002
Conc: 3.06 ug/ml