

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122719\
 Data File : FB023323.D
 Signal(s) : FID2B.CH
 Acq On : 27 Dec 2019 11:01
 Operator : DD/AJ
 Sample : BSF1227S1
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1227S1

Integration File: Calibration.e
 Quant Time: Dec 27 21:48:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	410899	17.327 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	802910	25.942 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	894345	26.772 ng/ml
3) t n-Heptane	7.752	288464	8.745 ng/ml
4) t Benzene	7.889	358222	8.971 ng/ml
6) t Toluene	10.626	1064079	27.636 ng/ml
7) t Ethylbenzene	13.066	340469	9.380 ng/ml
8) t m-Xylene	13.199	653837	18.836 ng/ml
9) t O-Xylene	13.927	638410	18.954 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	536928	19.136 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122719\
Data File : FB023323.D
Signal(s) : FID2B.CH
Acq On : 27 Dec 2019 11:01
Operator : DD/AJ
Sample : BSF1227S1
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1227S1

Integration File: Calibration.e
Quant Time: Dec 27 21:48:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

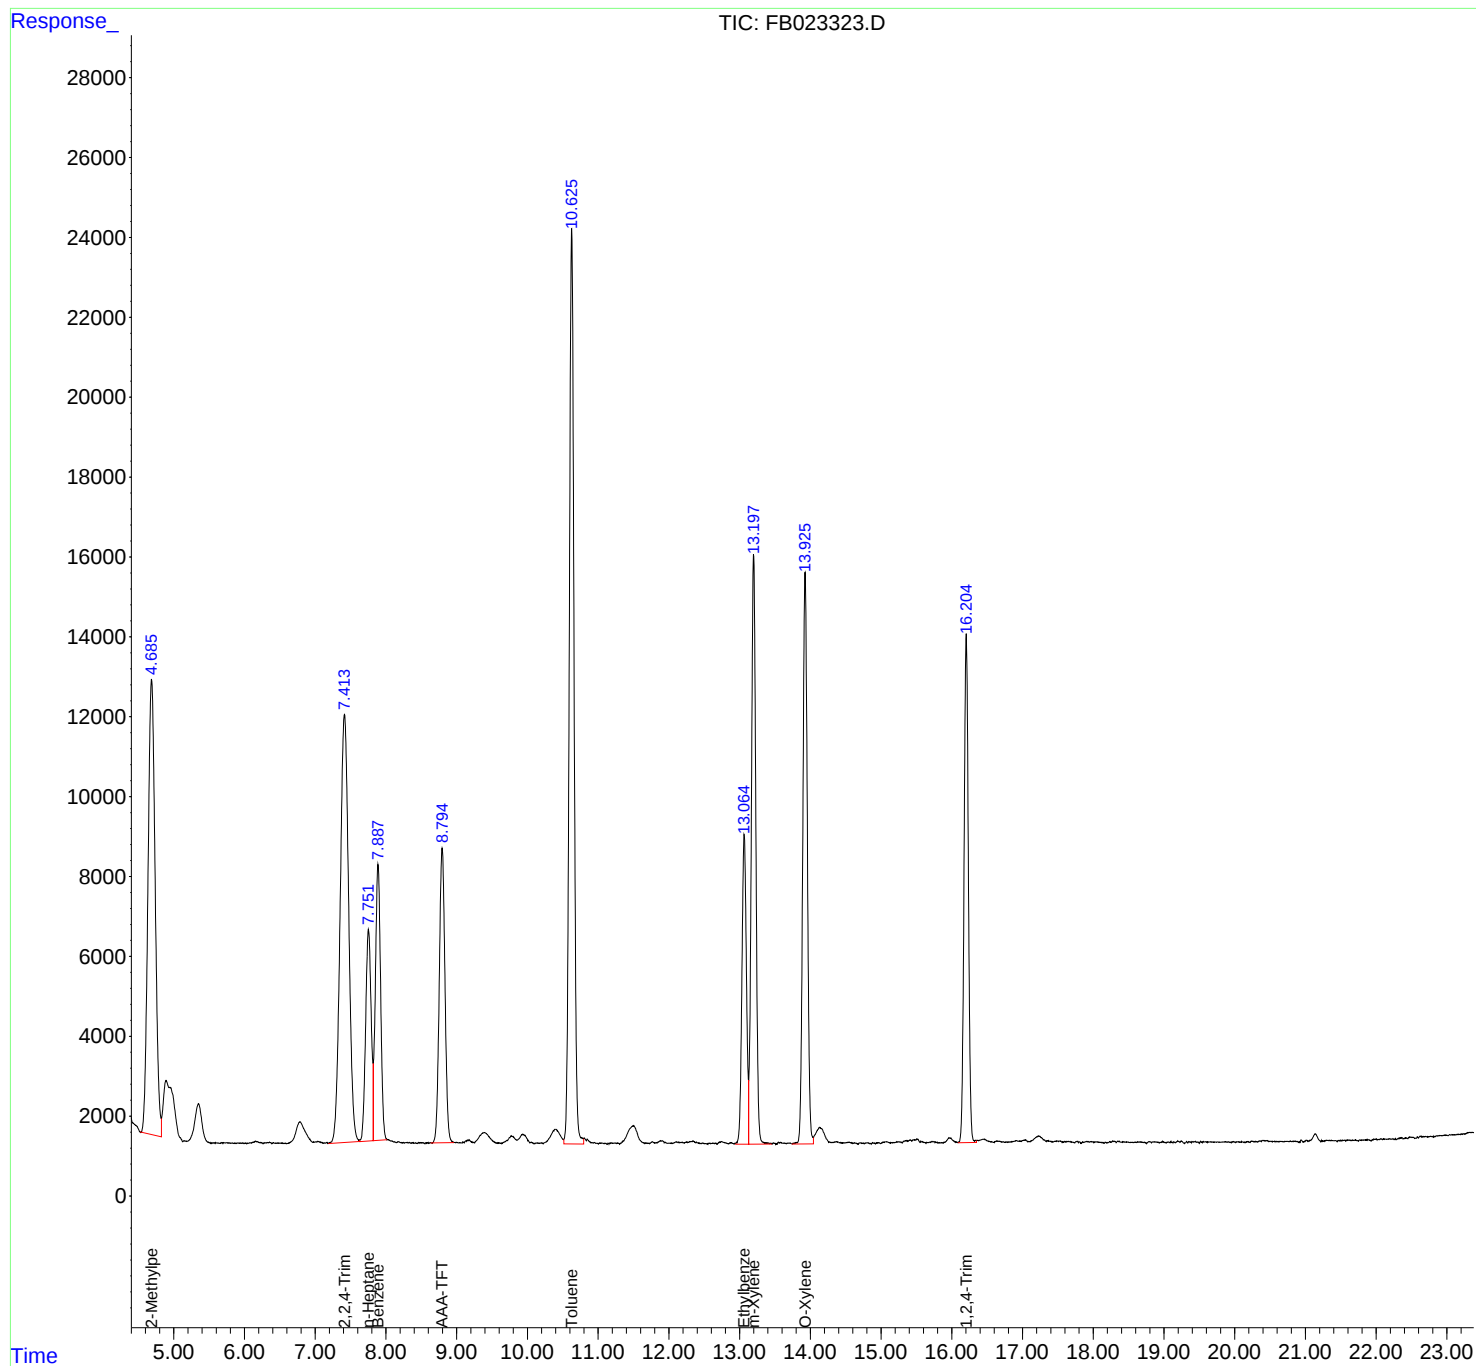


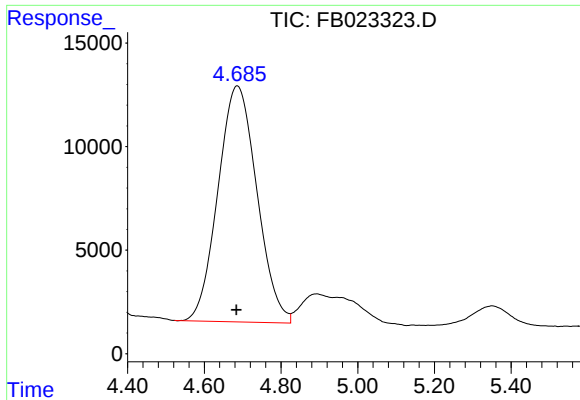

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: 0.003 min
Response: 802910
Conc: 25.94 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1227S1

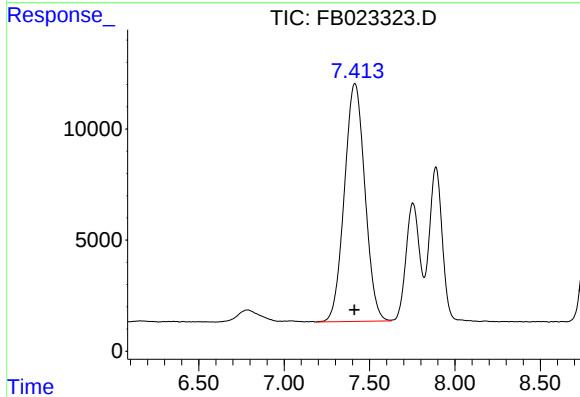


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: 0.003 min
Response: 894345
Conc: 26.77 ng/ml

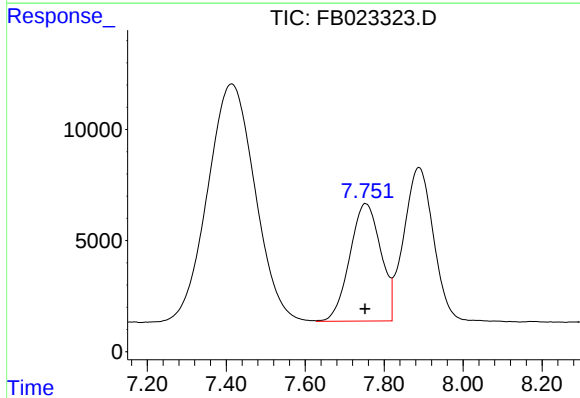


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 288464
Conc: 8.75 ng/ml

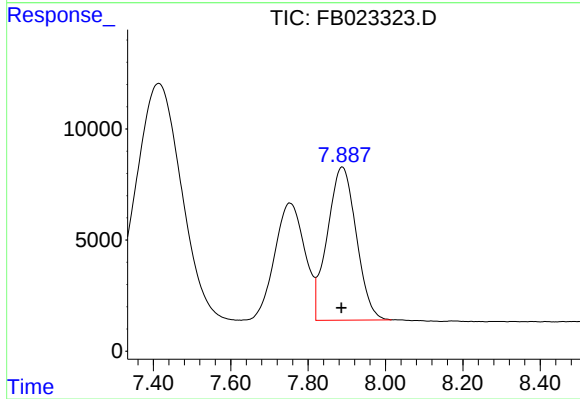

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.002 min
Response: 358222
Conc: 8.97 ng/ml

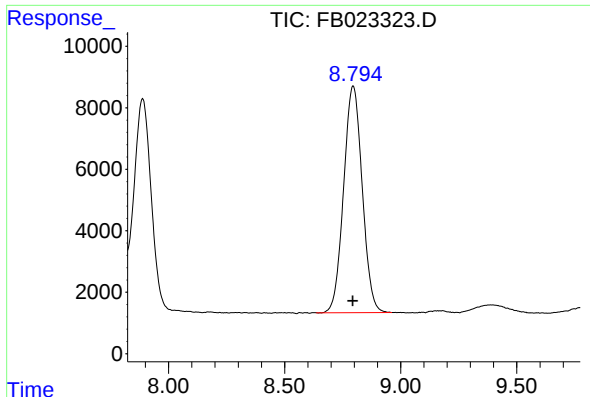

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.002 min
Response: 410899
Conc: 17.33 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1227S1

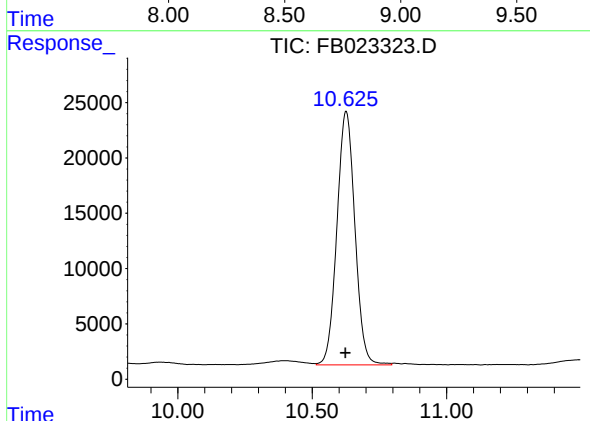


#6 Toluene

R.T.: 10.626 min
Delta R.T.: 0.003 min
Response: 1064079
Conc: 27.64 ng/ml

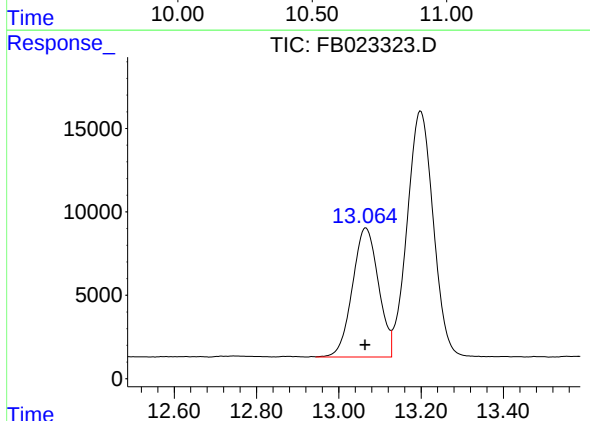


#7 Ethylbenzene

R.T.: 13.066 min
Delta R.T.: 0.002 min
Response: 340469
Conc: 9.38 ng/ml

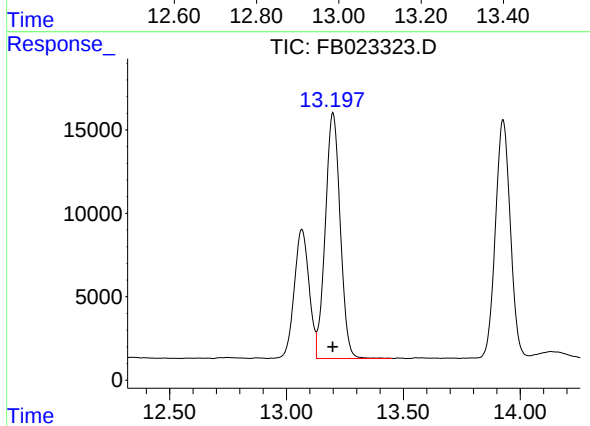

#8 m-Xylene


R.T.: 13.199 min
Delta R.T.: 0.002 min
Response: 653837
Conc: 18.84 ng/ml

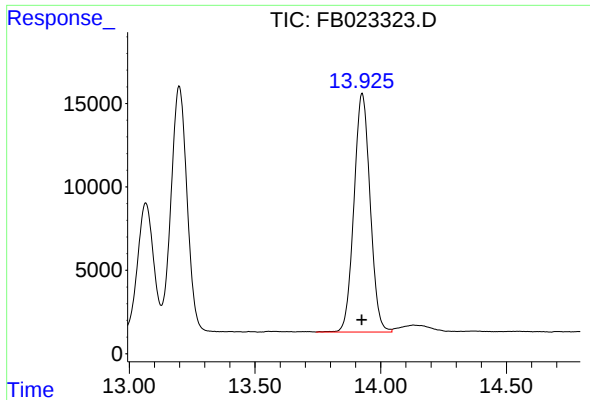

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: 0.002 min
Response: 638410
Conc: 18.95 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1227S1

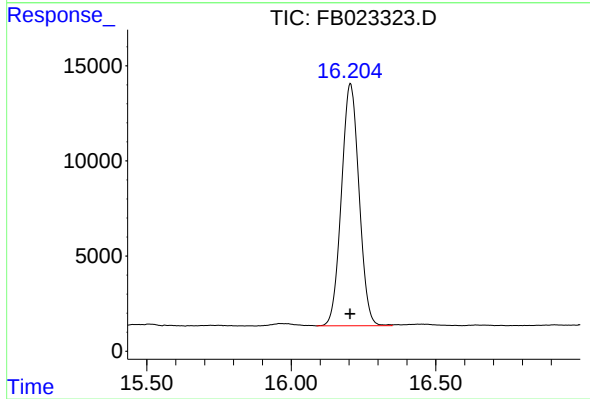

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: 0.002 min
Response: 536928
Conc: 19.14 ng/ml