

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122723\
 Data File : FB030514.D
 Signal(s) : FID2B.CH
 Acq On : 27 Dec 2023 10:21
 Operator : YP/AJ
 Sample : 10 GRO STD
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 27 10:05:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB122723.M
 Quant Title :
 QLast Update : Wed Dec 27 10:03:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.784	119336	10.178 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.702	240721	15.224 ng/ml
2) t 2,2,4-Trimethylpentane	7.408	227277	14.017 ng/ml
3) t n-Heptane	7.743	83577	5.084 ng/ml
4) t Benzene	7.880	105351	5.107 ng/ml
6) t Toluene	10.611	317494	15.555 ng/ml
7) t Ethylbenzene	13.047	97943	5.065 ng/ml
8) t m-Xylene	13.179	197902	10.156 ng/ml
9) t O-Xylene	13.907	195165	10.102 ng/ml
10) t 1,2,4-Trimethylbenzene	16.181	199850	9.962 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122723\
Data File : FB030514.D
Signal(s) : FID2B.CH
Acq On : 27 Dec 2023 10:21
Operator : YP/AJ
Sample : 10 GRO STD
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 27 10:05:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB122723.M
Quant Title :
QLast Update : Wed Dec 27 10:03:23 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

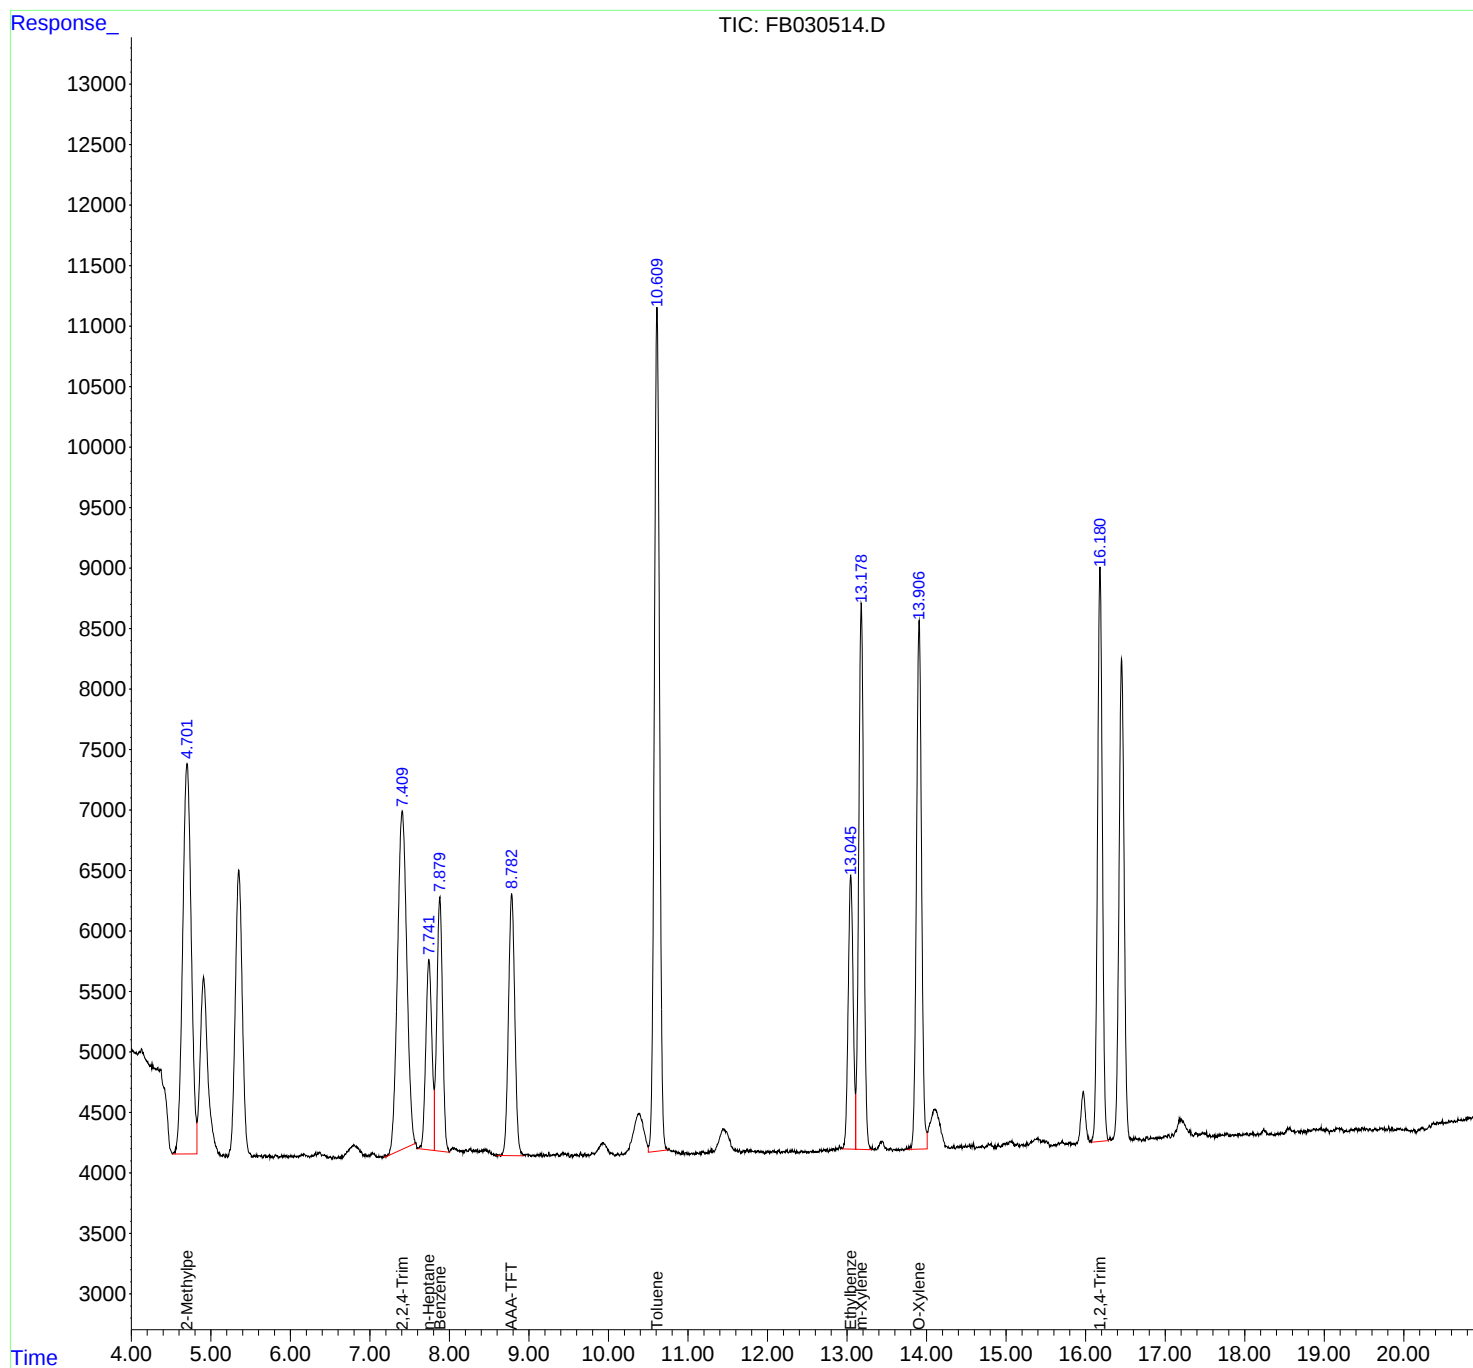

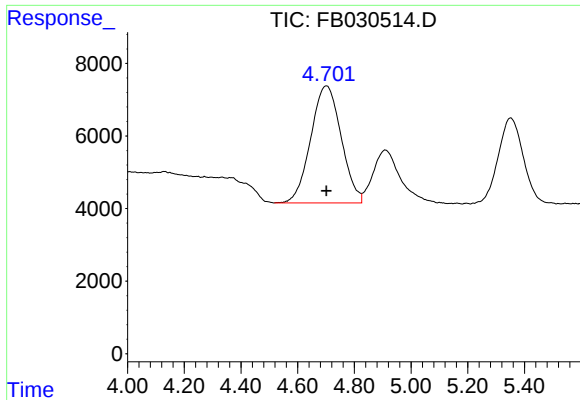


#1 2-Methylpentane

R.T.: 4.702 min
Delta R.T.: 0.000 min
Response: 240721
Conc: 15.22 ng/ml

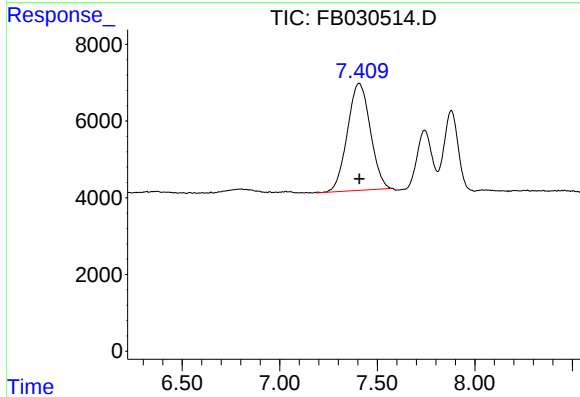


#2 2,2,4-Trimethylpentane

R.T.: 7.408 min
Delta R.T.: 0.000 min
Response: 227277
Conc: 14.02 ng/ml

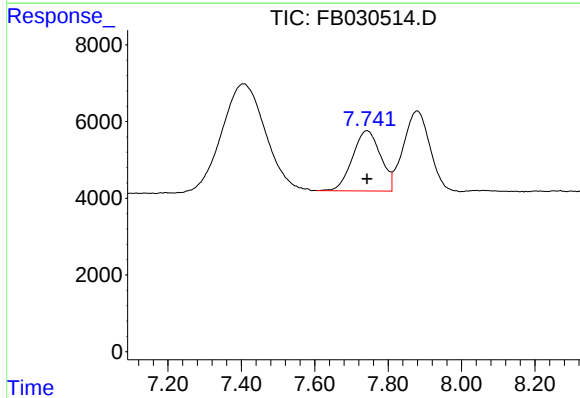


#3 n-Heptane

R.T.: 7.743 min
Delta R.T.: 0.000 min
Response: 83577
Conc: 5.08 ng/ml

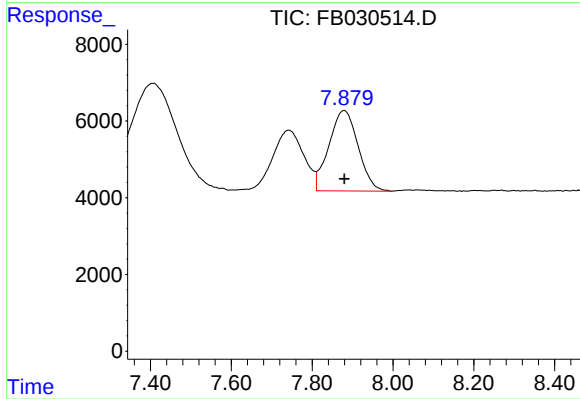


#4 Benzene

R.T.: 7.880 min
Delta R.T.: 0.000 min
Response: 105351
Conc: 5.11 ng/ml

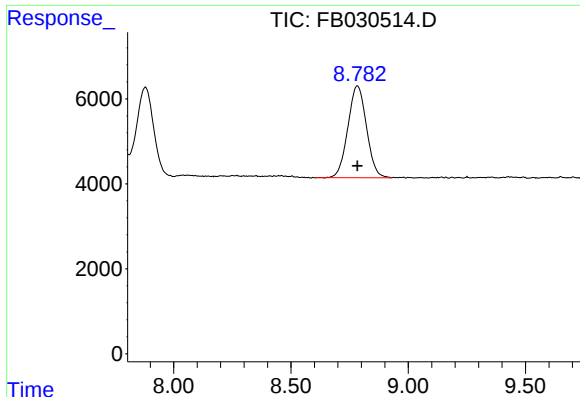


#5 AAA-TFT

R.T.: 8.784 min
Delta R.T.: 0.000 min
Response: 119336
Conc: 10.18 ng/ml

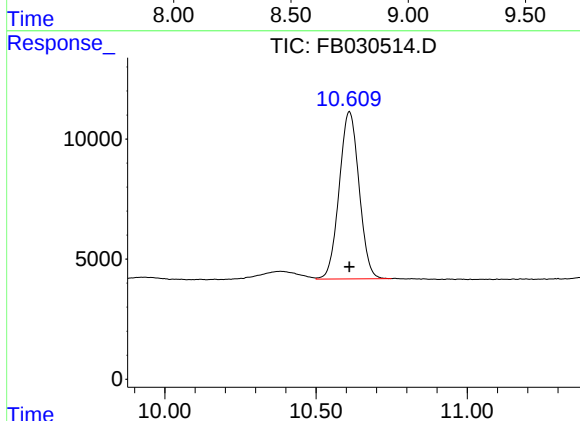


#6 Toluene

R.T.: 10.611 min
Delta R.T.: 0.000 min
Response: 317494
Conc: 15.56 ng/ml

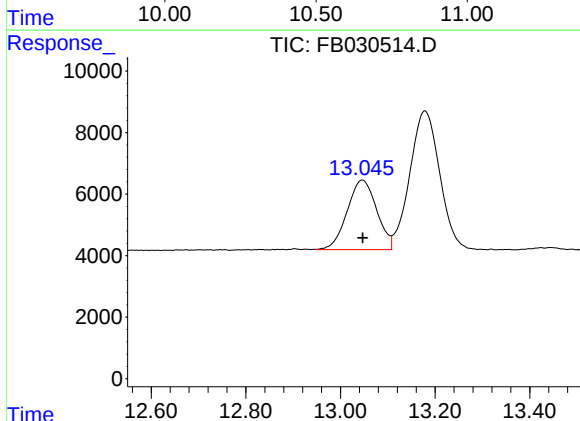


#7 Ethylbenzene

R.T.: 13.047 min
Delta R.T.: 0.000 min
Response: 97943
Conc: 5.06 ng/ml

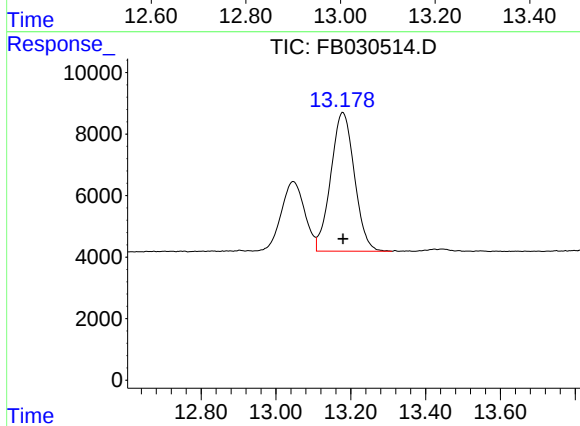


#8 m-Xylene

R.T.: 13.179 min
Delta R.T.: 0.000 min
Response: 197902
Conc: 10.16 ng/ml

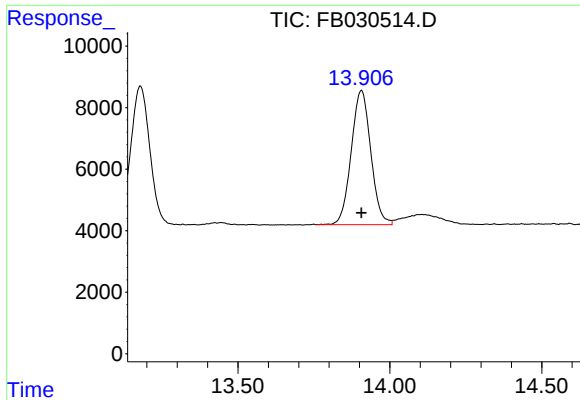

#9 O-Xylene

R.T.: 13.907 min
Delta R.T.: 0.000 min
Response: 195165
Conc: 10.10 ng/ml

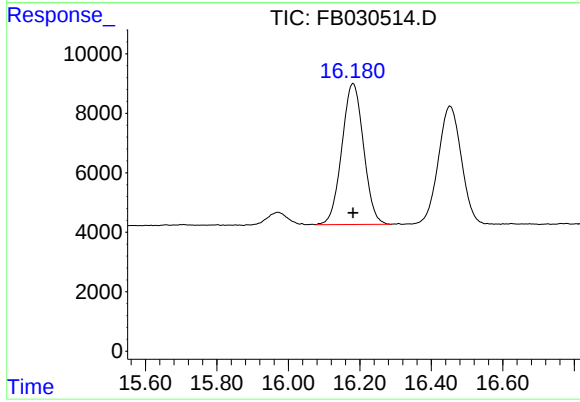

#10 1,2,4-Trimethylbenzene

R.T.: 16.181 min
Delta R.T.: 0.000 min
Response: 199850
Conc: 9.96 ng/ml