

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122821\
 Data File : FB026558.D
 Signal(s) : FID2B.CH
 Acq On : 28 Dec 2021 13:33
 Operator : AJ/MA
 Sample : BSF1228S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1228S1

Integration File: Calibration.e
 Quant Time: Dec 29 00:19:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
 Quant Title :
 QLast Update : Wed Dec 08 14:04:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	214161	19.062 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	430727	24.745 ng/ml
2) t 2,2,4-Trimethylpentane	7.440	534522	26.953 ng/ml
3) t n-Heptane	7.749	142159	7.426 ng/ml
4) t Benzene	7.886	179049	8.053 ng/ml
6) t Toluene	10.620	547331	25.650 ng/ml
7) t Ethylbenzene	13.057	177725	9.003 ng/ml
8) t m-Xylene	13.190	362228	18.372 ng/ml
9) t O-Xylene	13.917	366386	19.185 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	387762	19.960 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122821\
Data File : FB026558.D
Signal(s) : FID2B.CH
Acq On : 28 Dec 2021 13:33
Operator : AJ/MA
Sample : BSF1228S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1228S1

Integration File: Calibration.e
Quant Time: Dec 29 00:19:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
Quant Title :
QLast Update : Wed Dec 08 14:04:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

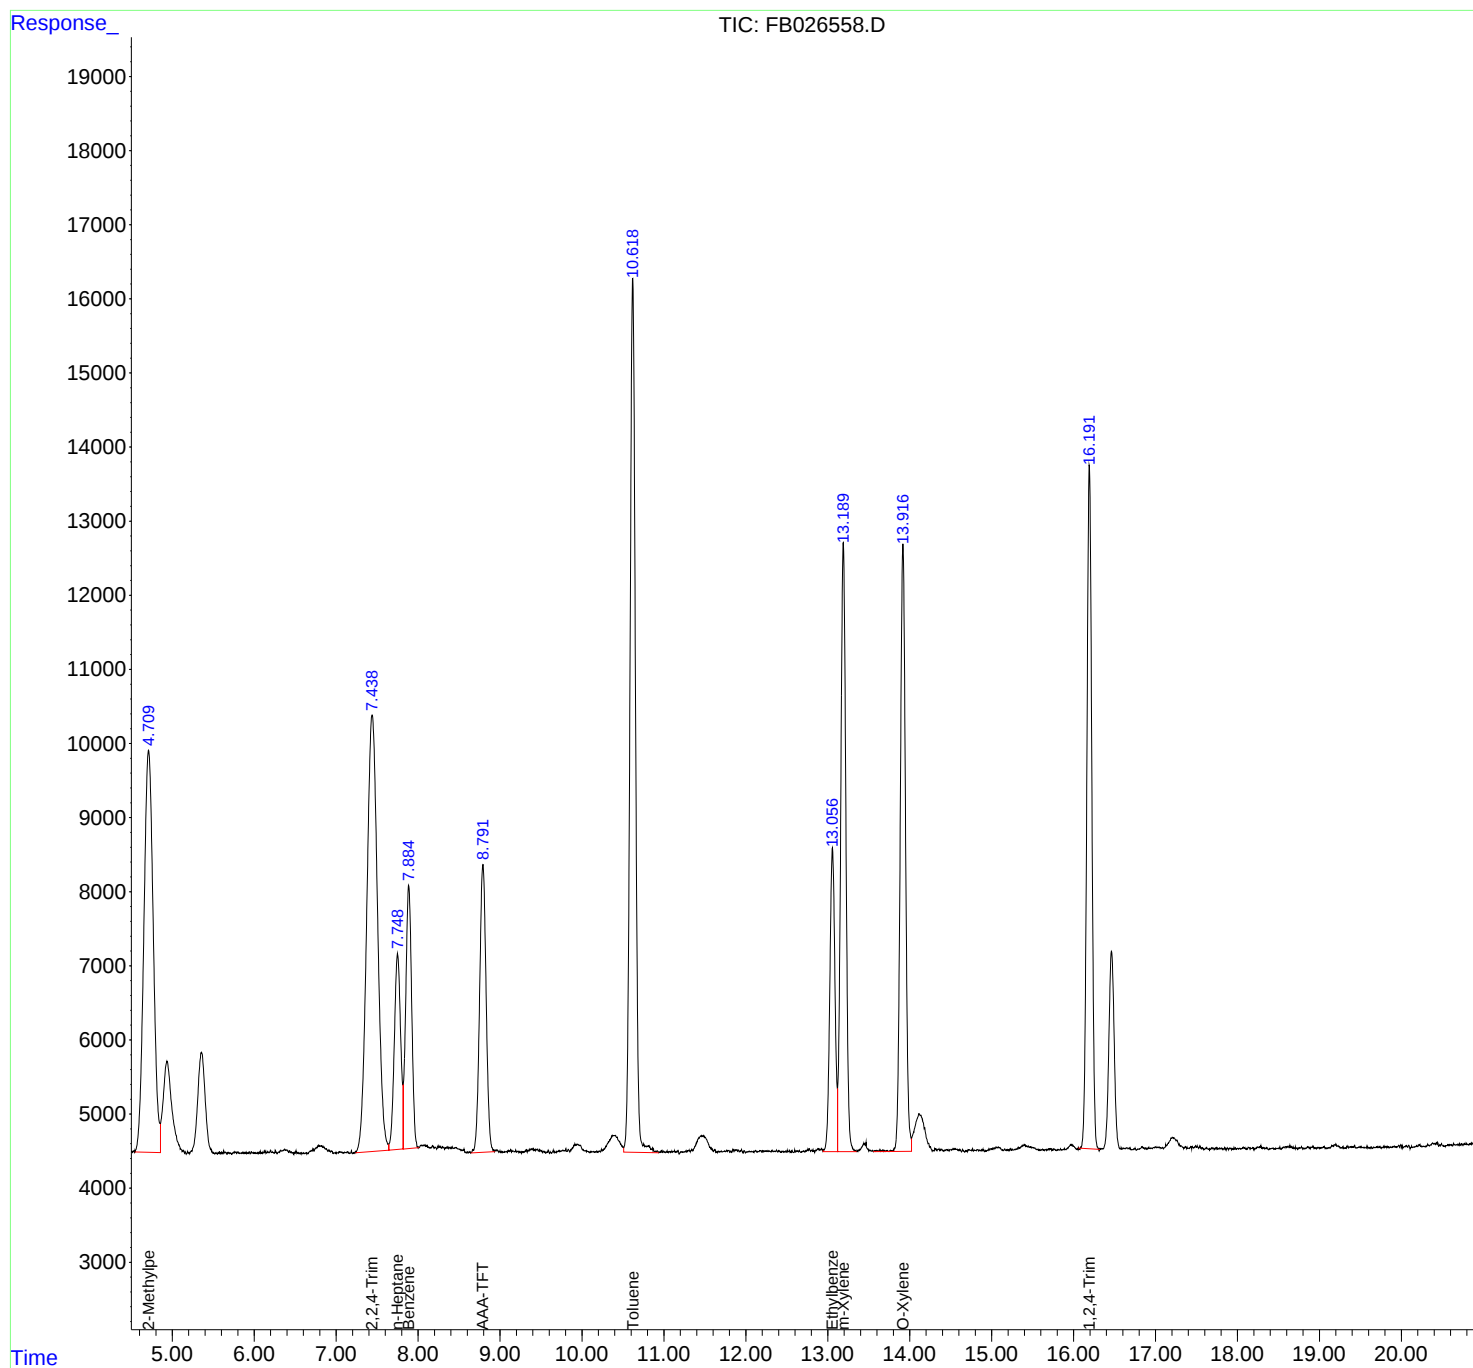


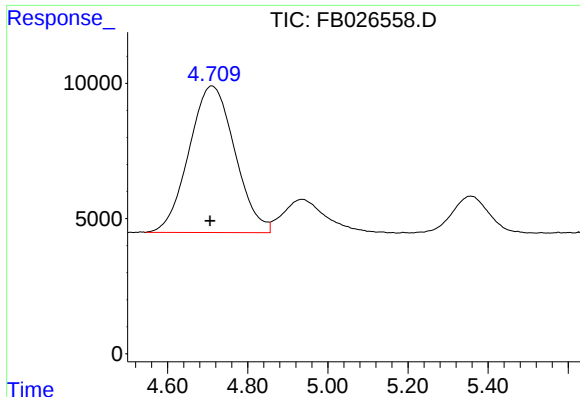

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.005 min
Response: 430727
Conc: 24.74 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1228S1

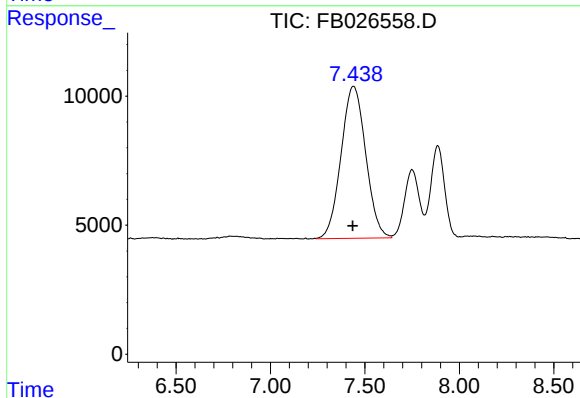


#2 2,2,4-Trimethylpentane

R.T.: 7.440 min
Delta R.T.: 0.005 min
Response: 534522
Conc: 26.95 ng/ml

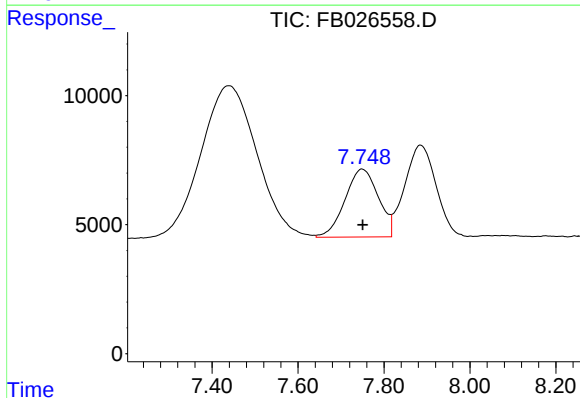


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.001 min
Response: 142159
Conc: 7.43 ng/ml

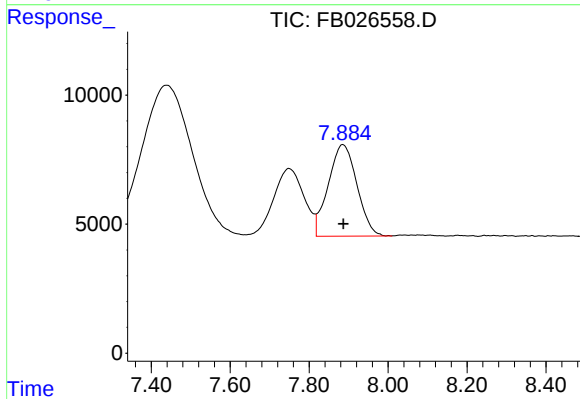

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.001 min
Response: 179049
Conc: 8.05 ng/ml

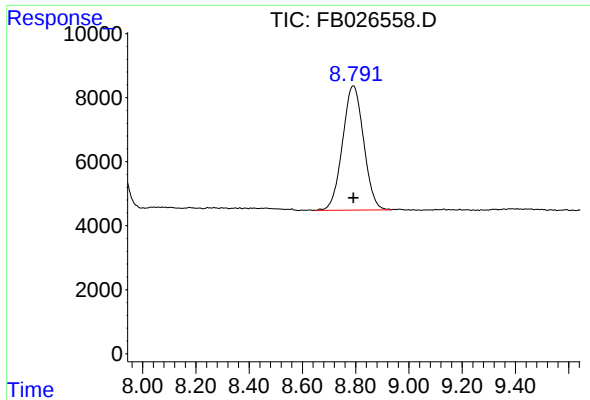

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 214161
Conc: 19.06 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1228S1

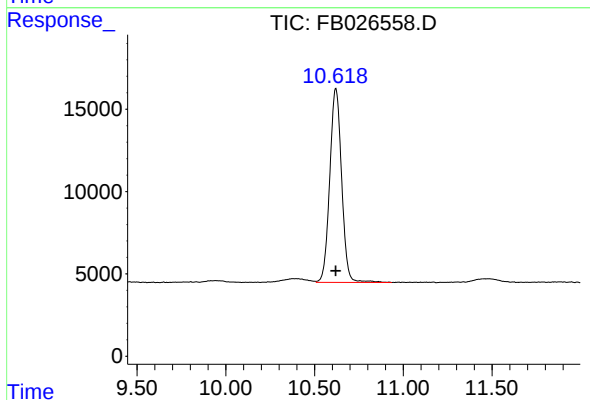


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.001 min
Response: 547331
Conc: 25.65 ng/ml

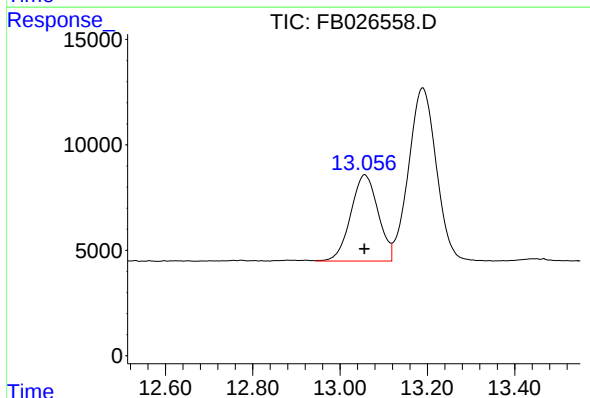


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.002 min
Response: 177725
Conc: 9.00 ng/ml

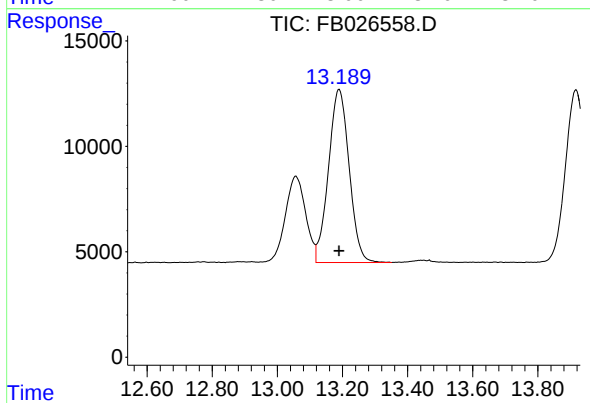

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.000 min
Response: 362228
Conc: 18.37 ng/ml

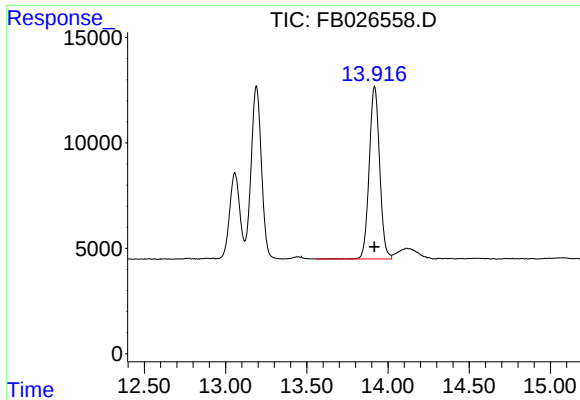

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.001 min
Response: 366386
Conc: 19.19 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1228S1

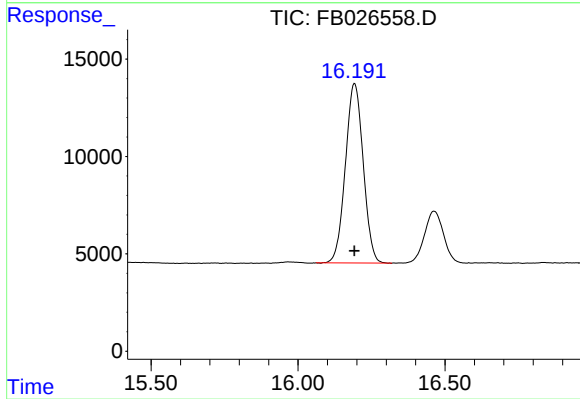

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.000 min
Response: 387762
Conc: 19.96 ng/ml