

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122821\
 Data File : FB026565.D
 Signal(s) : FID2B.CH
 Acq On : 28 Dec 2021 18:26
 Operator : AJ/MA
 Sample : M5239-04MS
 Misc : 5.04G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SASP2-123-1-40-57MS

Integration File: Calibration.e
 Quant Time: Dec 29 00:21:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
 Quant Title :
 QLast Update : Wed Dec 08 14:04:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	210083	18.699 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	462175	26.551 ng/ml
2) t 2,2,4-Trimethylpentane	7.436	558368	28.155 ng/ml
3) t n-Heptane	7.751	162929	8.511 ng/ml
4) t Benzene	7.888	193519	8.704 ng/ml
6) t Toluene	10.621	584794	27.406 ng/ml
7) t Ethylbenzene	13.058	183930	9.317 ng/ml
8) t m-Xylene	13.191	371849	18.860 ng/ml
9) t O-Xylene	13.918	370623	19.407 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	386999	19.920 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122821\
Data File : FB026565.D
Signal(s) : FID2B.CH
Acq On : 28 Dec 2021 18:26
Operator : AJ/MA
Sample : M5239-04MS
Misc : 5.04G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SASP2-123-1-40-57MS

Integration File: Calibration.e
Quant Time: Dec 29 00:21:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
Quant Title :
QLast Update : Wed Dec 08 14:04:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

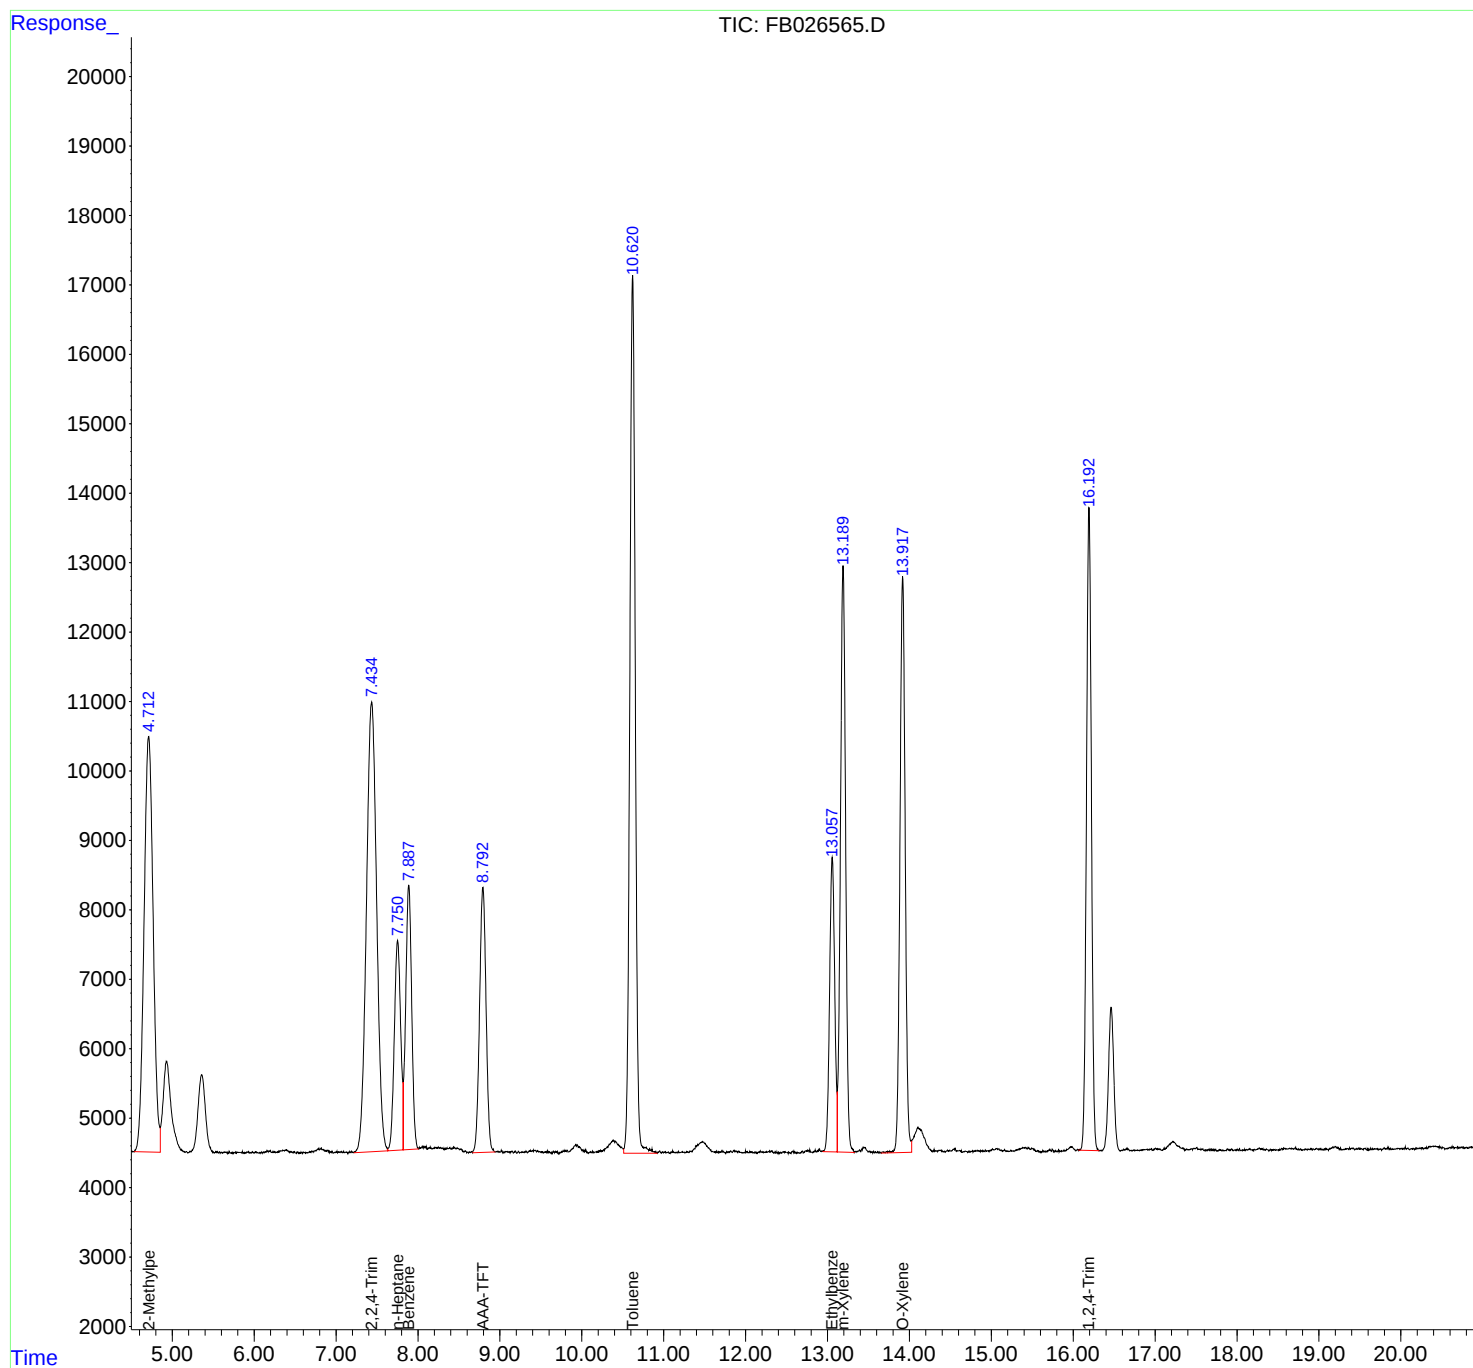


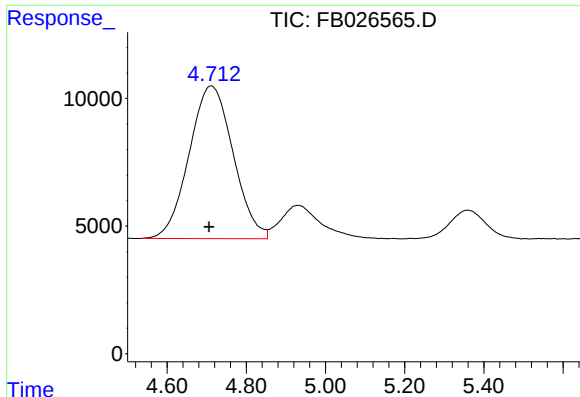

#1 2-Methylpentane


R.T.: 4.713 min
Delta R.T.: 0.007 min
Response: 462175
Conc: 26.55 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-123-1-40-57MS

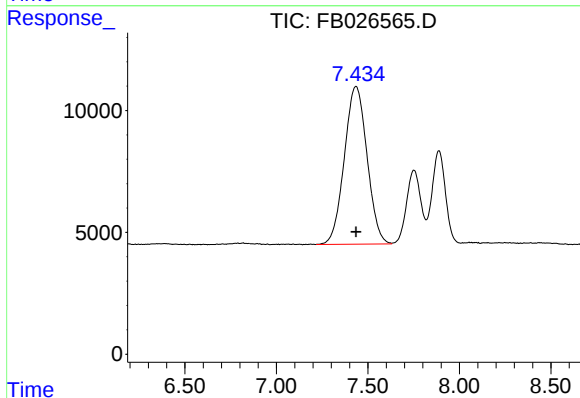


#2 2,2,4-Trimethylpentane

R.T.: 7.436 min
Delta R.T.: 0.000 min
Response: 558368
Conc: 28.16 ng/ml

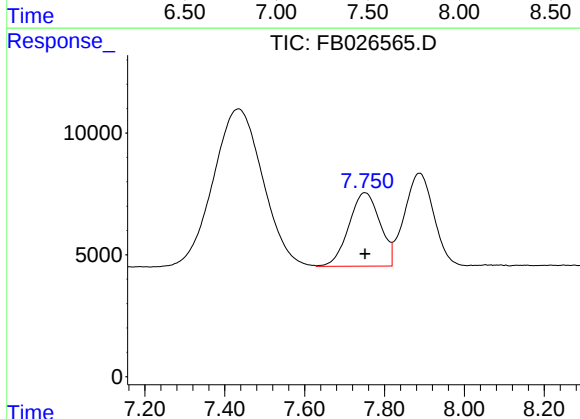


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 162929
Conc: 8.51 ng/ml

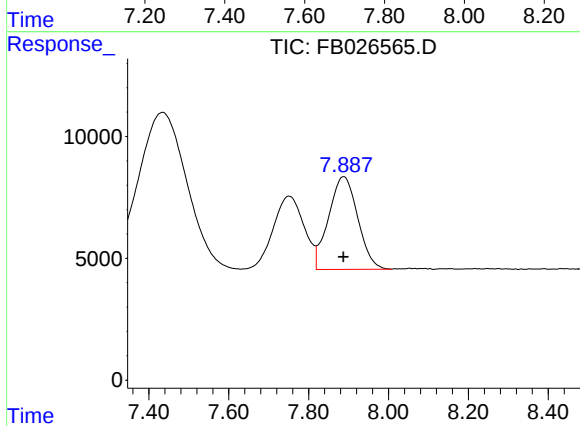

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.002 min
Response: 193519
Conc: 8.70 ng/ml

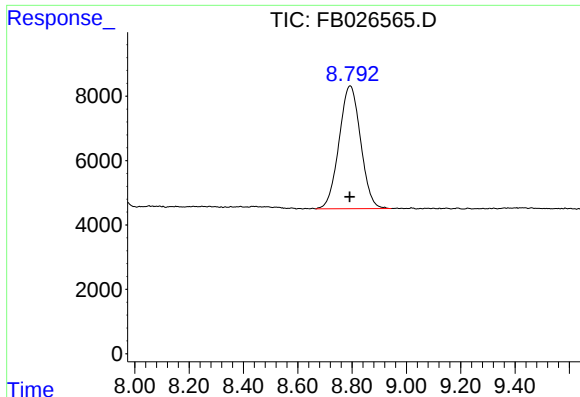

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.002 min
Response: 210083
Conc: 18.70 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-123-1-40-57MS

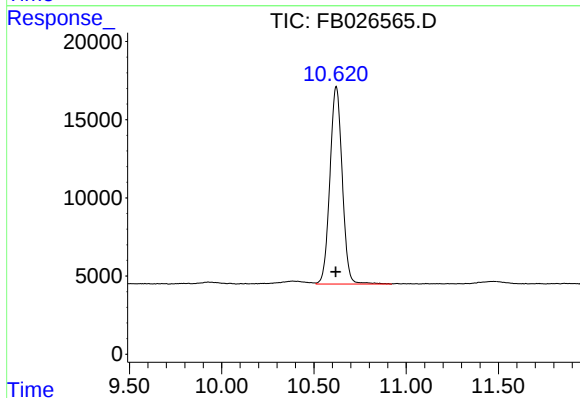


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.002 min
Response: 584794
Conc: 27.41 ng/ml

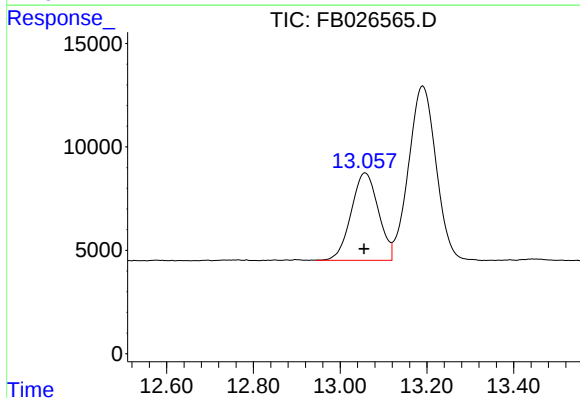


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.003 min
Response: 183930
Conc: 9.32 ng/ml

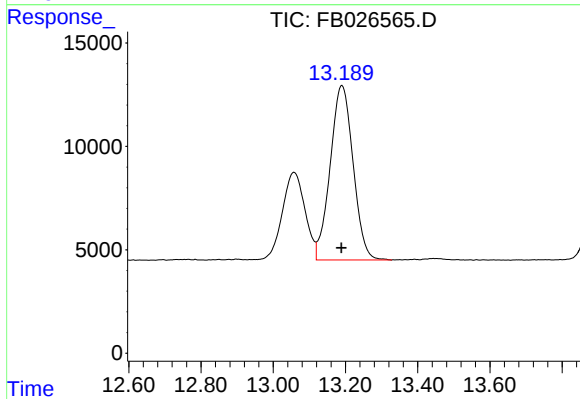

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.002 min
Response: 371849
Conc: 18.86 ng/ml

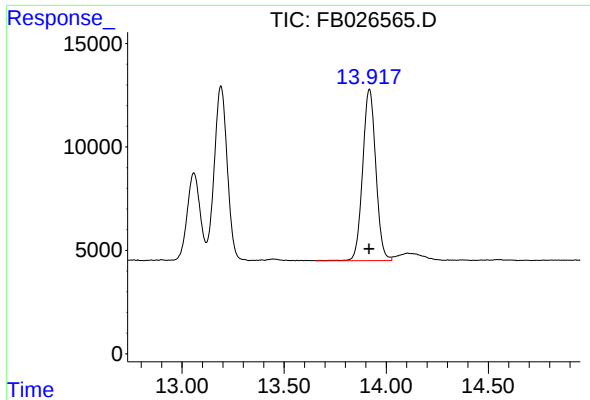

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.002 min
Response: 370623
Conc: 19.41 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-123-1-40-57MS

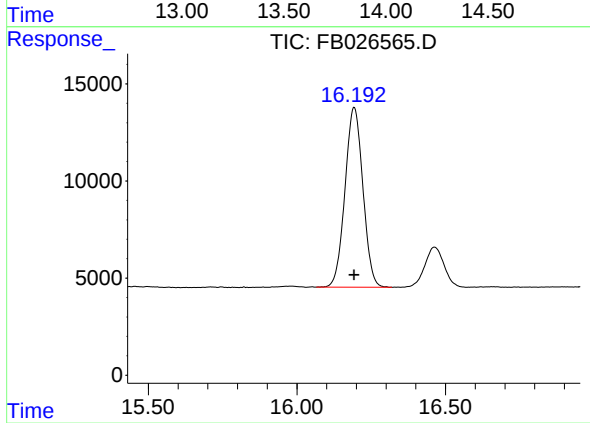

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.001 min
Response: 386999
Conc: 19.92 ng/ml