

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122821\
 Data File : FB026566.D
 Signal(s) : FID2B.CH
 Acq On : 28 Dec 2021 19:02
 Operator : AJ/MA
 Sample : M5239-04MSD
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SASP2-123-1-40-57MSD

Integration File: Calibration.e
 Quant Time: Dec 29 00:21:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
 Quant Title :
 QLast Update : Wed Dec 08 14:04:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	250621	22.307 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	512903	29.466 ng/ml
2) t 2,2,4-Trimethylpentane	7.436	589499	29.725 ng/ml
3) t n-Heptane	7.751	194151	10.142 ng/ml
4) t Benzene	7.886	227847	10.248 ng/ml
6) t Toluene	10.621	648877	30.409 ng/ml
7) t Ethylbenzene	13.058	205569	10.413 ng/ml
8) t m-Xylene	13.191	402989	20.440 ng/ml
9) t O-Xylene	13.918	387787	20.306 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	379705	19.545 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122821\
Data File : FB026566.D
Signal(s) : FID2B.CH
Acq On : 28 Dec 2021 19:02
Operator : AJ/MA
Sample : M5239-04MSD
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SASP2-123-1-40-57MSD

Integration File: Calibration.e
Quant Time: Dec 29 00:21:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
Quant Title :
QLast Update : Wed Dec 08 14:04:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

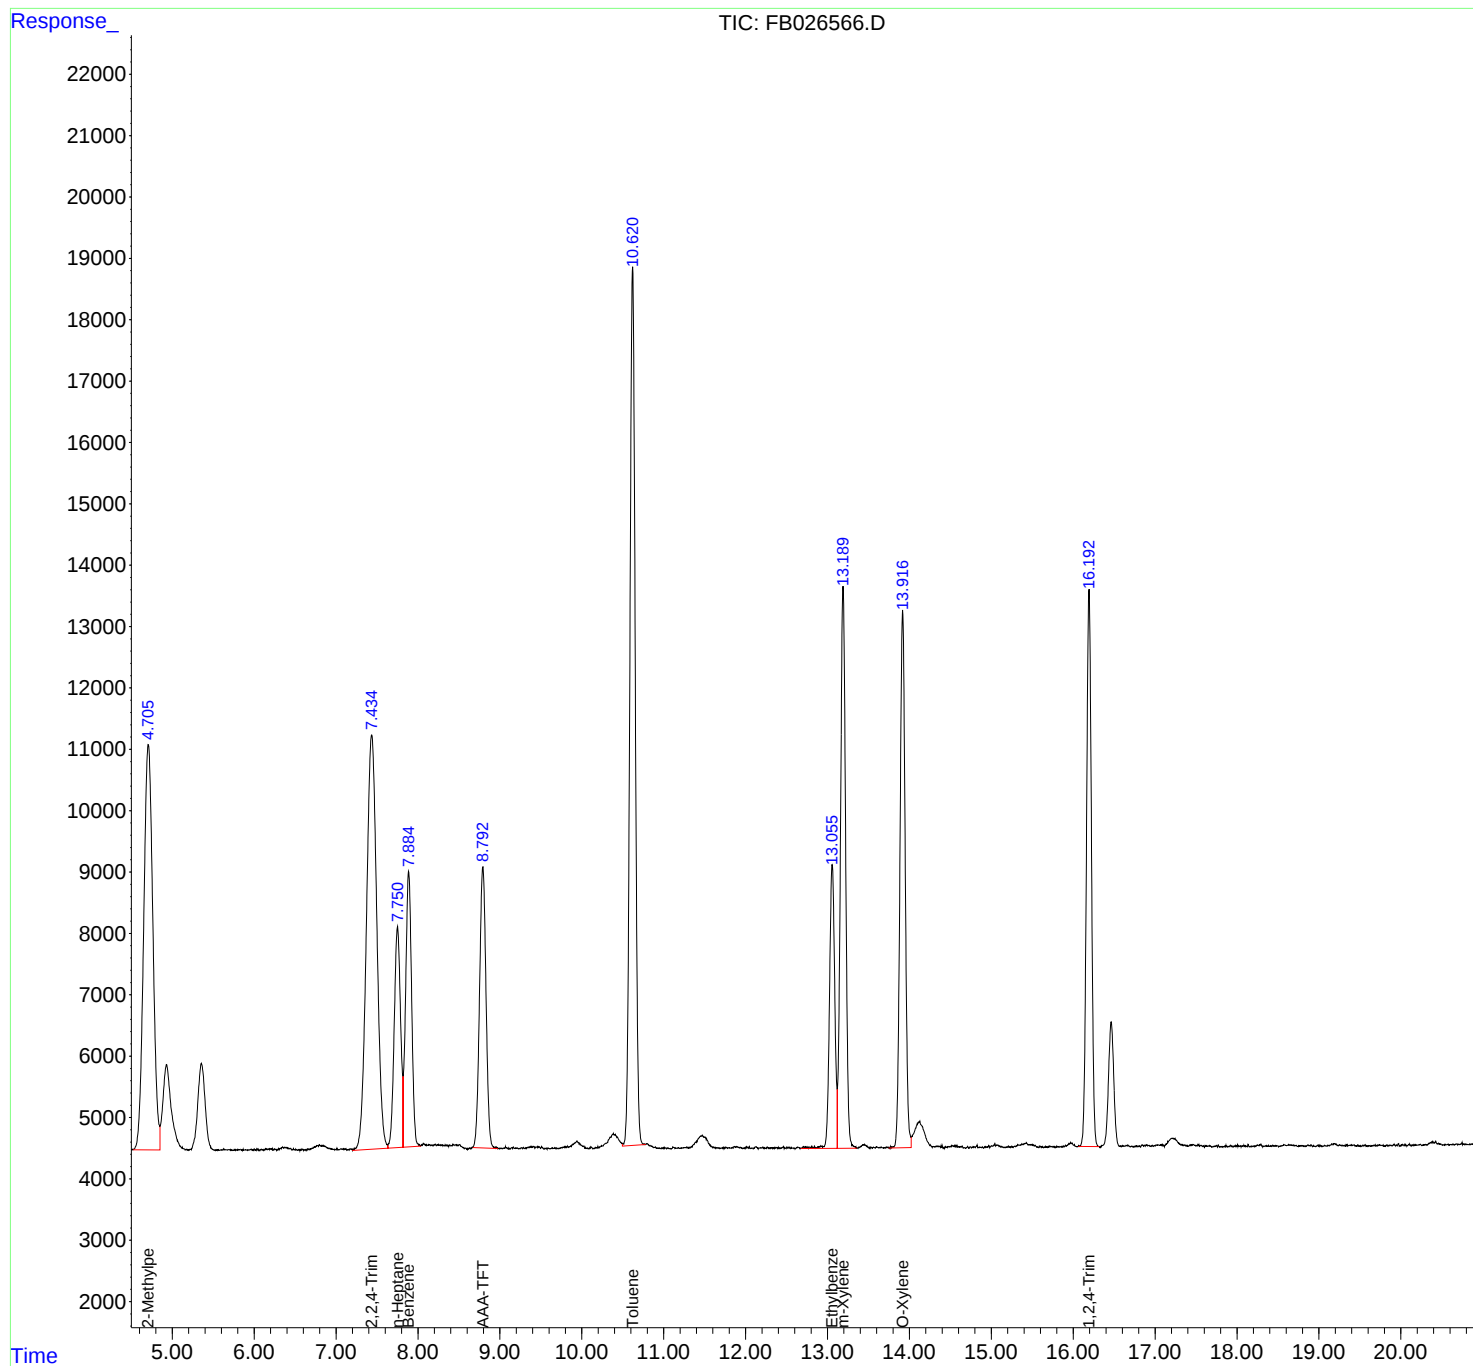


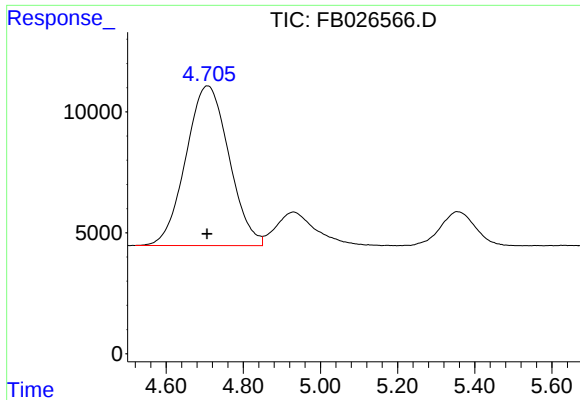

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 512903
Conc: 29.47 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-123-1-40-57MSD

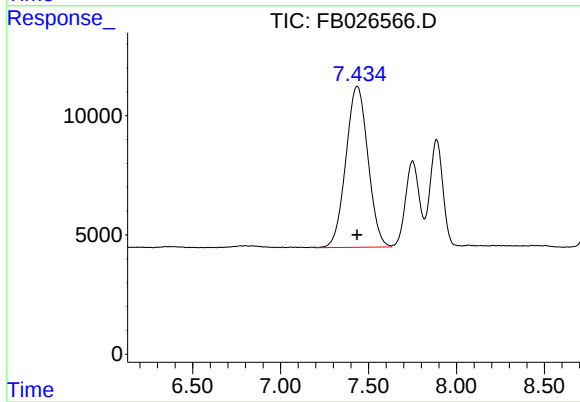


#2 2,2,4-Trimethylpentane

R.T.: 7.436 min
Delta R.T.: 0.000 min
Response: 589499
Conc: 29.73 ng/ml

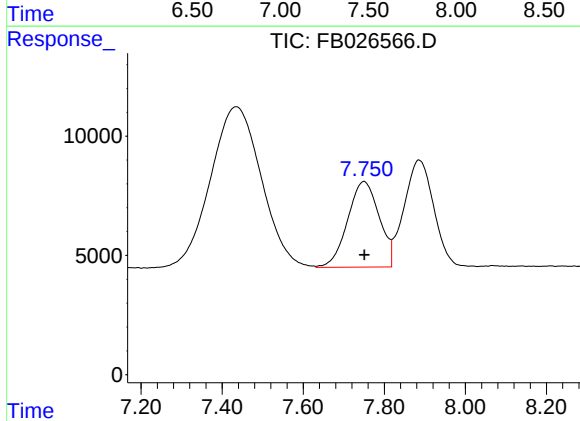


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 194151
Conc: 10.14 ng/ml

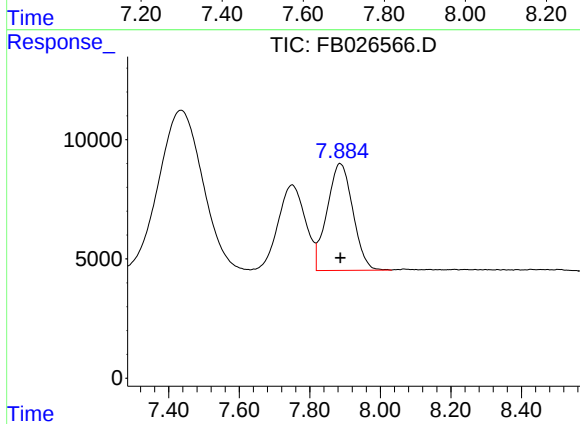

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 227847
Conc: 10.25 ng/ml

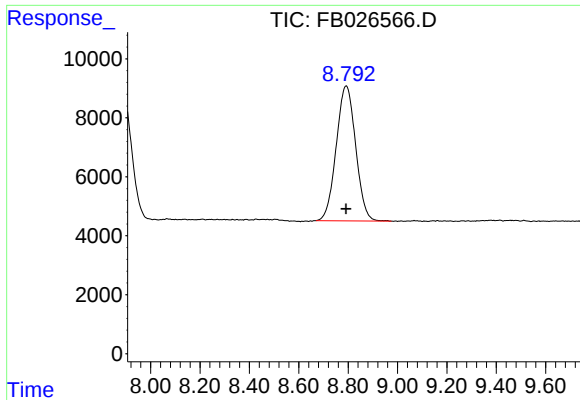

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.001 min
Response: 250621
Conc: 22.31 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-123-1-40-57MSD

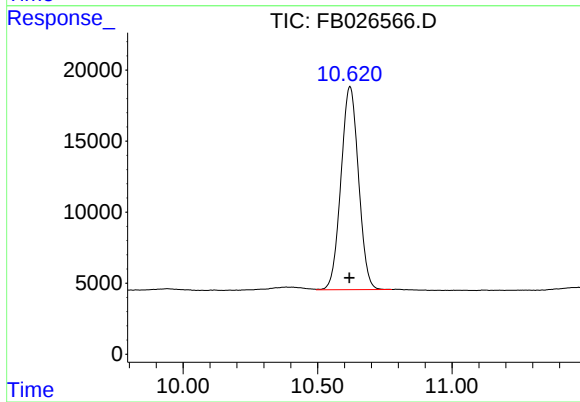


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.002 min
Response: 648877
Conc: 30.41 ng/ml

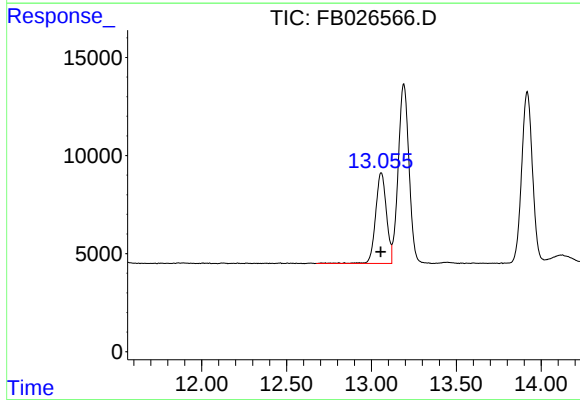


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.002 min
Response: 205569
Conc: 10.41 ng/ml

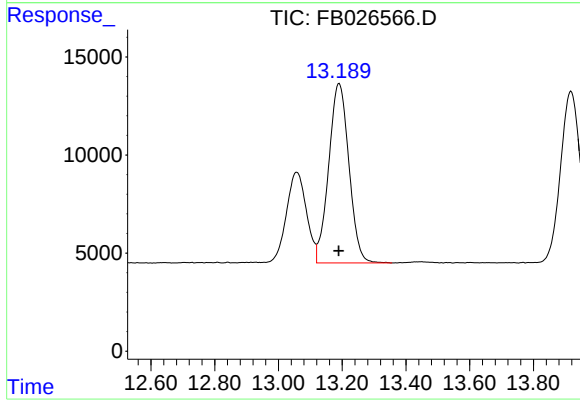

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.001 min
Response: 402989
Conc: 20.44 ng/ml

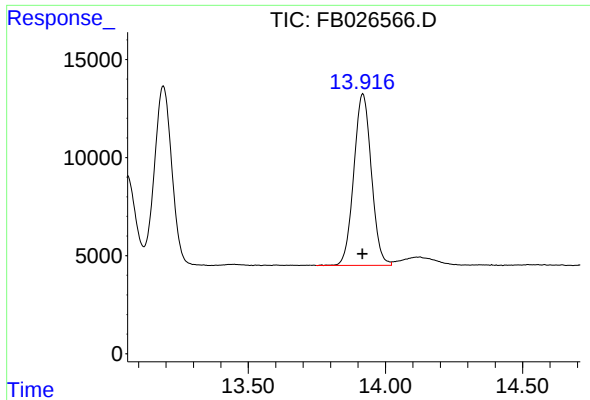

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.002 min
Response: 387787
Conc: 20.31 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-123-1-40-57MSD

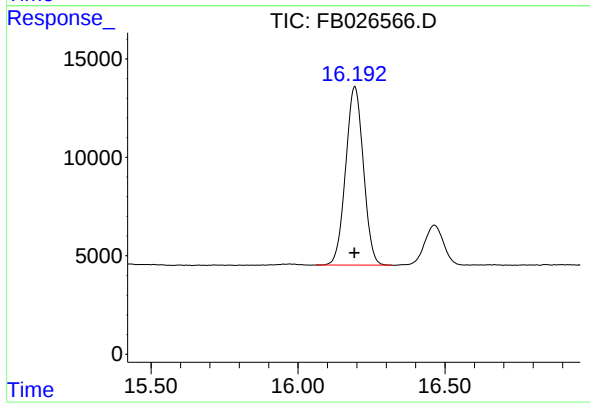

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.001 min
Response: 379705
Conc: 19.55 ng/ml