

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122921\
 Data File : FB026572.D
 Signal(s) : FID2B.CH
 Acq On : 29 Dec 2021 12:04
 Operator : AJ/MA
 Sample : M5245-01MS
 Misc : 5.06G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SASP2-123-1-65-72MS

Integration File: Calibration.e
 Quant Time: Dec 30 00:03:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
 Quant Title :
 QLast Update : Wed Dec 08 14:04:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	197051	17.539 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.714	450863	25.902 ng/ml
2) t 2,2,4-Trimethylpentane	7.437	566590	28.570 ng/ml
3) t n-Heptane	7.752	152823	7.983 ng/ml
4) t Benzene	7.889	187029	8.412 ng/ml
6) t Toluene	10.621	564829	26.470 ng/ml
7) t Ethylbenzene	13.058	183220	9.281 ng/ml
8) t m-Xylene	13.191	370750	18.805 ng/ml
9) t O-Xylene	13.918	370693	19.411 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	398143	20.494 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122921\
Data File : FB026572.D
Signal(s) : FID2B.CH
Acq On : 29 Dec 2021 12:04
Operator : AJ/MA
Sample : M5245-01MS
Misc : 5.06G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SASP2-123-1-65-72MS

Integration File: Calibration.e
Quant Time: Dec 30 00:03:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
Quant Title :
QLast Update : Wed Dec 08 14:04:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

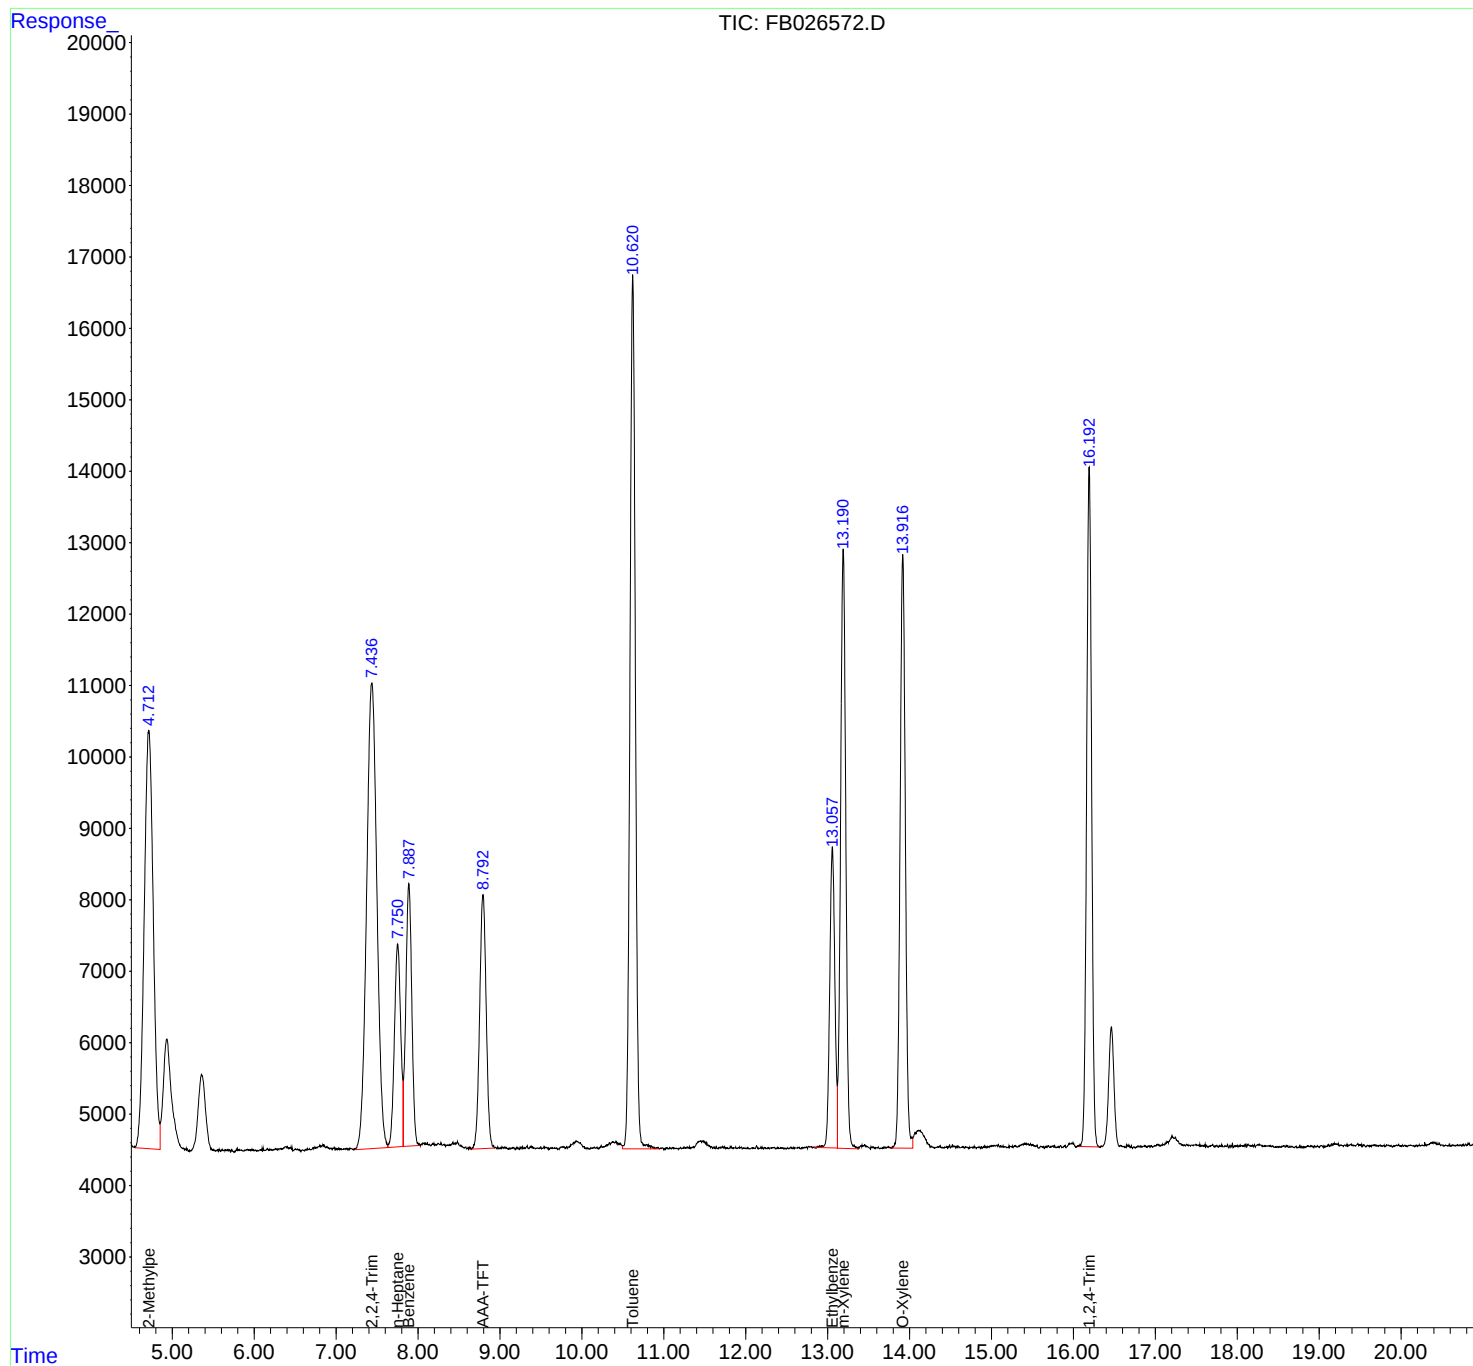


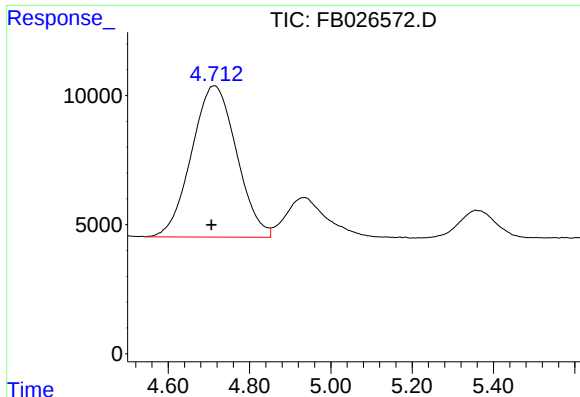

#1 2-Methylpentane


R.T.: 4.714 min
Delta R.T.: 0.008 min
Response: 450863
Conc: 25.90 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-123-1-65-72MS

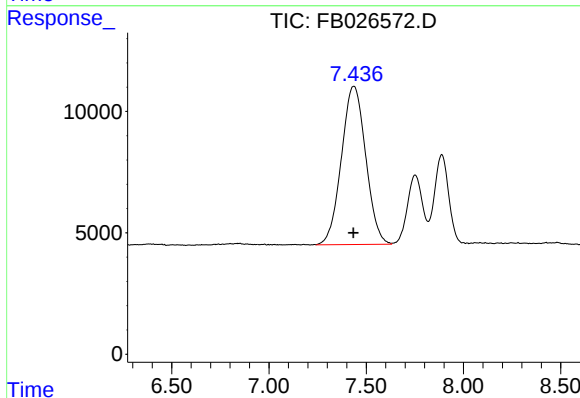


#2 2,2,4-Trimethylpentane

R.T.: 7.437 min
Delta R.T.: 0.002 min
Response: 566590
Conc: 28.57 ng/ml

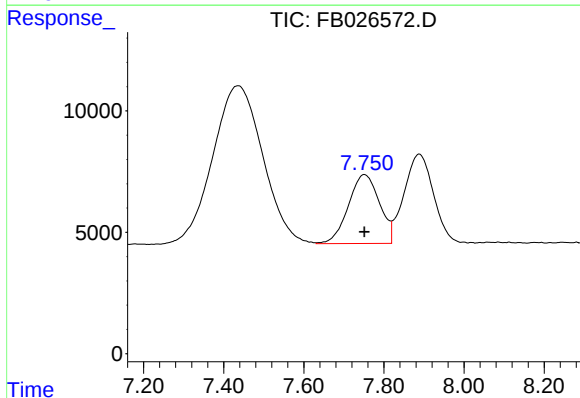


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 152823
Conc: 7.98 ng/ml

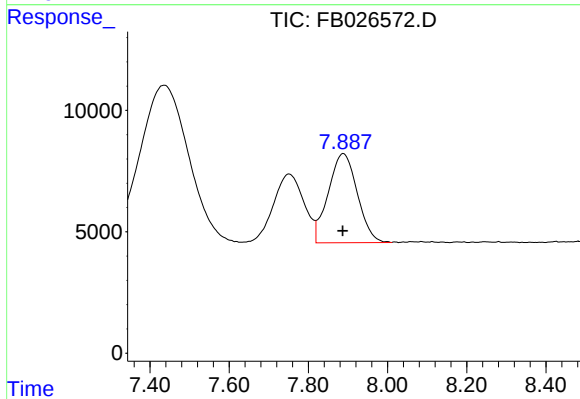

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.002 min
Response: 187029
Conc: 8.41 ng/ml

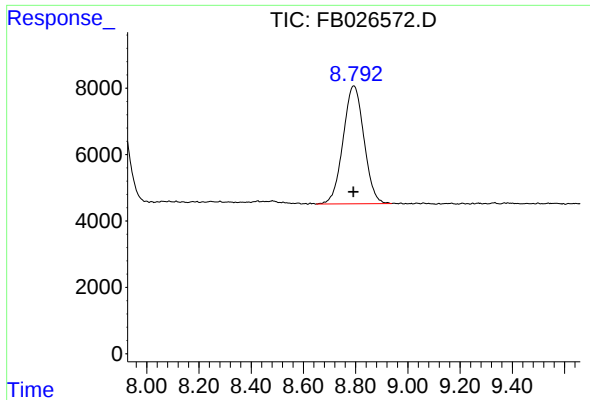

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.002 min
Response: 197051
Conc: 17.54 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-123-1-65-72MS

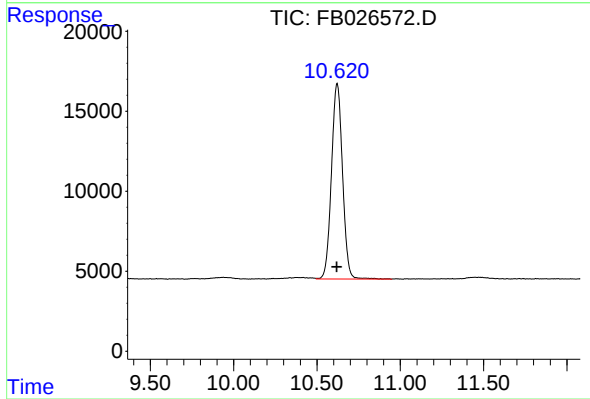


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.002 min
Response: 564829
Conc: 26.47 ng/ml

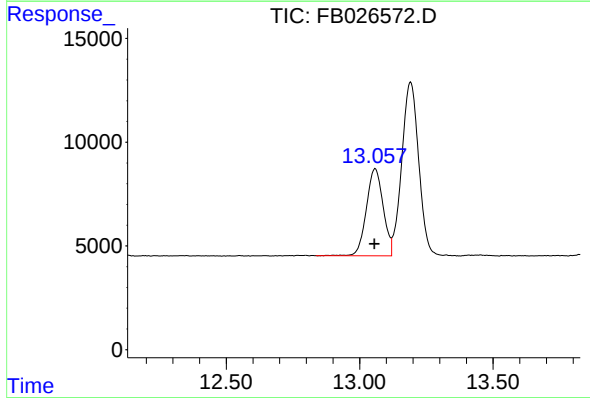


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.003 min
Response: 183220
Conc: 9.28 ng/ml

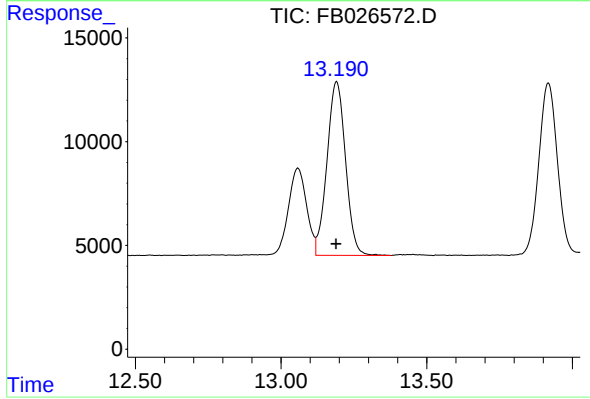

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.002 min
Response: 370750
Conc: 18.80 ng/ml

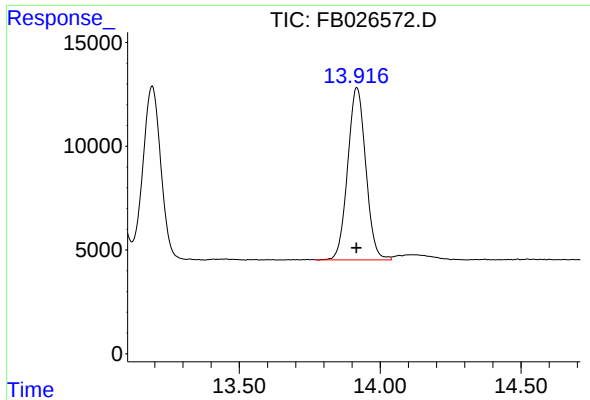

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.002 min
Response: 370693
Conc: 19.41 ng/ml

Instrument :
FID_B
ClientSampleId :
SASP2-123-1-65-72MS

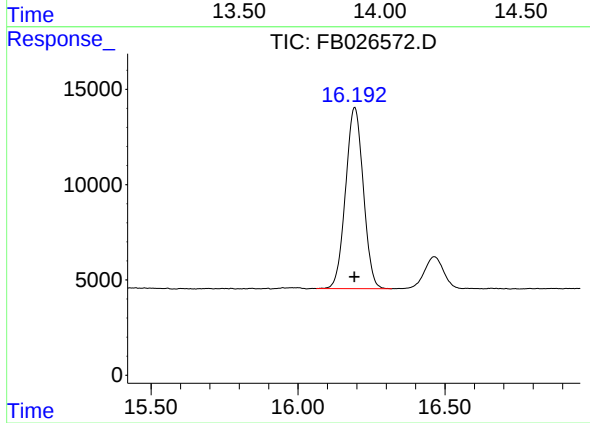

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.001 min
Response: 398143
Conc: 20.49 ng/ml