

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122921\
 Data File : FB026574.D
 Signal(s) : FID2B.CH
 Acq On : 29 Dec 2021 13:16
 Operator : AJ/MA
 Sample : BSF1229S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1229S1

Integration File: Calibration.e
 Quant Time: Dec 30 00:03:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
 Quant Title :
 QLast Update : Wed Dec 08 14:04:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	194112	17.278 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.713	443042	25.452 ng/ml
2) t 2,2,4-Trimethylpentane	7.436	548342	27.650 ng/ml
3) t n-Heptane	7.751	153719	8.030 ng/ml
4) t Benzene	7.888	188094	8.460 ng/ml
6) t Toluene	10.621	569687	26.698 ng/ml
7) t Ethylbenzene	13.058	183653	9.303 ng/ml
8) t m-Xylene	13.190	373569	18.948 ng/ml
9) t O-Xylene	13.918	371078	19.431 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	390282	20.090 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB122921\
Data File : FB026574.D
Signal(s) : FID2B.CH
Acq On : 29 Dec 2021 13:16
Operator : AJ/MA
Sample : BSF1229S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1229S1

Integration File: Calibration.e
Quant Time: Dec 30 00:03:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
Quant Title :
QLast Update : Wed Dec 08 14:04:26 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

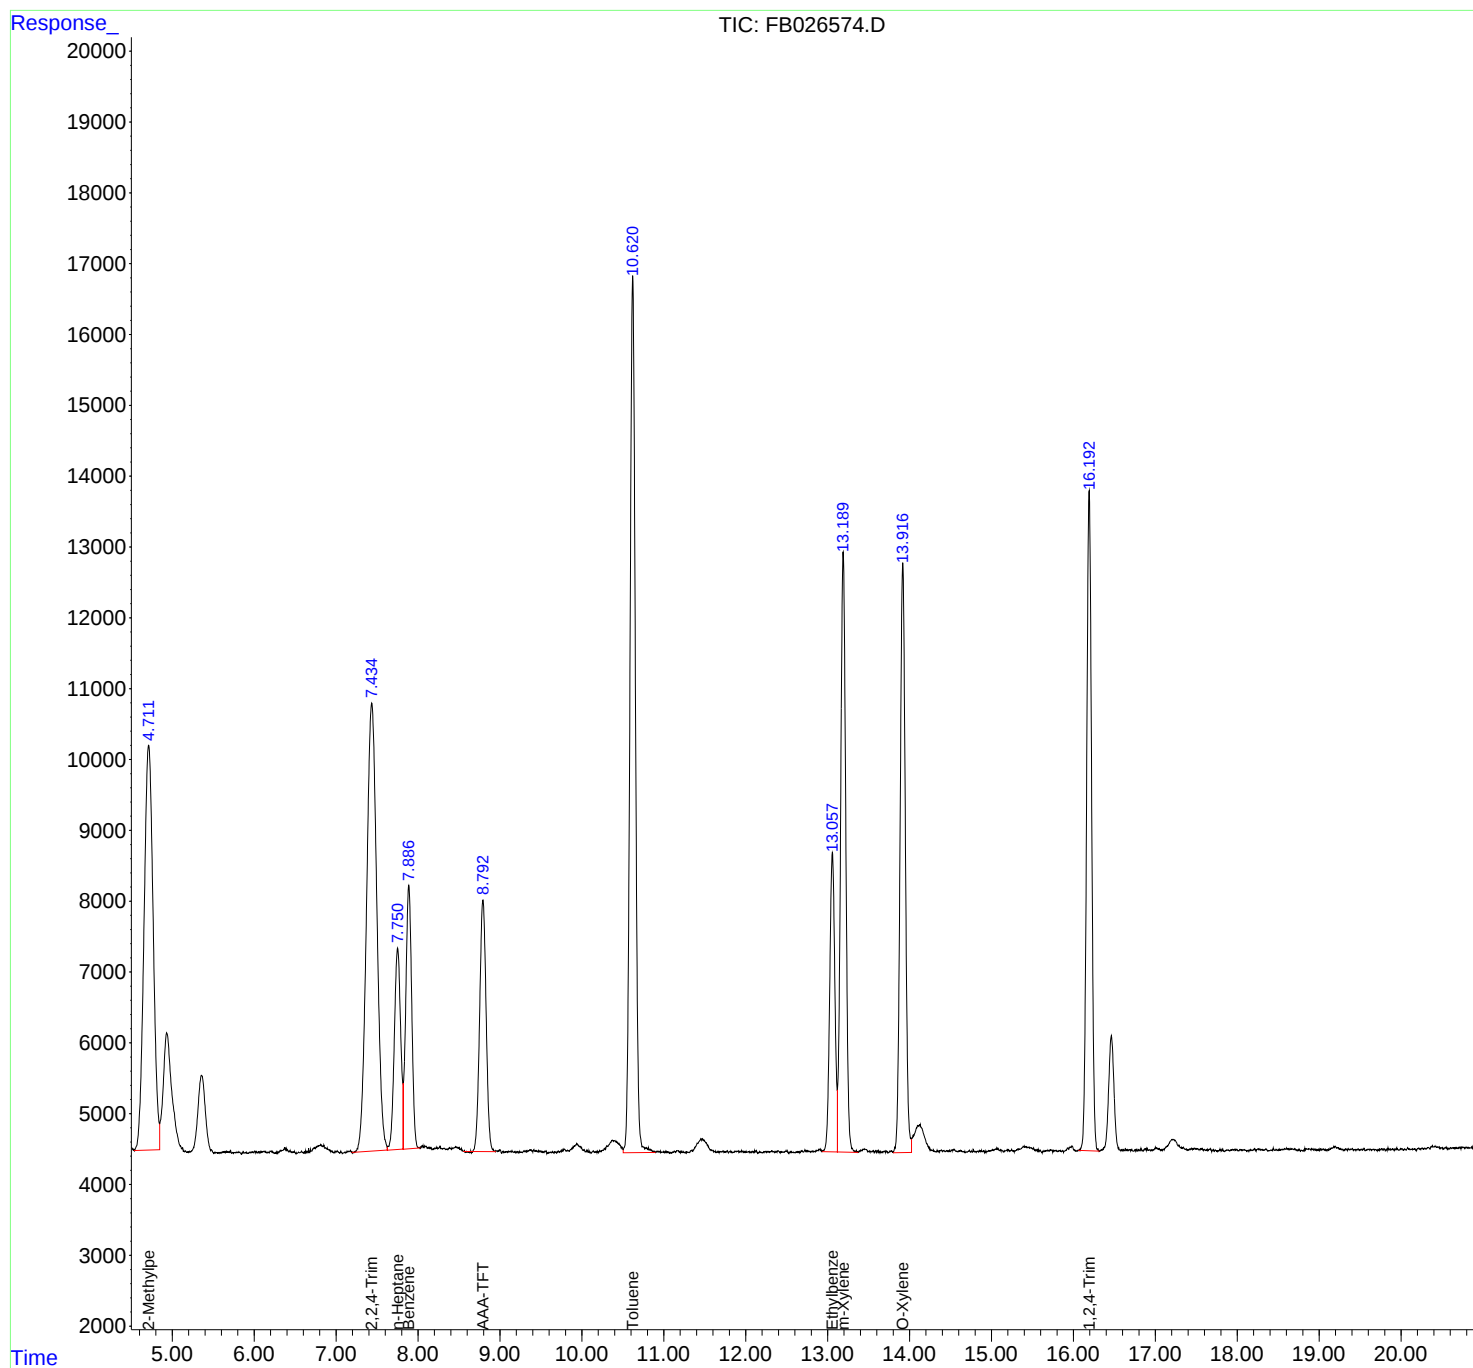


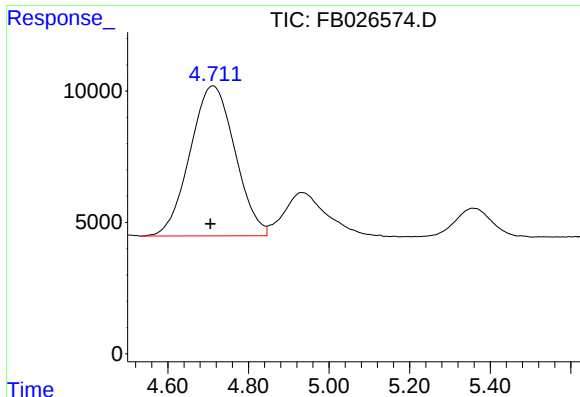

#1 2-Methylpentane


R.T.: 4.713 min
Delta R.T.: 0.007 min
Response: 443042
Conc: 25.45 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1229S1

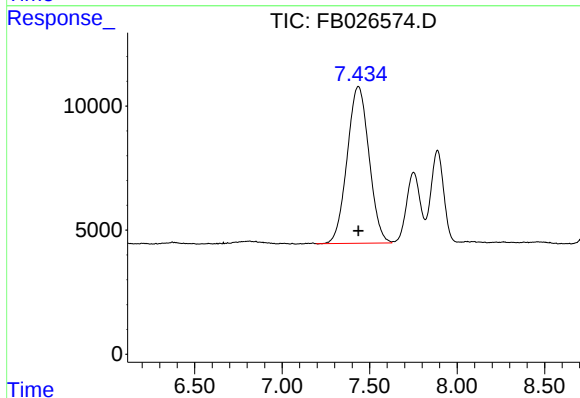


#2 2,2,4-Trimethylpentane

R.T.: 7.436 min
Delta R.T.: 0.000 min
Response: 548342
Conc: 27.65 ng/ml

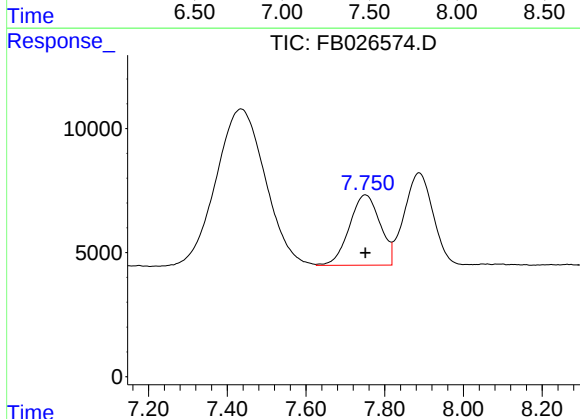


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 153719
Conc: 8.03 ng/ml

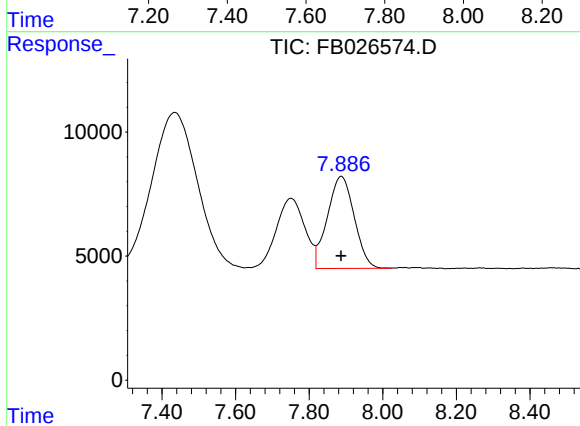

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.001 min
Response: 188094
Conc: 8.46 ng/ml

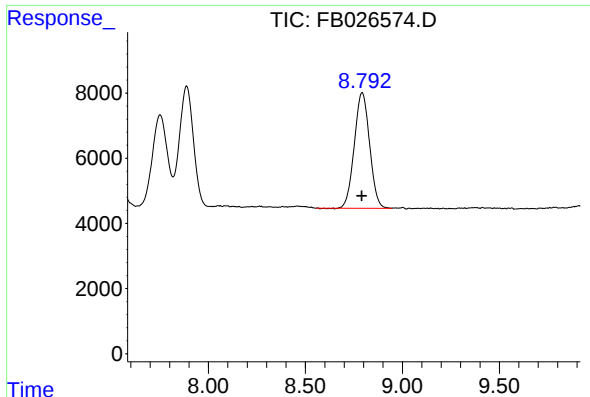

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.000 min
Response: 194112
Conc: 17.28 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1229S1

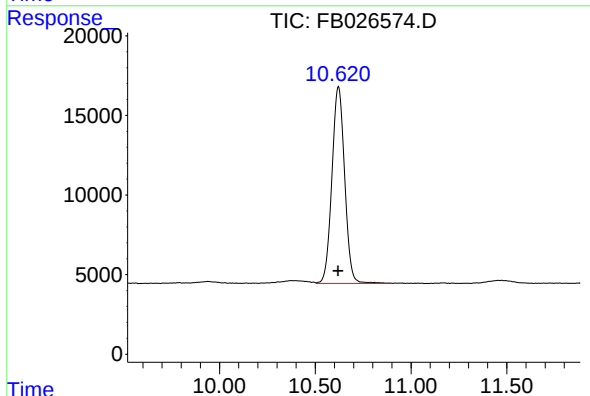


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.002 min
Response: 569687
Conc: 26.70 ng/ml

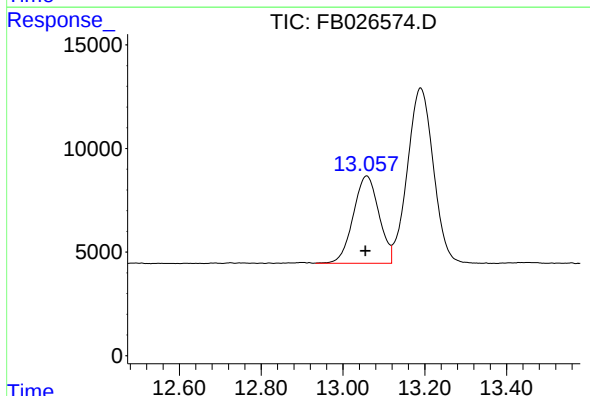


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.003 min
Response: 183653
Conc: 9.30 ng/ml

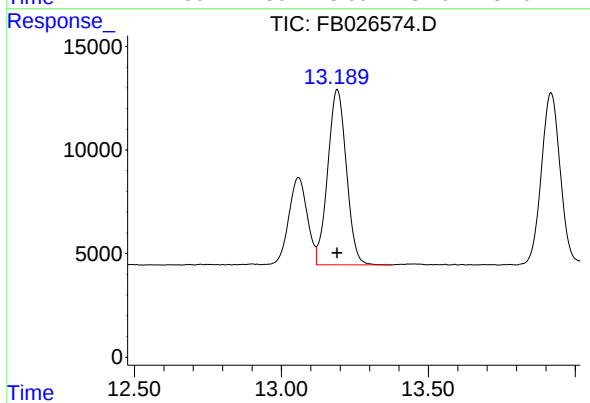

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.001 min
Response: 373569
Conc: 18.95 ng/ml

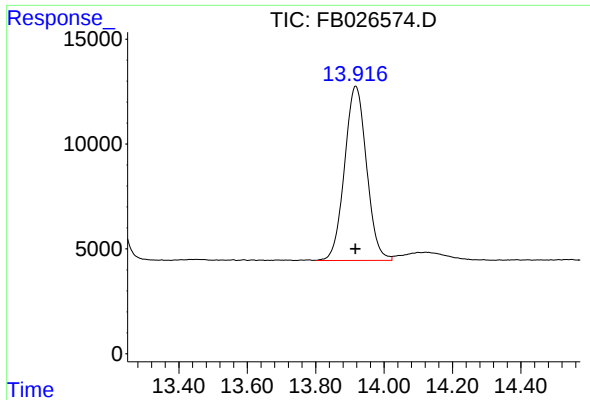

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.002 min
Response: 371078
Conc: 19.43 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1229S1

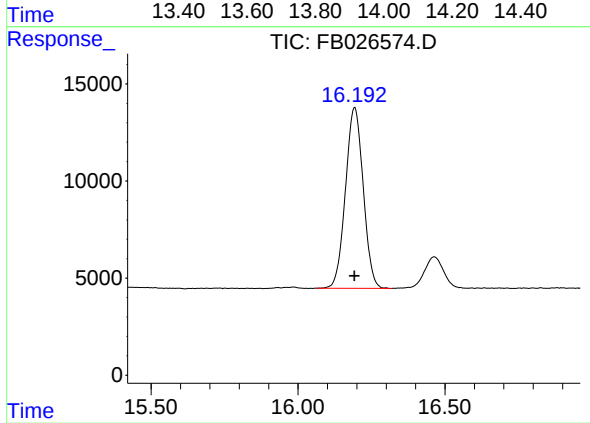

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.000 min
Response: 390282
Conc: 20.09 ng/ml