

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB123019\
 Data File : FB023339.D
 Signal(s) : FID2B.CH
 Acq On : 30 Dec 2019 10:40
 Operator : DD/AJ
 Sample : BSF1230S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 31 00:38:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	473477	19.966 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	944862	30.529 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	1049230	31.409 ng/ml
3) t n-Heptane	7.756	341805	10.362 ng/ml
4) t Benzene	7.891	401154	10.046 ng/ml
6) t Toluene	10.629	1190763	30.926 ng/ml
7) t Ethylbenzene	13.069	378859	10.438 ng/ml
8) t m-Xylene	13.202	730316	21.039 ng/ml
9) t O-Xylene	13.929	702619	20.860 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	588774	20.984 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB123019\
Data File : FB023339.D
Signal(s) : FID2B.CH
Acq On : 30 Dec 2019 10:40
Operator : DD/AJ
Sample : BSF1230S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 31 00:38:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

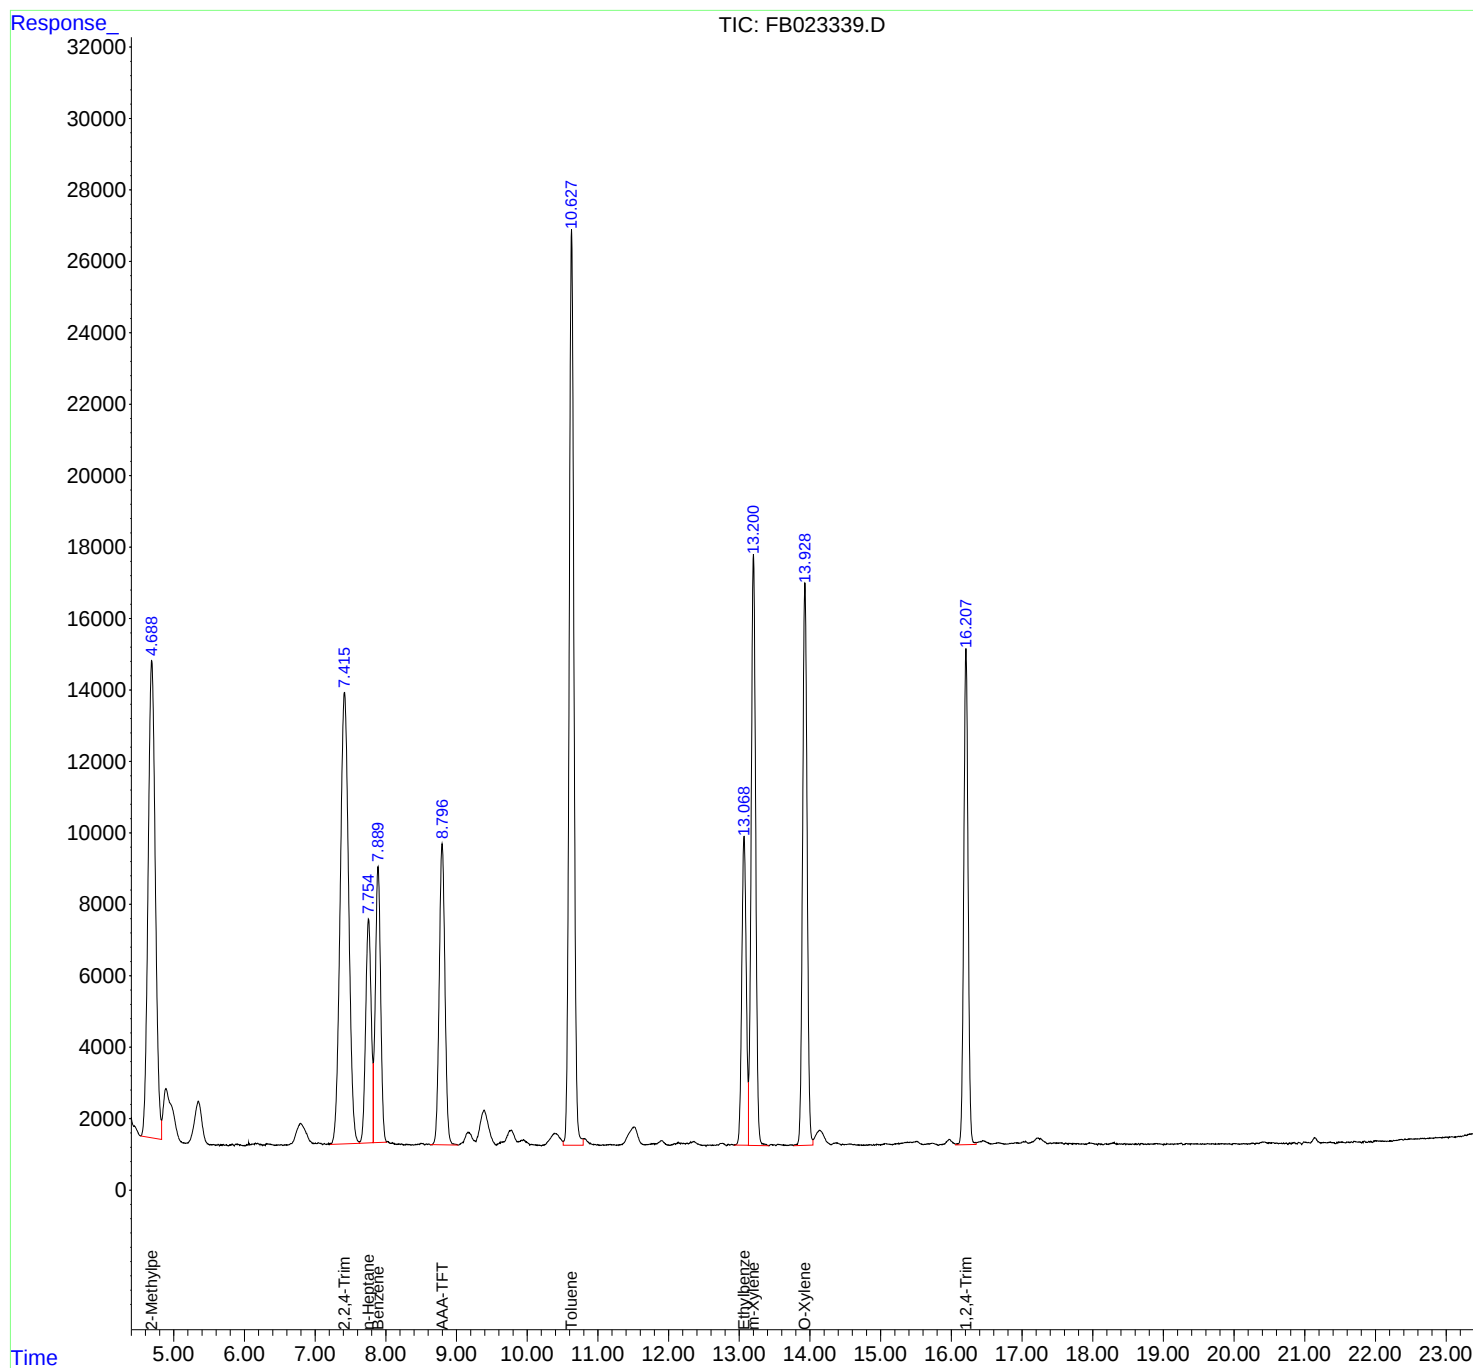

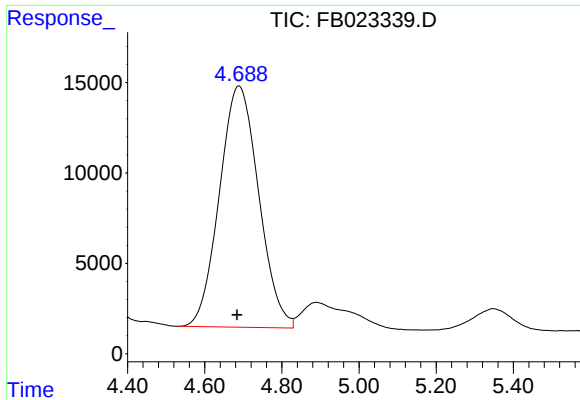


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: 0.005 min
Response: 944862
Conc: 30.53 ng/ml

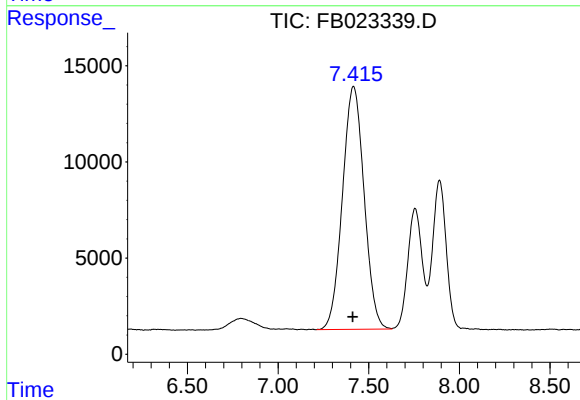


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.005 min
Response: 1049230
Conc: 31.41 ng/ml

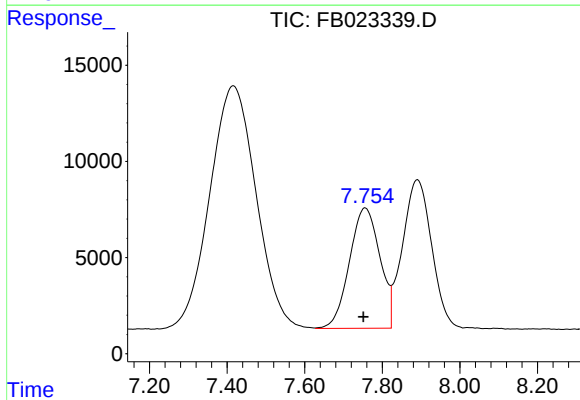


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: 0.004 min
Response: 341805
Conc: 10.36 ng/ml

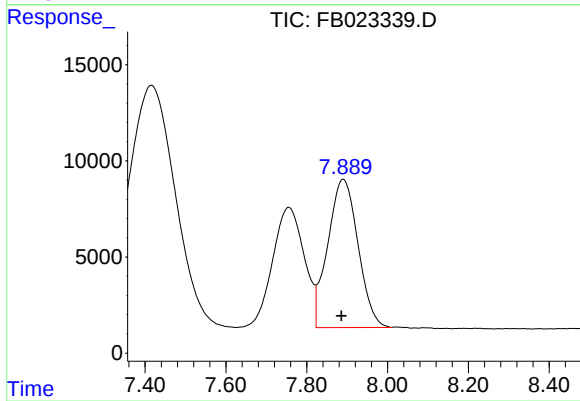


#4 Benzene

R.T.: 7.891 min
Delta R.T.: 0.004 min
Response: 401154
Conc: 10.05 ng/ml

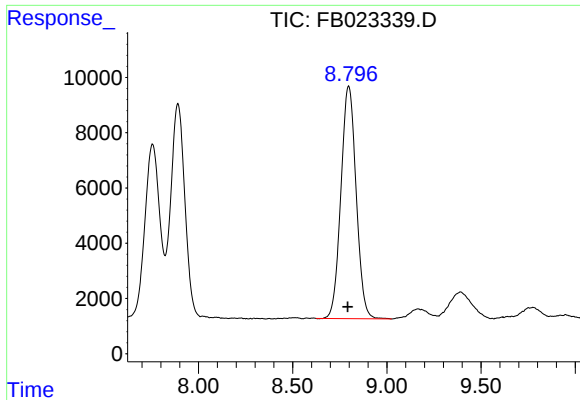


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: 0.004 min
Response: 473477
Conc: 19.97 ng/ml

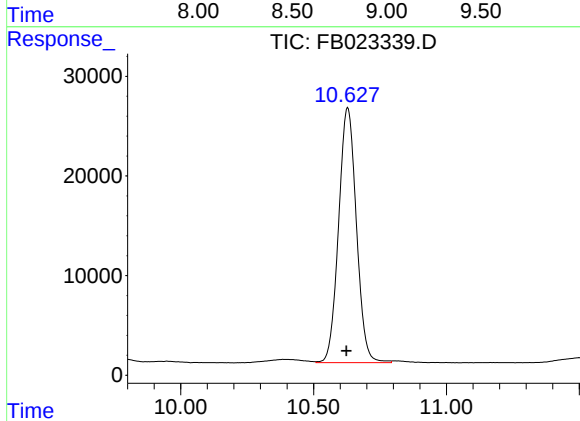


#6 Toluene

R.T.: 10.629 min
Delta R.T.: 0.005 min
Response: 1190763
Conc: 30.93 ng/ml

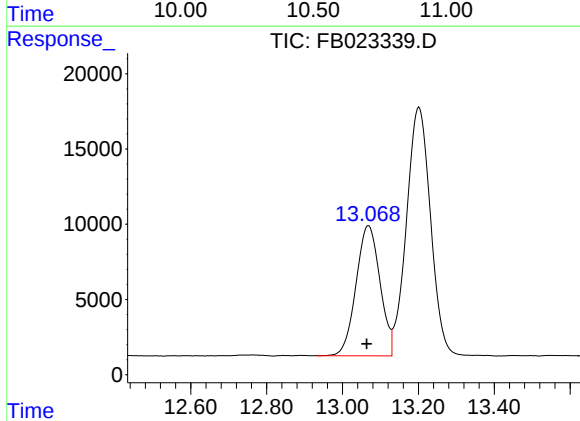


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.005 min
Response: 378859
Conc: 10.44 ng/ml

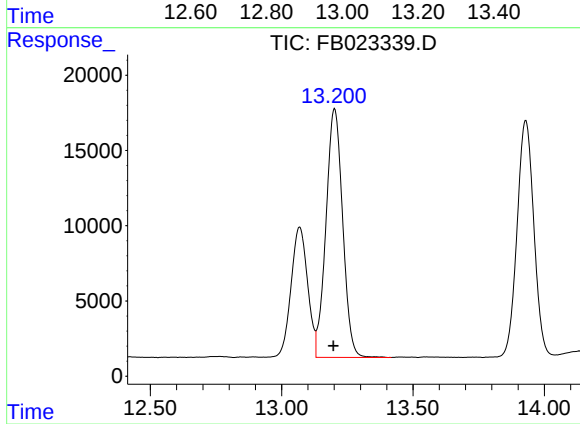


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: 0.004 min
Response: 730316
Conc: 21.04 ng/ml

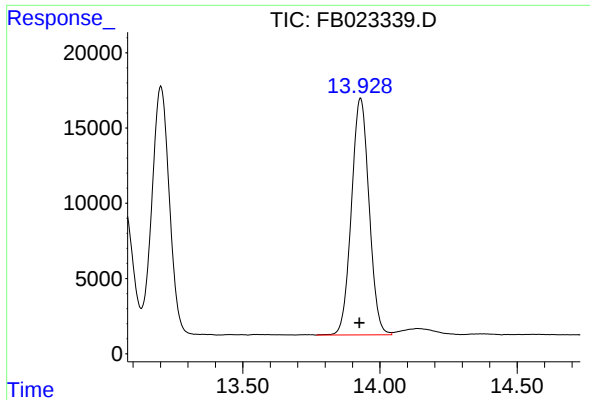

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: 0.004 min
Response: 702619
Conc: 20.86 ng/ml

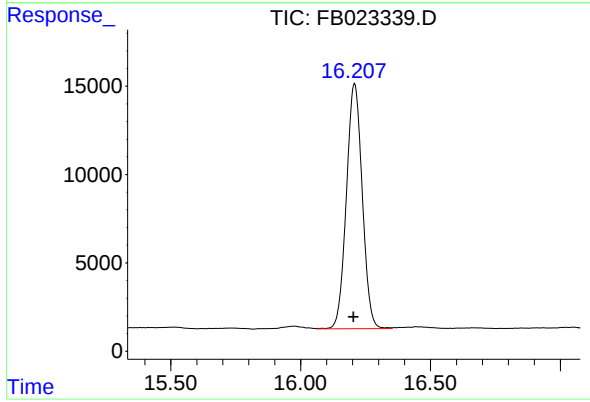

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: 0.005 min
Response: 588774
Conc: 20.98 ng/ml