

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB123019\
 Data File : FB023342.D
 Signal(s) : FID2B.CH
 Acq On : 30 Dec 2019 13:07
 Operator : DD/AJ
 Sample : K6441-07MSD
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 31 00:38:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
 Quant Title :
 QLast Update : Thu Dec 19 12:43:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	462809	19.516 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	842163	27.211 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	899969	26.941 ng/ml
3) t n-Heptane	7.757	293383	8.894 ng/ml
4) t Benzene	7.891	393100	9.844 ng/ml
6) t Toluene	10.630	1108885	28.799 ng/ml
7) t Ethylbenzene	13.069	352717	9.718 ng/ml
8) t m-Xylene	13.203	665388	19.169 ng/ml
9) t O-Xylene	13.930	641821	19.055 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	528375	18.831 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB123019\
Data File : FB023342.D
Signal(s) : FID2B.CH
Acq On : 30 Dec 2019 13:07
Operator : DD/AJ
Sample : K6441-07MSD
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 31 00:38:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB121919.M
Quant Title :
QLast Update : Thu Dec 19 12:43:06 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

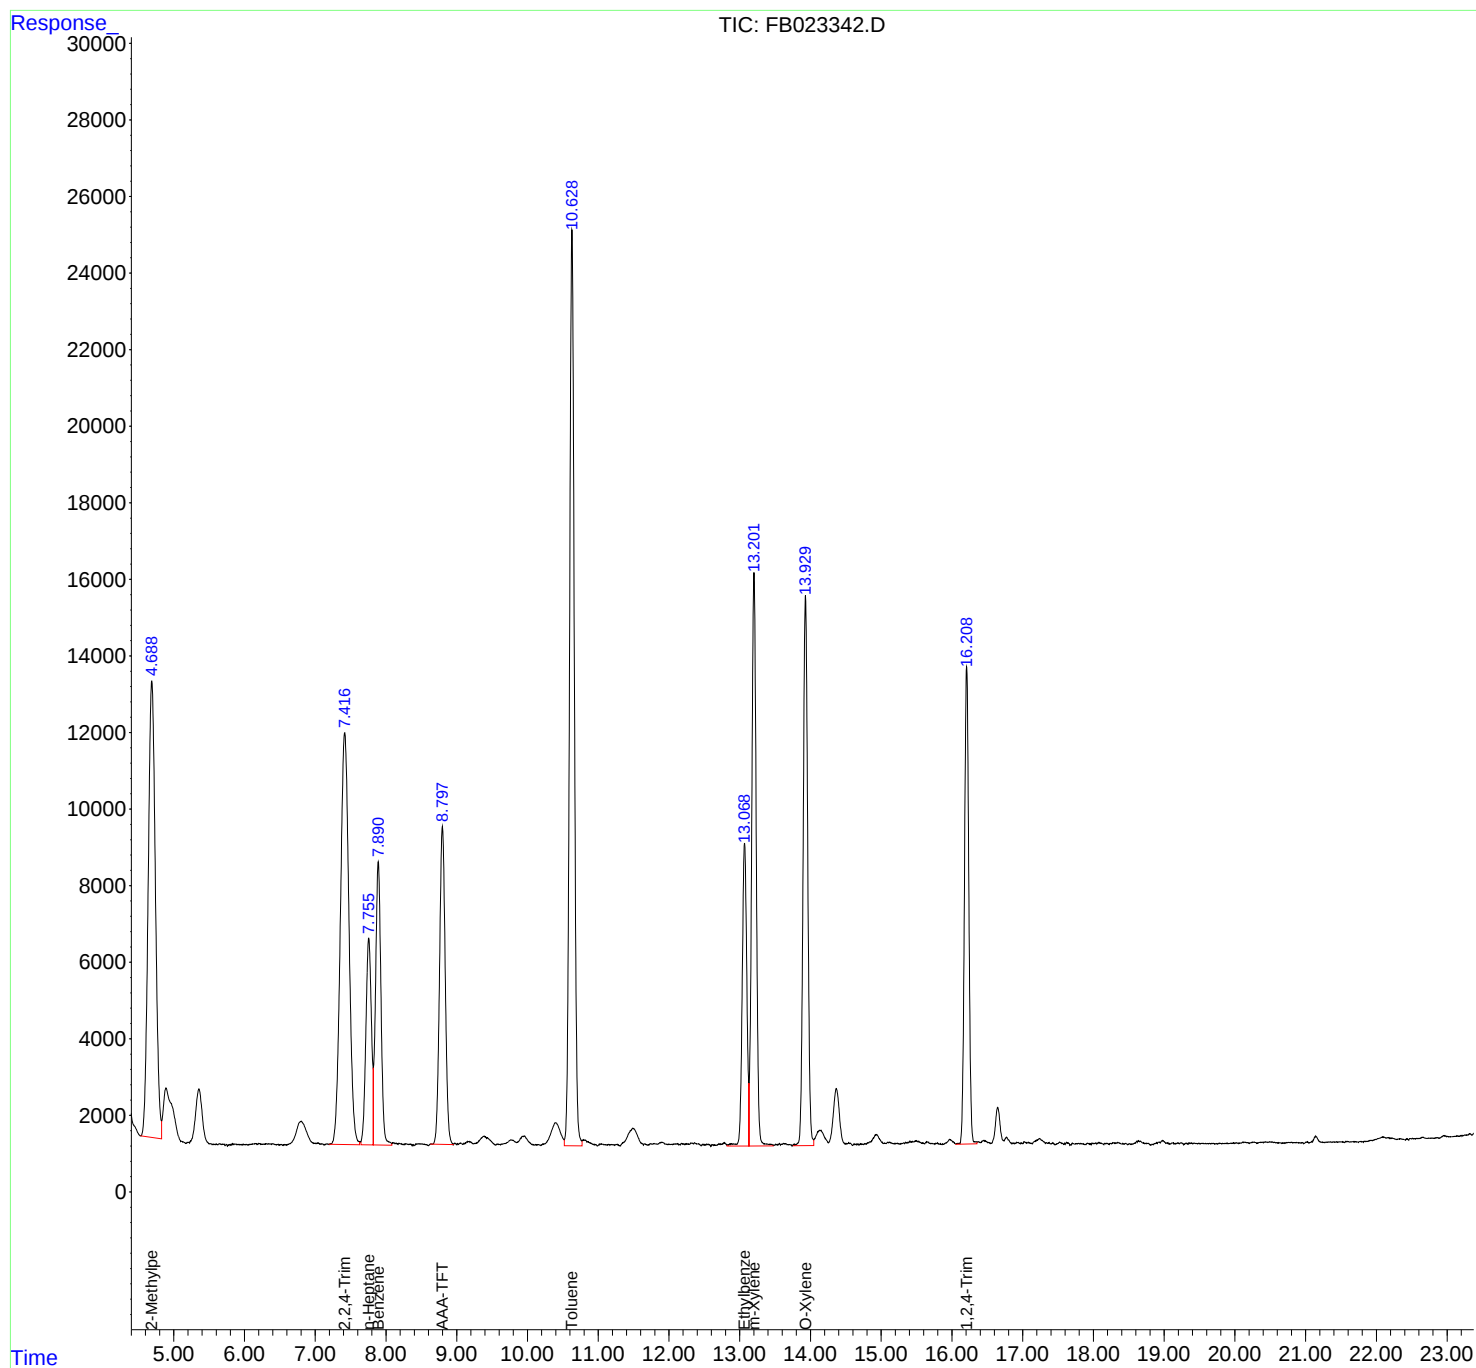

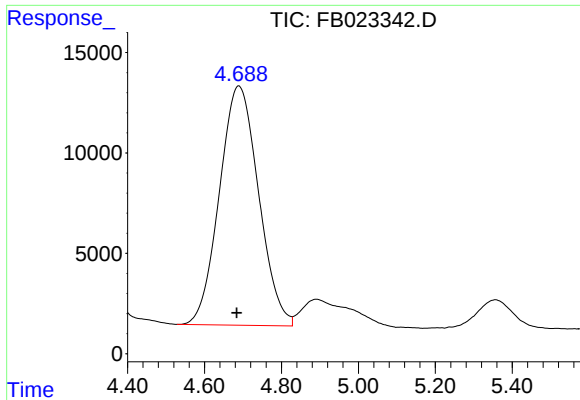


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: 0.006 min
Response: 842163
Conc: 27.21 ng/ml

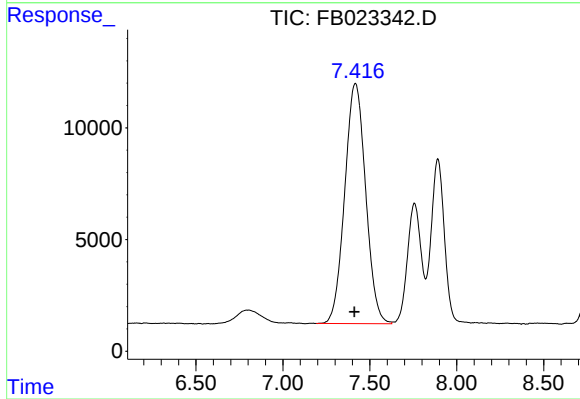


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.006 min
Response: 899969
Conc: 26.94 ng/ml

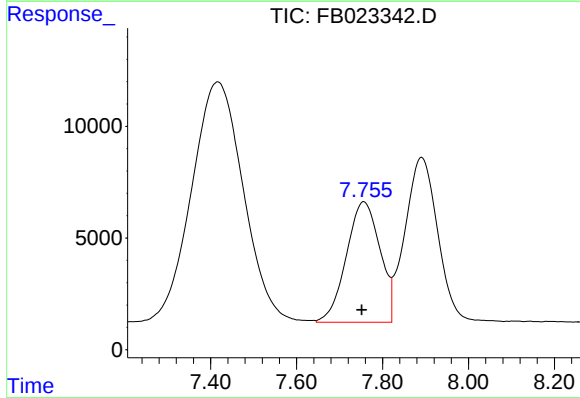


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.005 min
Response: 293383
Conc: 8.89 ng/ml

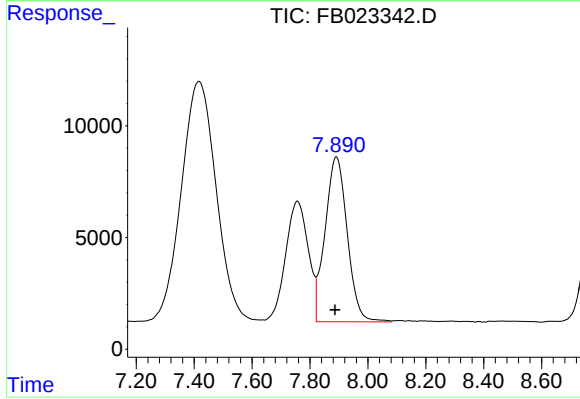


#4 Benzene

R.T.: 7.891 min
Delta R.T.: 0.005 min
Response: 393100
Conc: 9.84 ng/ml

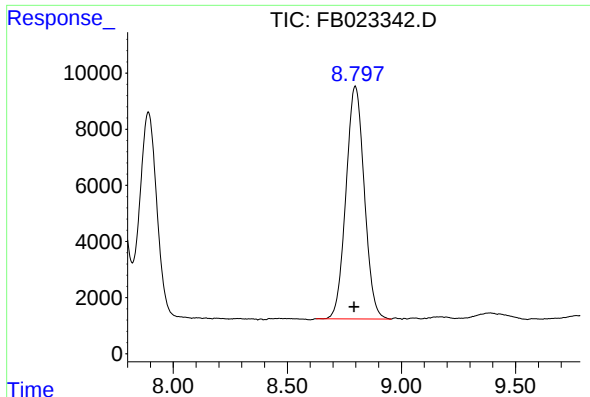


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.005 min
Response: 462809
Conc: 19.52 ng/ml

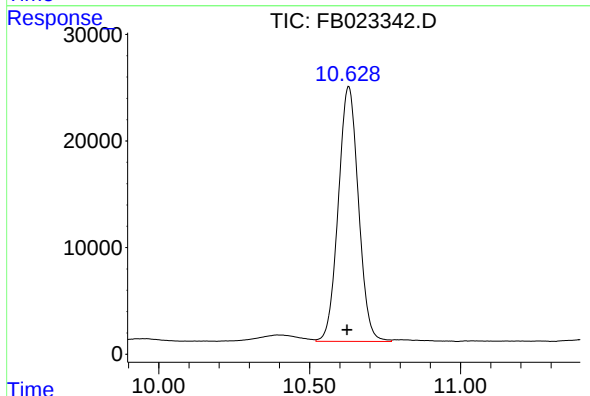


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.006 min
Response: 1108885
Conc: 28.80 ng/ml

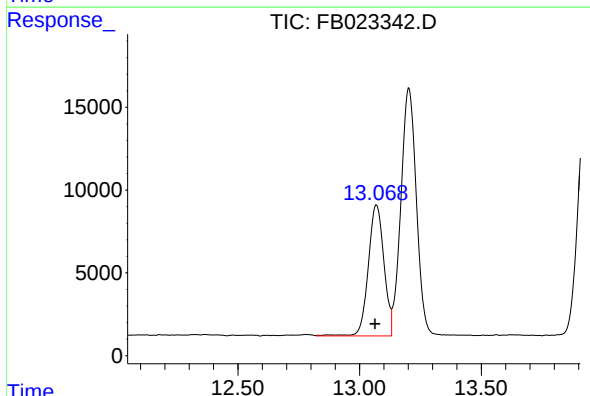


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: 0.005 min
Response: 352717
Conc: 9.72 ng/ml

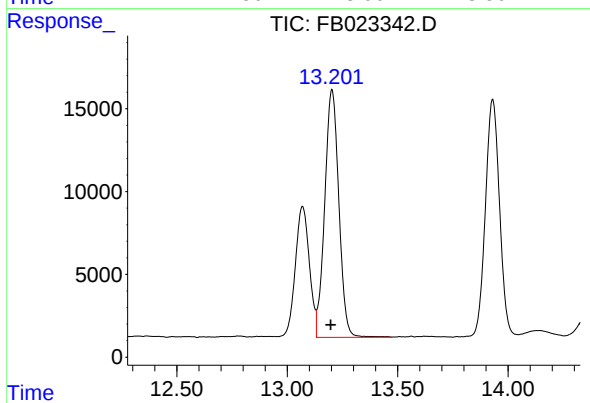


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: 0.005 min
Response: 665388
Conc: 19.17 ng/ml

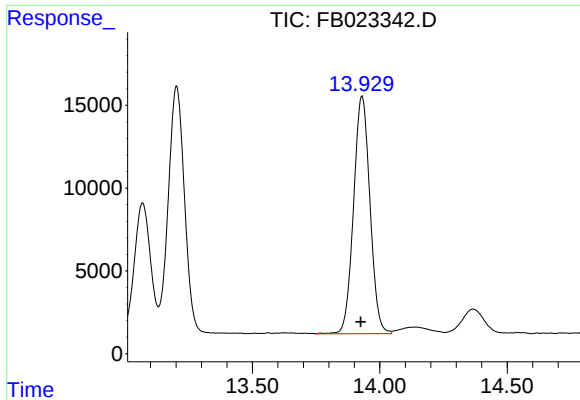

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: 0.005 min
Response: 641821
Conc: 19.05 ng/ml

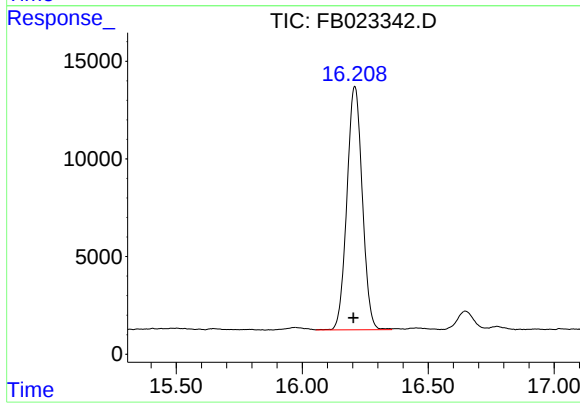

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.006 min
Response: 528375
Conc: 18.83 ng/ml