

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB123020\
 Data File : FB025363.D
 Signal(s) : FID2B.CH
 Acq On : 30 Dec 2020 17:17
 Operator : DD/AJ
 Sample : BSW1230W1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF1230W1

Integration File: Calibration.e
 Quant Time: Dec 31 00:18:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
 Quant Title :
 QLast Update : Wed Dec 02 15:24:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	468362	22.278 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	974938	32.429 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	1038552	34.516 ng/ml
3) t n-Heptane	7.757	339286	11.458 ng/ml
4) t Benzene	7.892	406231	10.983 ng/ml
6) t Toluene	10.629	1144996	32.583 ng/ml
7) t Ethylbenzene	13.069	356792	10.923 ng/ml
8) t m-Xylene	13.202	716381	22.133 ng/ml
9) t O-Xylene	13.929	702242	22.214 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	601440	22.148 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB123020\
Data File : FB025363.D
Signal(s) : FID2B.CH
Acq On : 30 Dec 2020 17:17
Operator : DD/AJ
Sample : BSW1230W1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF1230W1

Integration File: Calibration.e
Quant Time: Dec 31 00:18:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120220.M
Quant Title :
QLast Update : Wed Dec 02 15:24:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

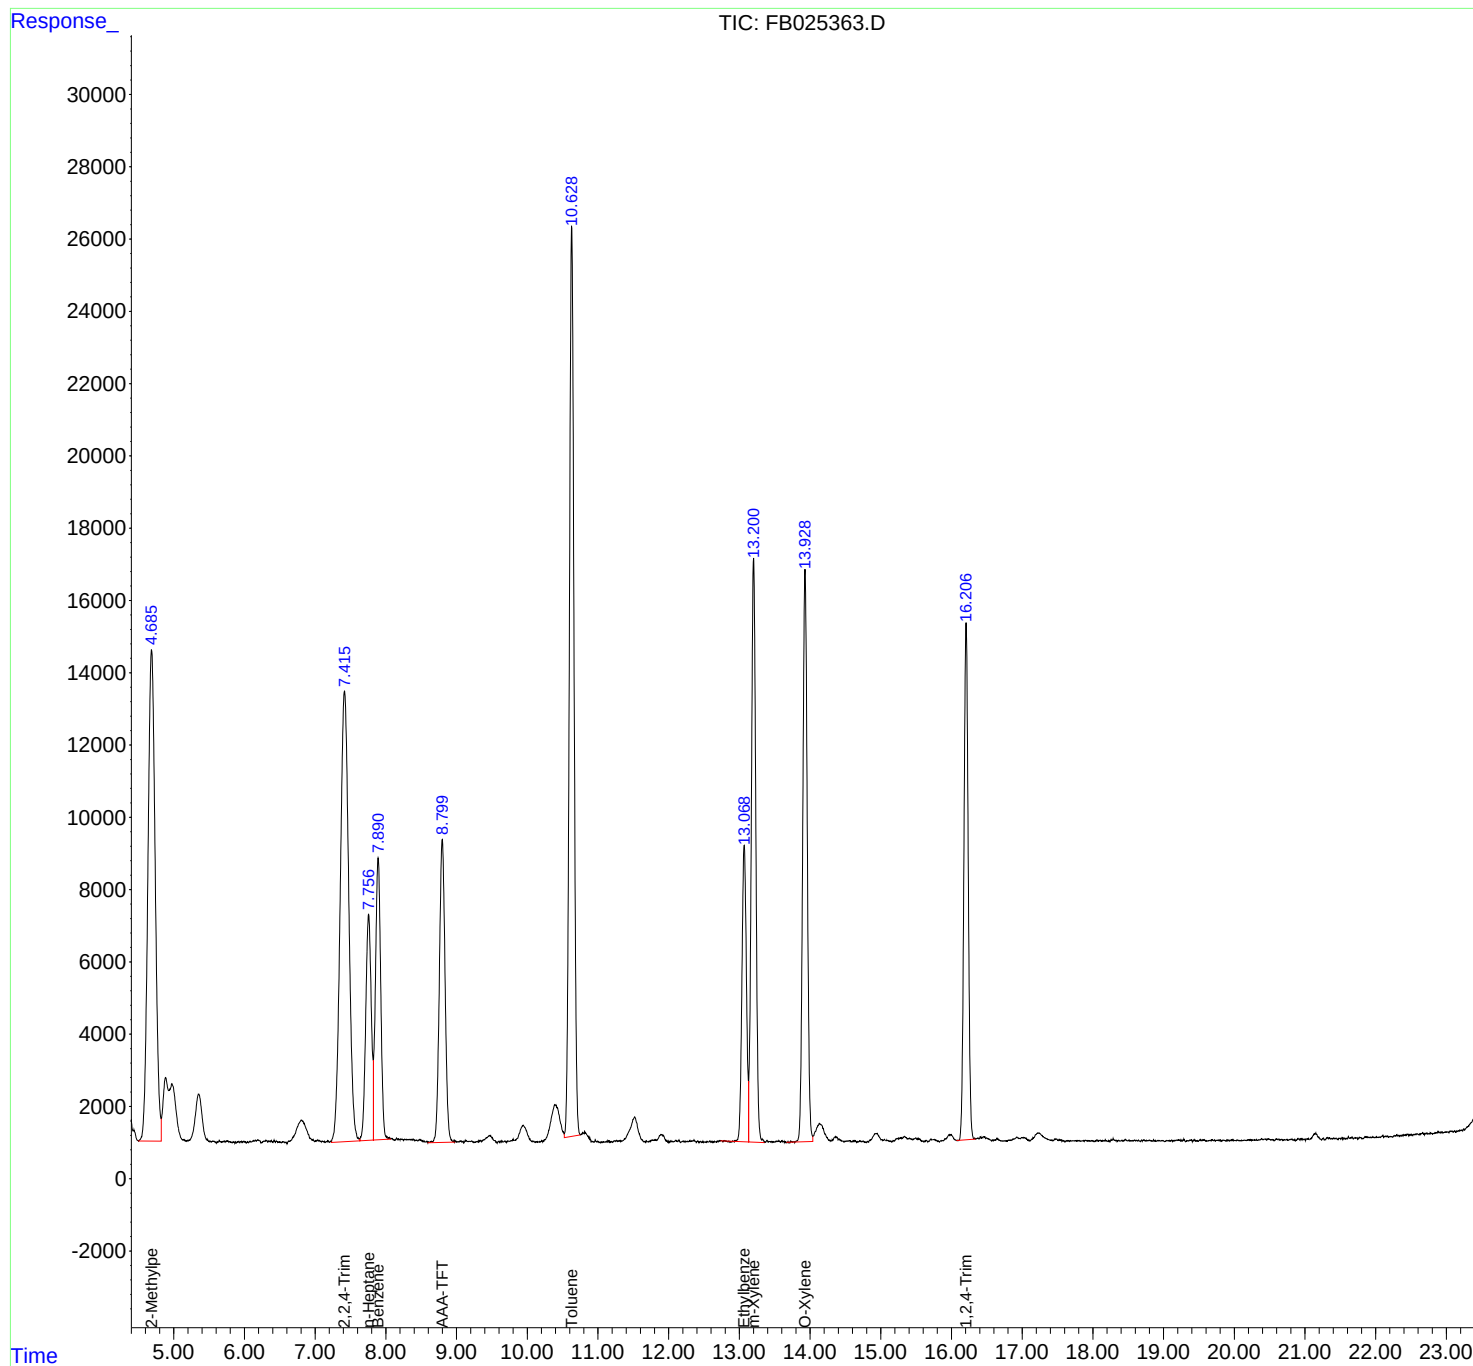


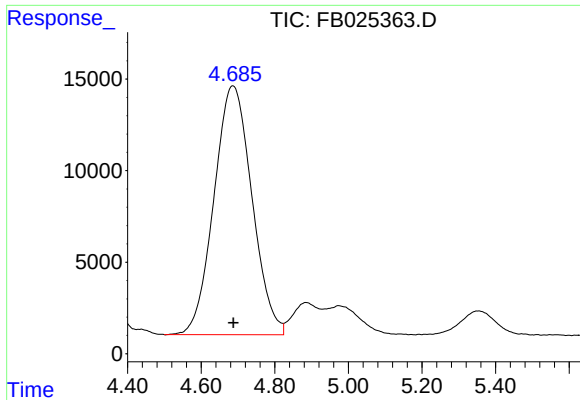

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: 0.000 min
Response: 974938
Conc: 32.43 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1230W1

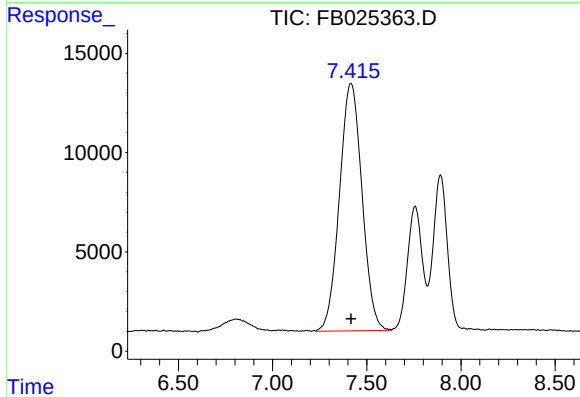


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 1038552
Conc: 34.52 ng/ml

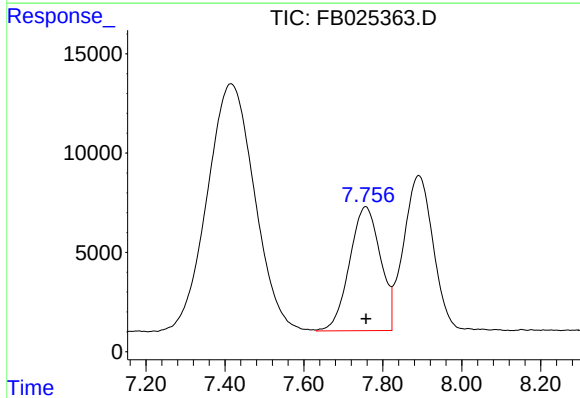


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: 0.000 min
Response: 339286
Conc: 11.46 ng/ml

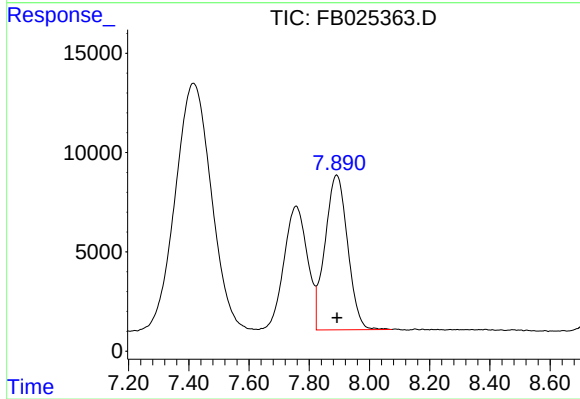

#4 Benzene


R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 406231
Conc: 10.98 ng/ml

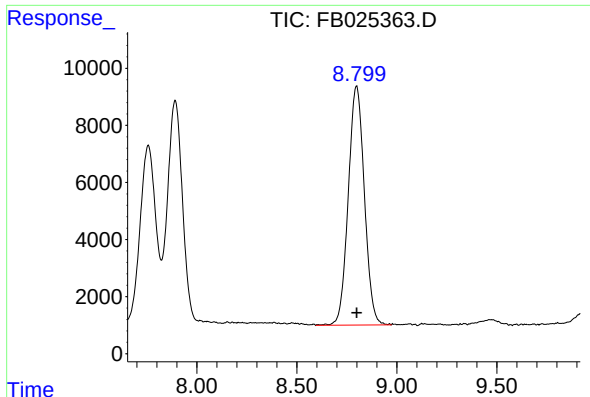

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 468362
Conc: 22.28 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1230W1

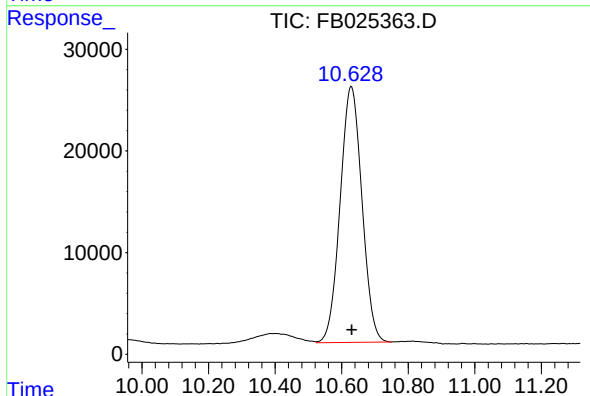


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.001 min
Response: 1144996
Conc: 32.58 ng/ml

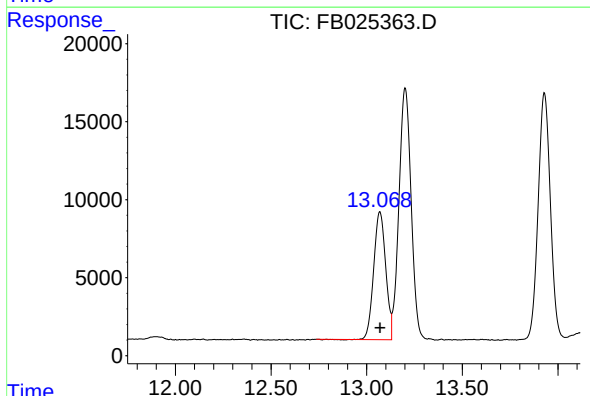


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.002 min
Response: 356792
Conc: 10.92 ng/ml

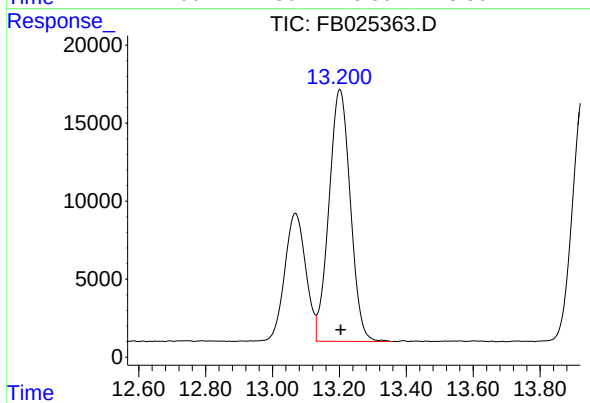

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: -0.002 min
Response: 716381
Conc: 22.13 ng/ml

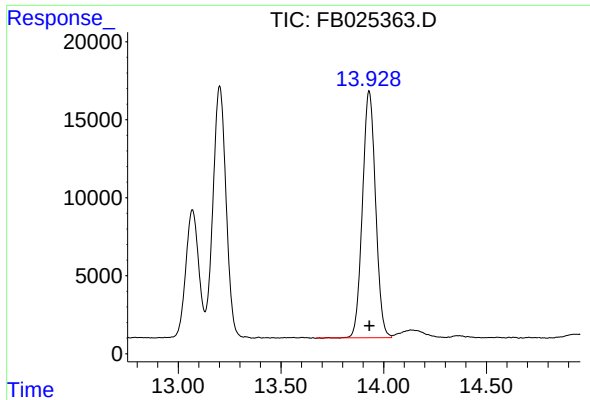

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.002 min
Response: 702242
Conc: 22.21 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF1230W1

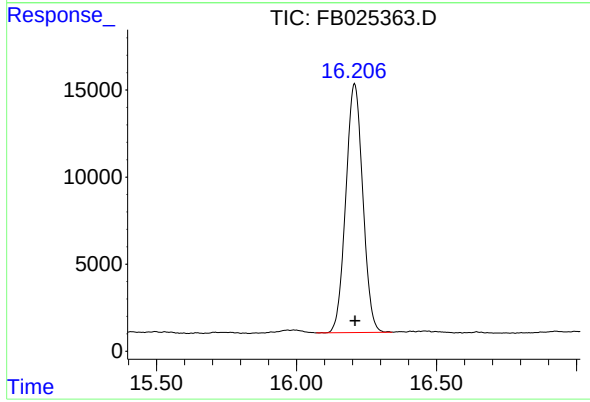

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.002 min
Response: 601440
Conc: 22.15 ng/ml