

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB123021\
 Data File : FB026578.D
 Signal(s) : FID2B.CH
 Acq On : 30 Dec 2021 13:11
 Operator : AJ/MA
 Sample : BSF1230S1
 Misc : 4.99G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 30 23:57:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
 Quant Title :
 QLast Update : Wed Dec 08 14:04:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.792	241493	21.495 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.708	459413	26.393 ng/ml
2) t	2,2,4-Trimethylpentane	7.435	544145	27.438 ng/ml
3) t	n-Heptane	7.750	172968	9.036 ng/ml
4) t	Benzene	7.888	201321	9.055 ng/ml
6) t	Toluene	10.620	585808	27.454 ng/ml
7) t	Ethylbenzene	13.058	184184	9.330 ng/ml
8) t	m-Xylene	13.190	368222	18.676 ng/ml
9) t	O-Xylene	13.917	356384	18.662 ng/ml
10) t	1,2,4-Trimethylbenzene	16.193	360450	18.554 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB123021\
Data File : FB026578.D
Signal(s) : FID2B.CH
Acq On : 30 Dec 2021 13:11
Operator : AJ/MA
Sample : BSF1230S1
Misc : 4.99G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 30 23:57:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
Quant Title :
QLast Update : Wed Dec 08 14:04:26 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

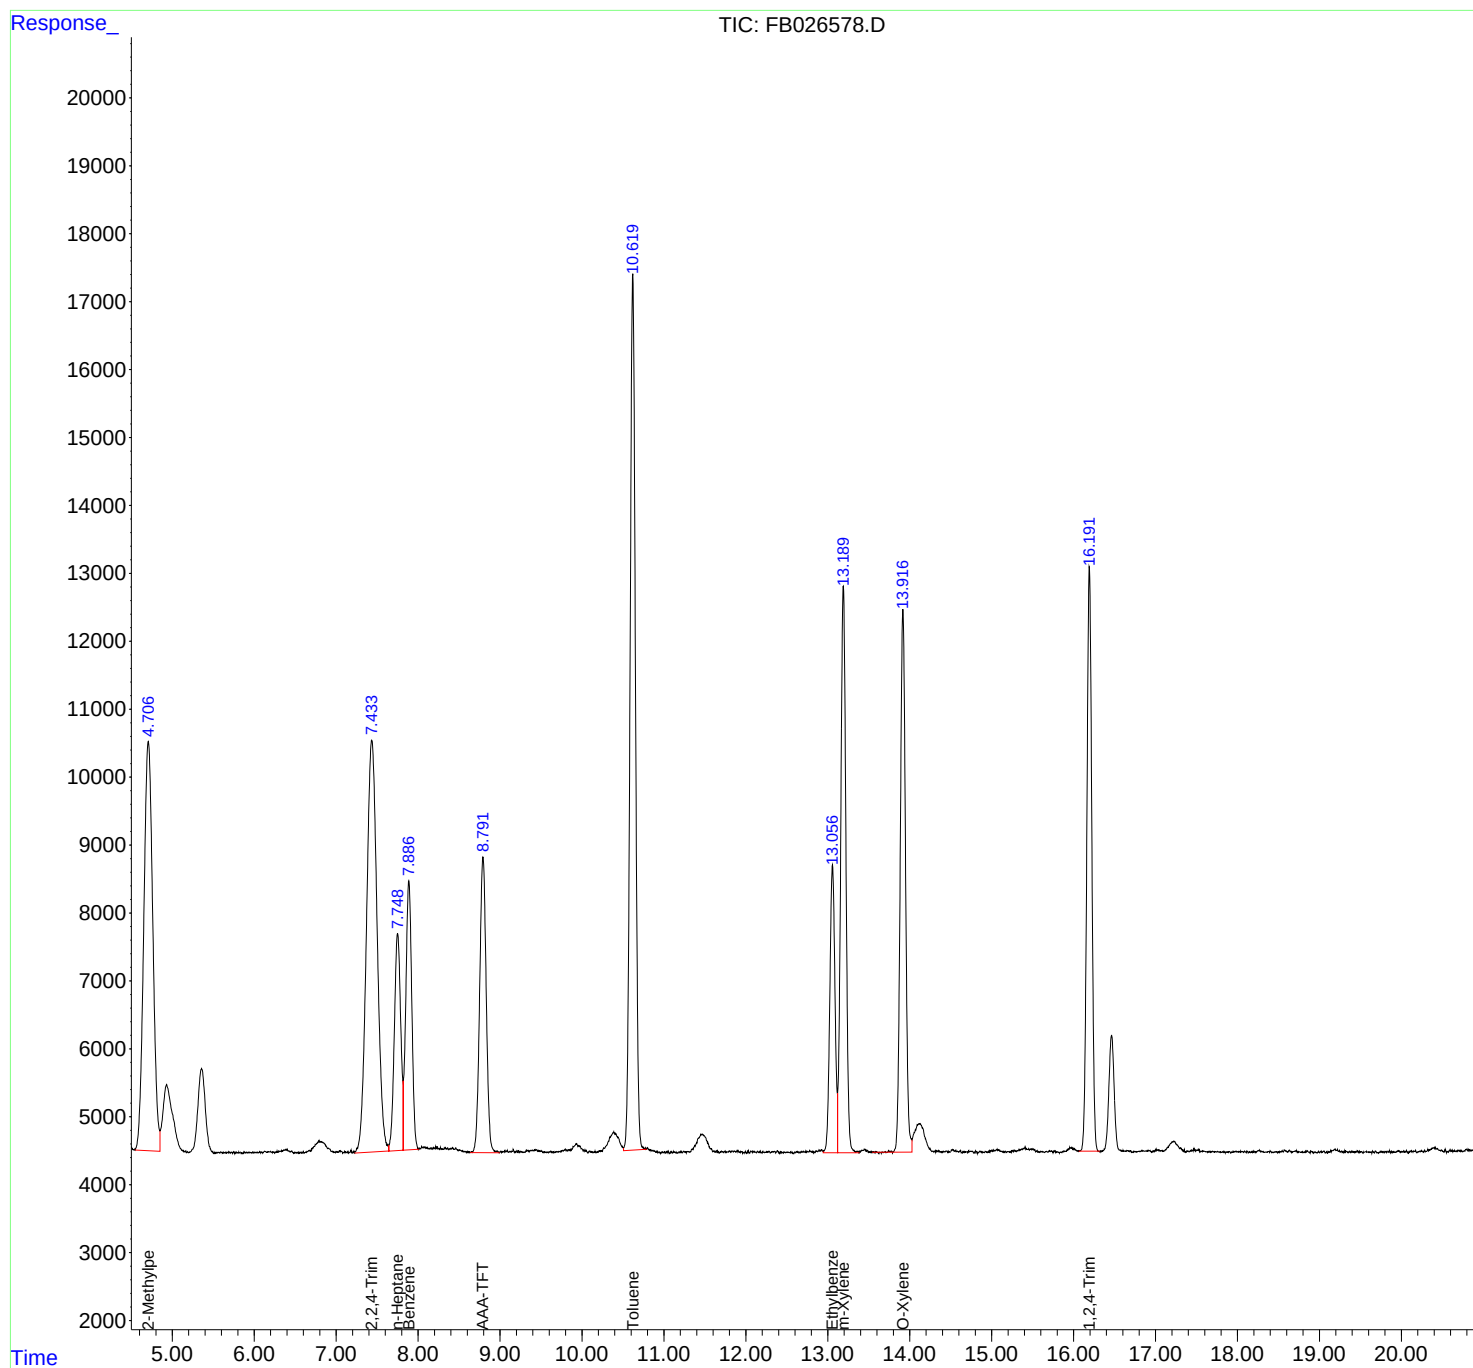

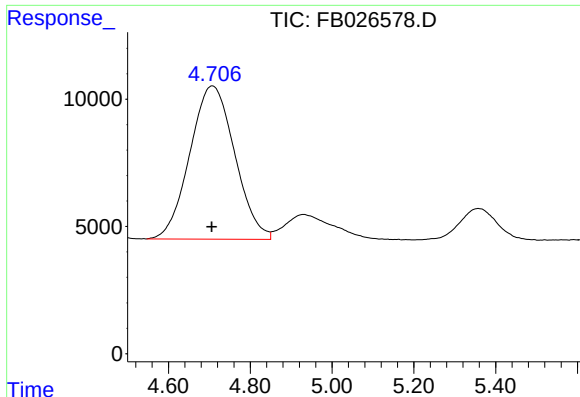


#1 2-Methylpentane

R.T.: 4.708 min
Delta R.T.: 0.002 min
Response: 459413
Conc: 26.39 ng/ml

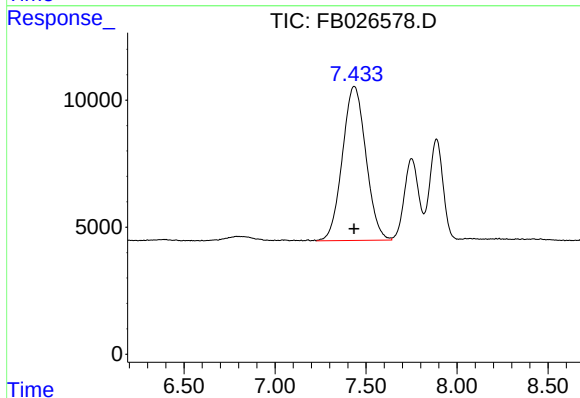


#2 2,2,4-Trimethylpentane

R.T.: 7.435 min
Delta R.T.: 0.000 min
Response: 544145
Conc: 27.44 ng/ml

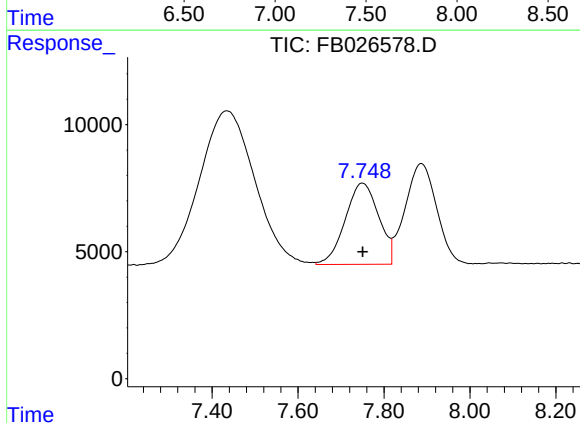


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.000 min
Response: 172968
Conc: 9.04 ng/ml

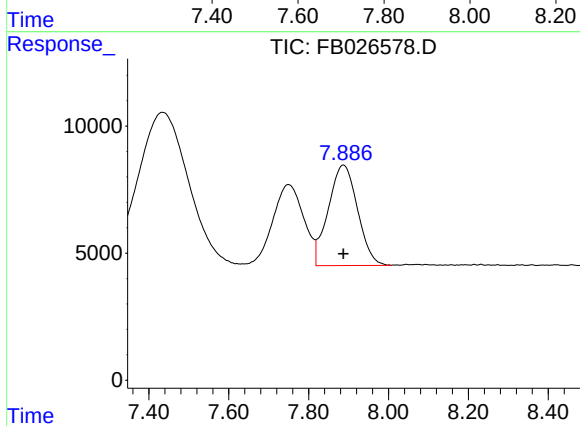


#4 Benzene

R.T.: 7.888 min
Delta R.T.: 0.000 min
Response: 201321
Conc: 9.05 ng/ml

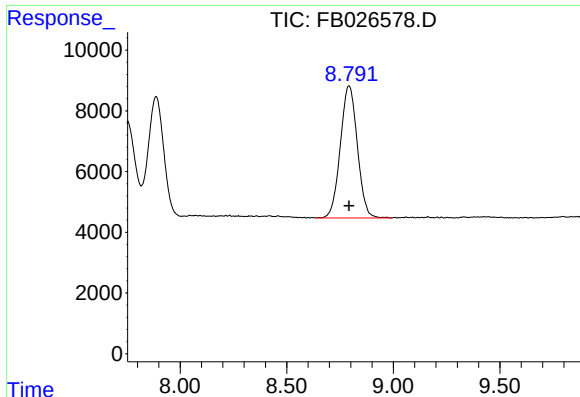


#5 AAA-TFT

R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 241493
Conc: 21.49 ng/ml

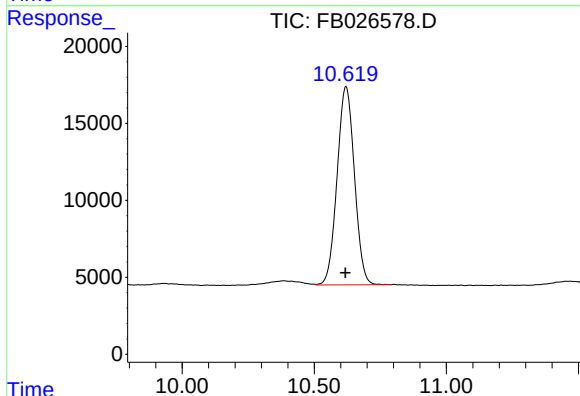


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.002 min
Response: 585808
Conc: 27.45 ng/ml

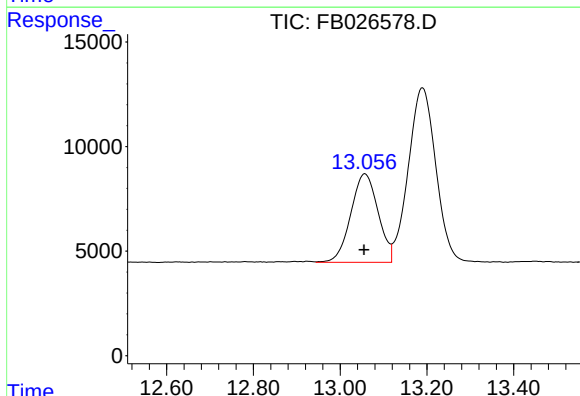


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.002 min
Response: 184184
Conc: 9.33 ng/ml

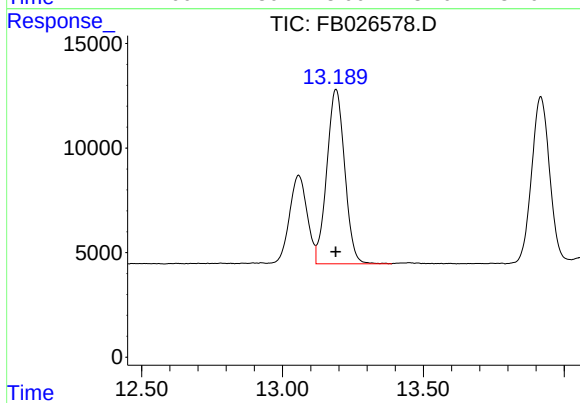


#8 m-Xylene

R.T.: 13.190 min
Delta R.T.: 0.001 min
Response: 368222
Conc: 18.68 ng/ml

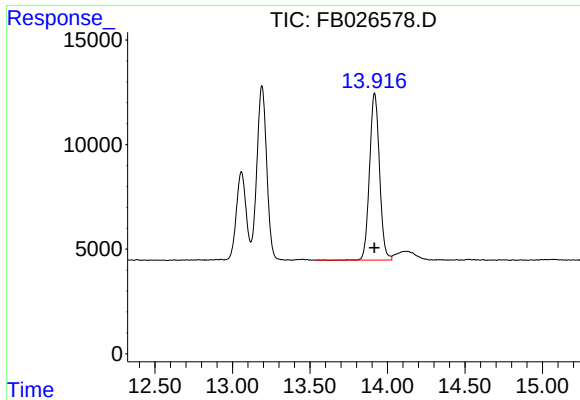

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.000 min
Response: 356384
Conc: 18.66 ng/ml

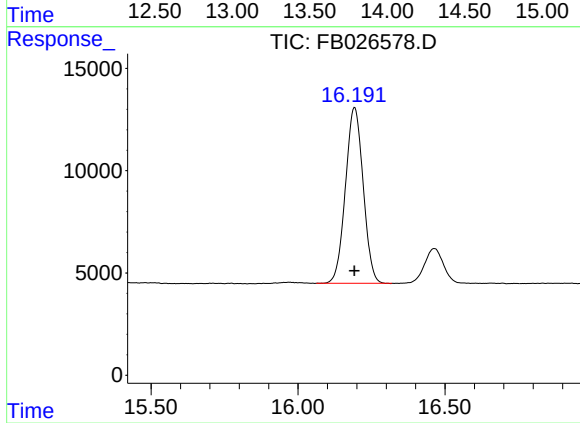

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.000 min
Response: 360450
Conc: 18.55 ng/ml