

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB123021\
 Data File : FB026582.D
 Signal(s) : FID2B.CH
 Acq On : 30 Dec 2021 15:35
 Operator : AJ/MA
 Sample : 20 PPB GRO STD
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Dec 30 23:58:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
 Quant Title :
 QLast Update : Wed Dec 08 14:04:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	231038	20.564 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	465874	26.764 ng/ml
2) t 2,2,4-Trimethylpentane	7.441	547255	27.595 ng/ml
3) t n-Heptane	7.753	175876	9.188 ng/ml
4) t Benzene	7.888	206422	9.284 ng/ml
6) t Toluene	10.621	586982	27.509 ng/ml
7) t Ethylbenzene	13.058	183418	9.291 ng/ml
8) t m-Xylene	13.191	366012	18.564 ng/ml
9) t O-Xylene	13.918	353119	18.491 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	349506	17.991 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB123021\
Data File : FB026582.D
Signal(s) : FID2B.CH
Acq On : 30 Dec 2021 15:35
Operator : AJ/MA
Sample : 20 PPB GRO STD
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Dec 30 23:58:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB120821.M
Quant Title :
QLast Update : Wed Dec 08 14:04:26 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

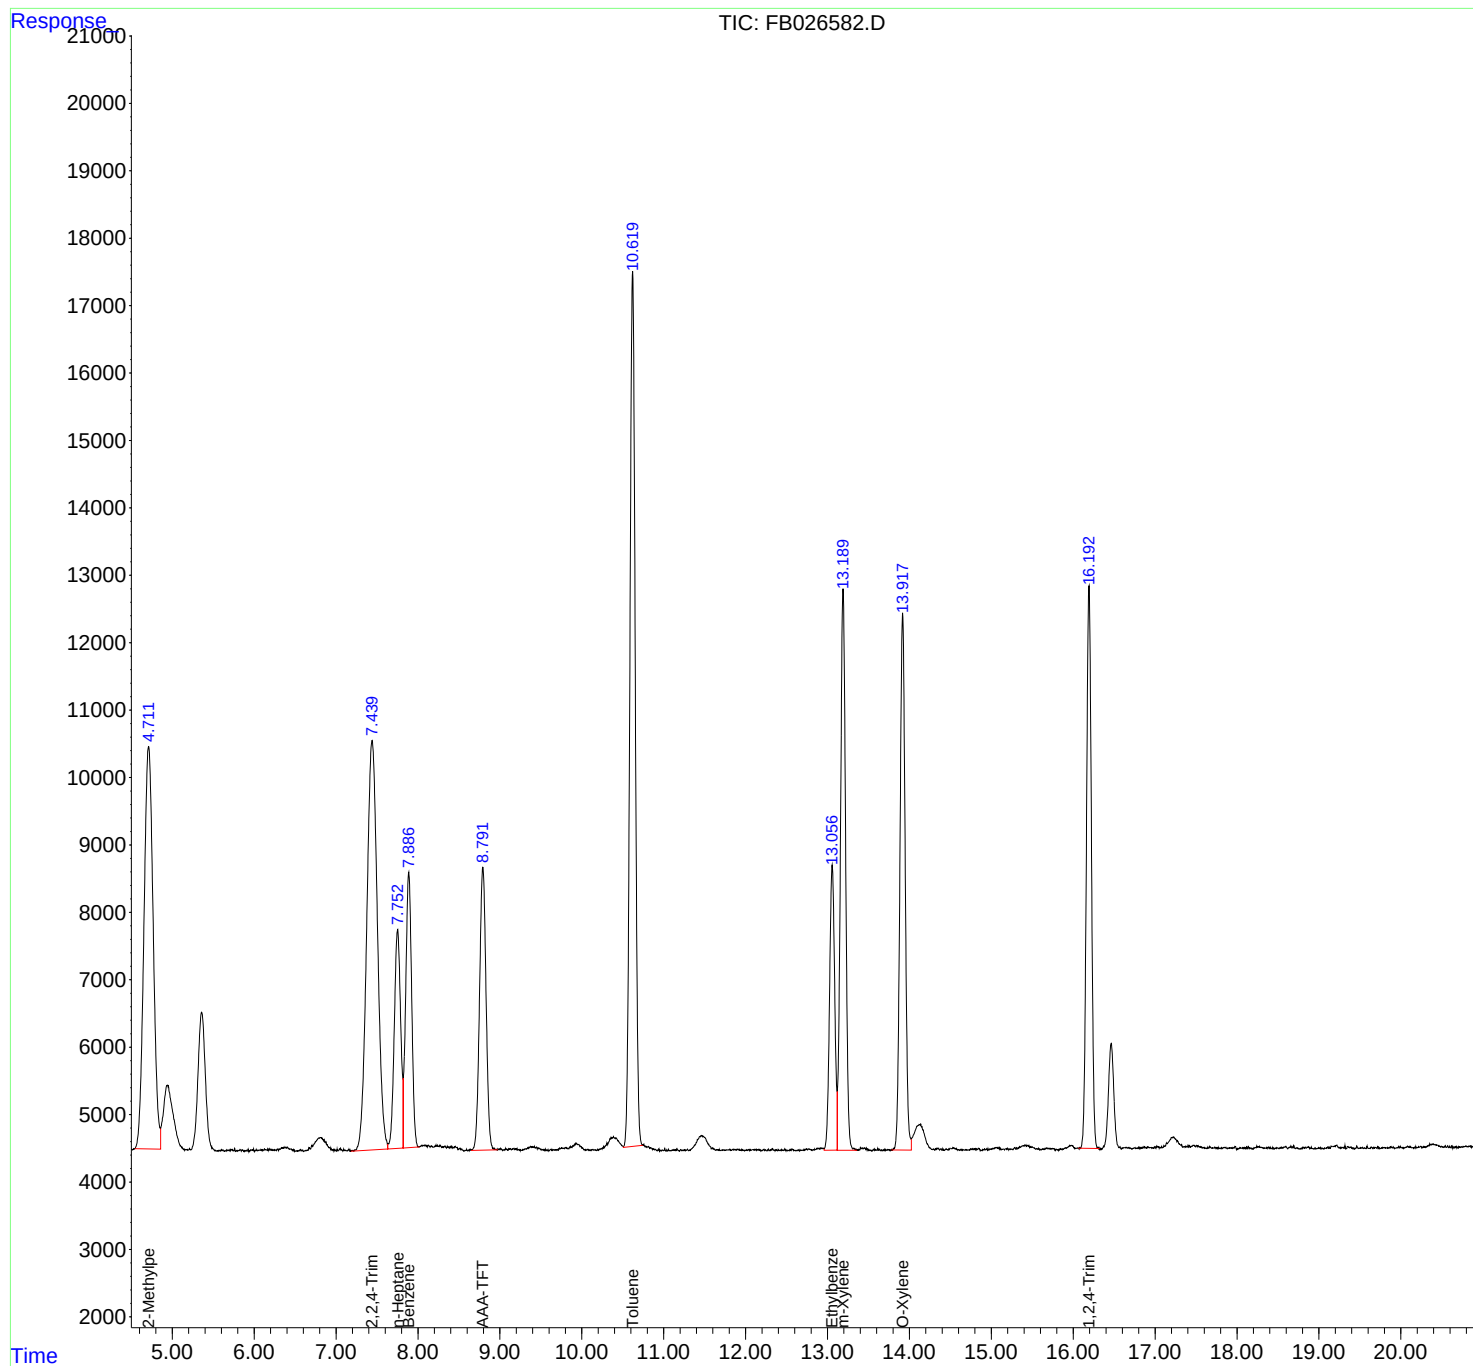

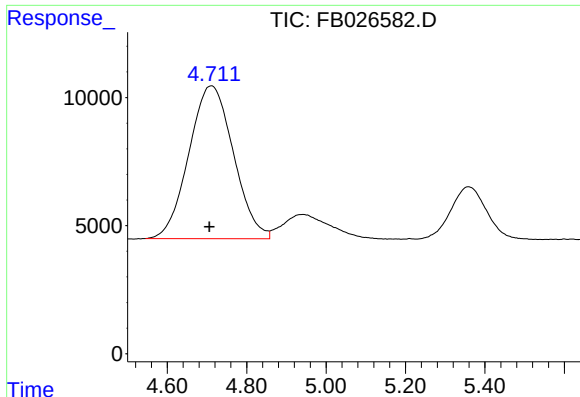


#1 2-Methylpentane

R.T.: 4.712 min
Delta R.T.: 0.006 min
Response: 465874
Conc: 26.76 ng/ml

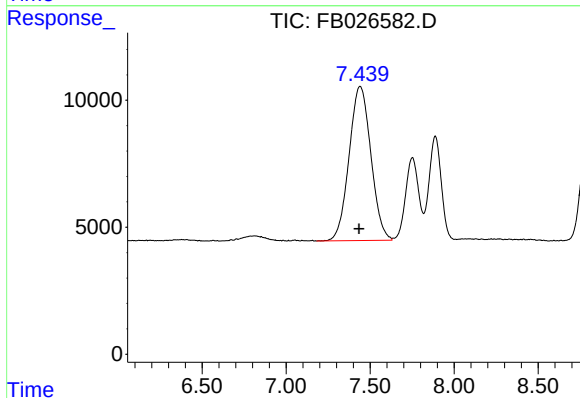


#2 2,2,4-Trimethylpentane

R.T.: 7.441 min
Delta R.T.: 0.005 min
Response: 547255
Conc: 27.60 ng/ml

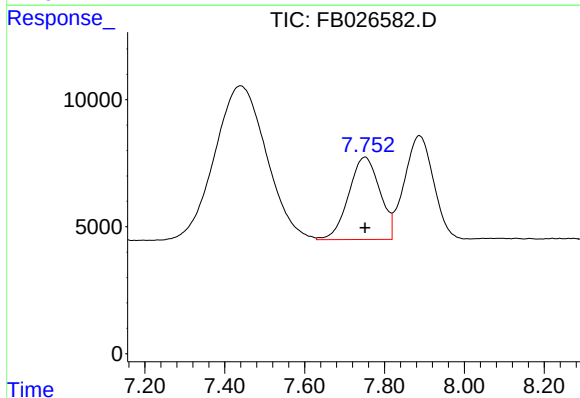


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: 0.002 min
Response: 175876
Conc: 9.19 ng/ml

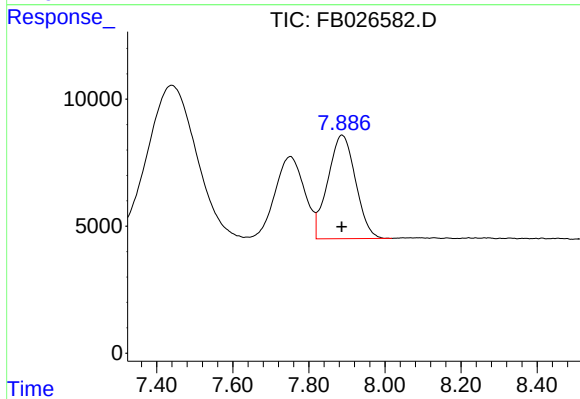


#4 Benzene

R.T.: 7.888 min
Delta R.T.: 0.000 min
Response: 206422
Conc: 9.28 ng/ml

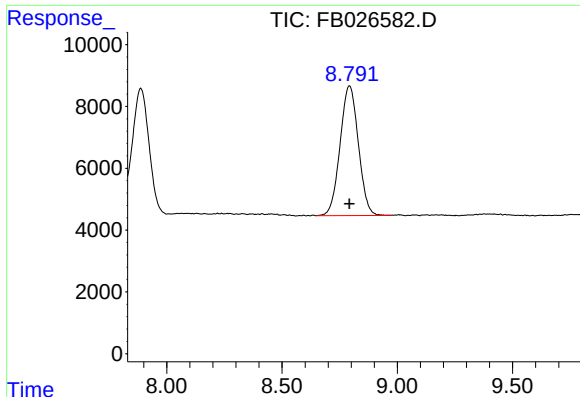


#5 AAA-TFT

R.T.: 8.793 min
Delta R.T.: 0.000 min
Response: 231038
Conc: 20.56 ng/ml

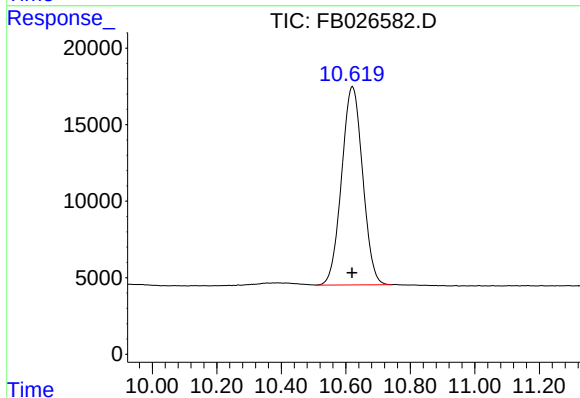


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.002 min
Response: 586982
Conc: 27.51 ng/ml

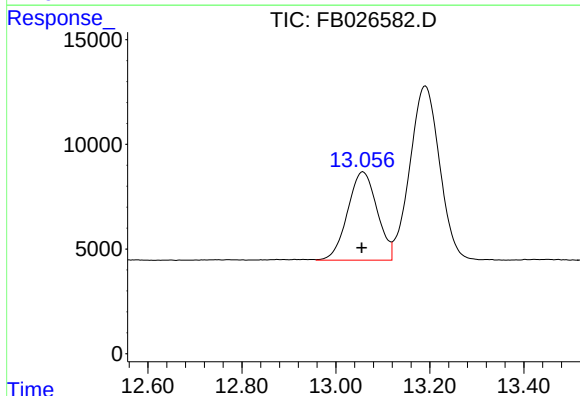


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.002 min
Response: 183418
Conc: 9.29 ng/ml

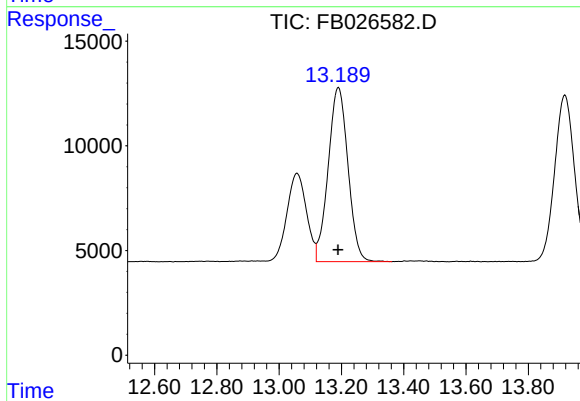


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: 0.001 min
Response: 366012
Conc: 18.56 ng/ml

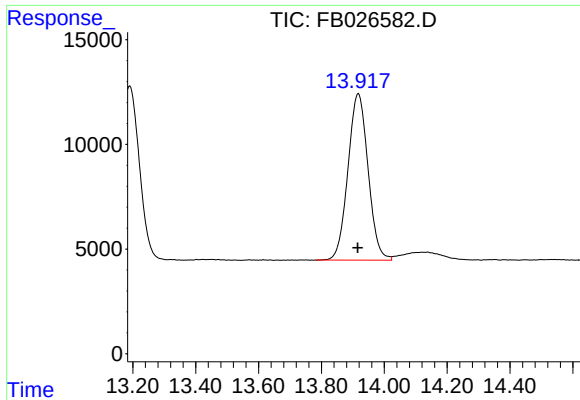

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.002 min
Response: 353119
Conc: 18.49 ng/ml

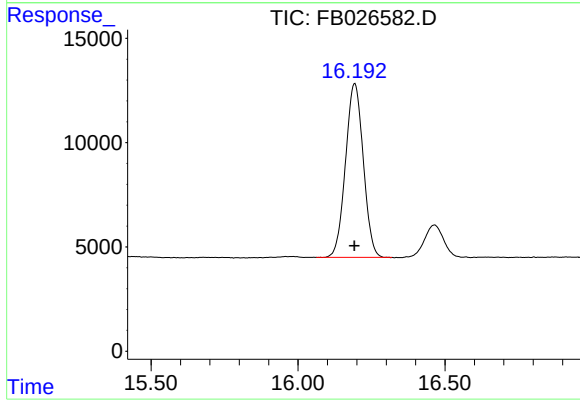

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.001 min
Response: 349506
Conc: 17.99 ng/ml