

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062618\
 Data File : FB016401.D
 Signal(s) : FID2B.CH
 Acq On : 26 Jun 2018 20:20
 Operator : MJ/SJ
 Sample : J3240-05MSD
 Misc : 5.02g/5.00mL DI Water
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Jun 27 09:34:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
 Quant Title :
 QLast Update : Fri Jun 01 13:25:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.116	151665	21.581 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.968	305941	25.230 ng/ml
2) t 2,2,4-Trimethylpentane	7.734	324404	28.012 ng/ml
3) t n-Heptane	8.072	92529	8.455 ng/ml
4) t Benzene	8.210	168032	11.317 ng/ml
6) t Toluene	10.965	331316	26.692 ng/ml
7) t Ethylbenzene	13.413	129758	9.270 ng/ml
8) t m-Xylene	13.547	276399	18.159 ng/ml
9) t O-Xylene	14.278	297182	19.044 ng/ml
10) t 1,2,4-Trimethylbenzene	16.560	330608	19.196 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB062618\
Data File : FB016401.D
Signal(s) : FID2B.CH
Acq On : 26 Jun 2018 20:20
Operator : MJ/SJ
Sample : J3240-05MSD
Misc : 5.02g/5.00mL DI Water
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Jun 27 09:34:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB060118.M
Quant Title :
QLast Update : Fri Jun 01 13:25:03 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

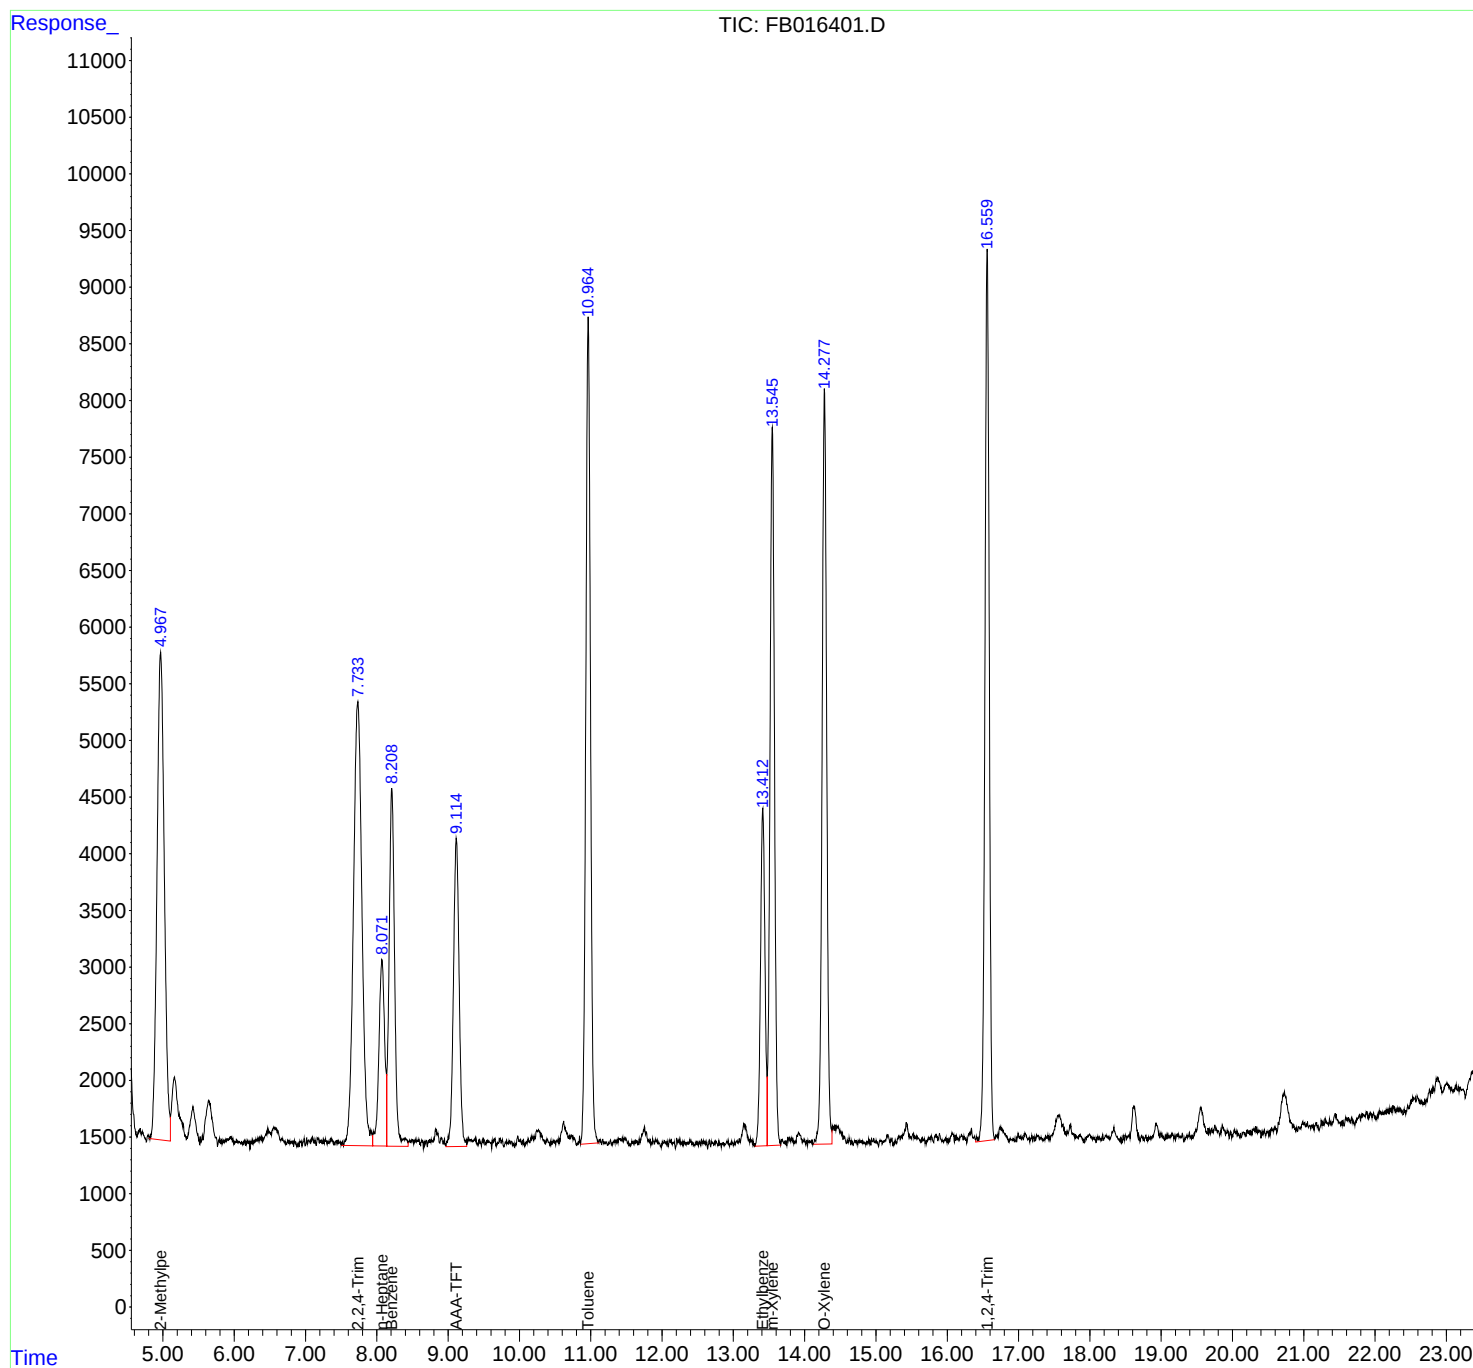

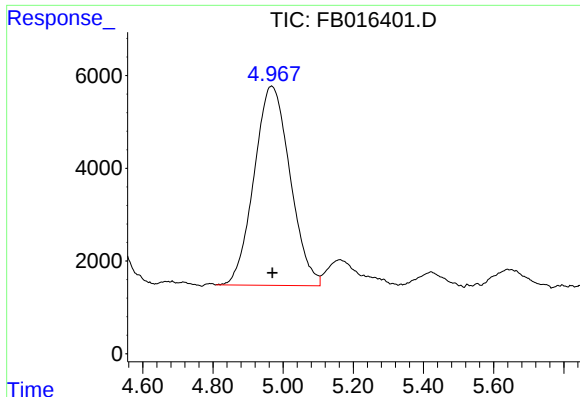


#1 2-Methylpentane

R.T.: 4.968 min
Delta R.T.: -0.001 min
Response: 305941
Conc: 25.23 ng/ml

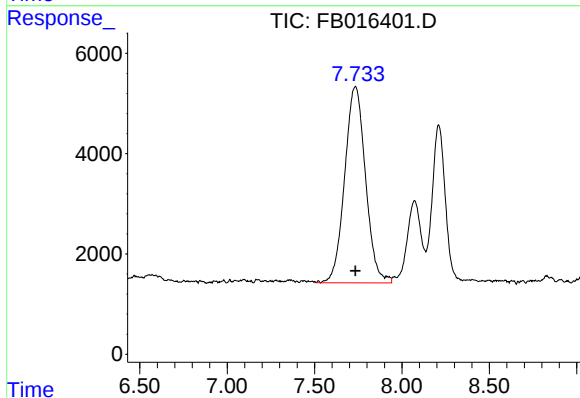


#2 2,2,4-Trimethylpentane

R.T.: 7.734 min
Delta R.T.: 0.000 min
Response: 324404
Conc: 28.01 ng/ml

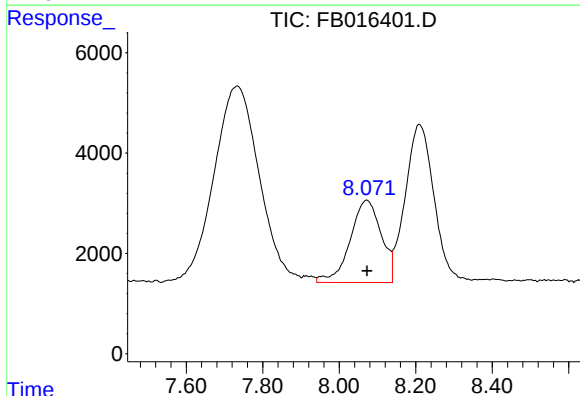


#3 n-Heptane

R.T.: 8.072 min
Delta R.T.: 0.000 min
Response: 92529
Conc: 8.45 ng/ml

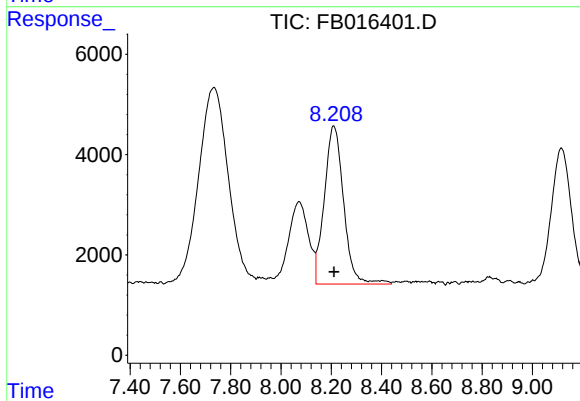


#4 Benzene

R.T.: 8.210 min
Delta R.T.: -0.001 min
Response: 168032
Conc: 11.32 ng/ml

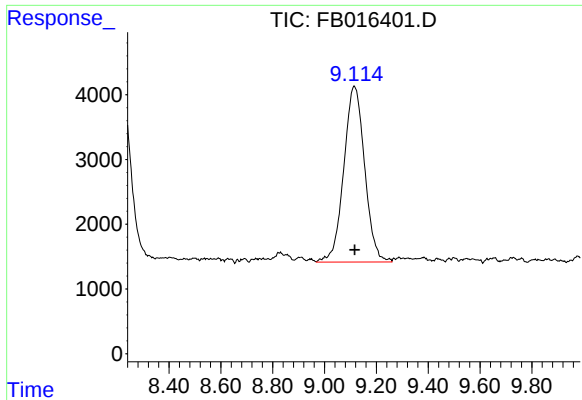


#5 AAA-TFT

R.T.: 9.116 min
Delta R.T.: -0.001 min
Response: 151665
Conc: 21.58 ng/ml

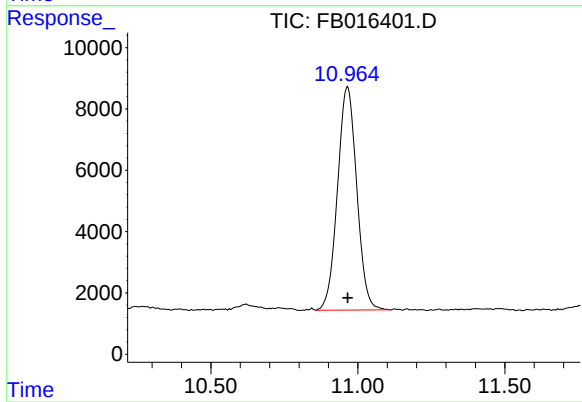


#6 Toluene

R.T.: 10.965 min
Delta R.T.: 0.000 min
Response: 331316
Conc: 26.69 ng/ml

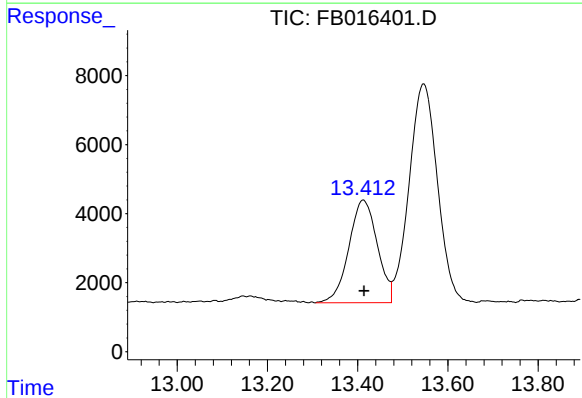


#7 Ethylbenzene

R.T.: 13.413 min
Delta R.T.: -0.001 min
Response: 129758
Conc: 9.27 ng/ml

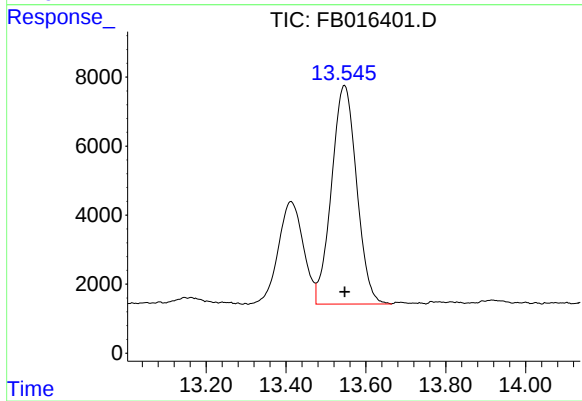

#8 m-Xylene

R.T.: 13.547 min
Delta R.T.: 0.000 min
Response: 276399
Conc: 18.16 ng/ml

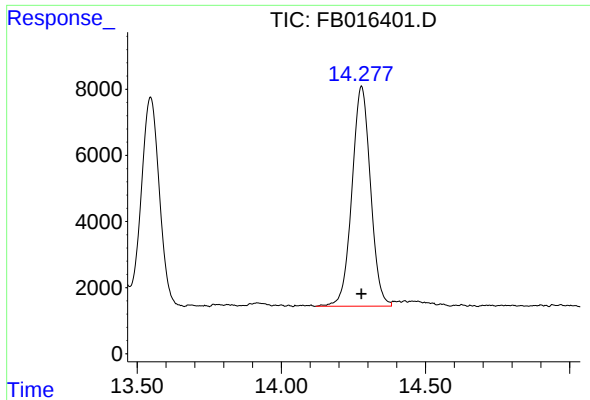


#9 O-Xylene

R.T.: 14.278 min

Delta R.T.: 0.000 min

Response: 297182

Conc: 19.04 ng/ml

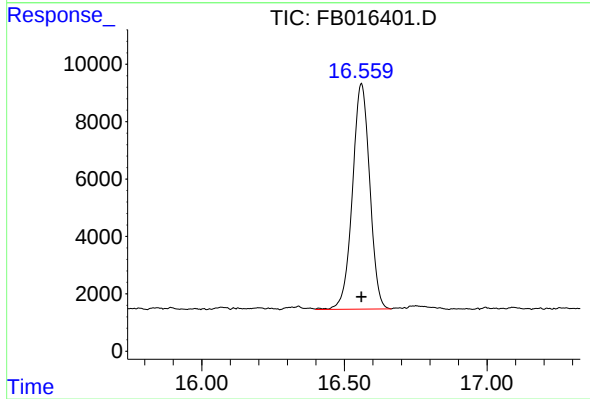

#10 1,2,4-Trimethylbenzene

R.T.: 16.560 min

Delta R.T.: 0.000 min

Response: 330608

Conc: 19.20 ng/ml