

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB082219\  
Data File : FB022075.D  
Signal(s) : FID2B.CH  
Acq On : 22 Aug 2019 13:23  
Operator : DD/AJ  
Sample : K4087-02  
Misc : 5.02/5.00ml DI WATER  
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Aug 23 02:10:51 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB082019.M  
Quant Title :  
QLast Update : Wed Aug 21 07:59:08 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                    | R.T.  | Response | Conc Units   |
|-----------------------------|-------|----------|--------------|
| -----                       |       |          |              |
| System Monitoring Compounds |       |          |              |
| 5) s AAA-TFT                | 8.986 | 418747   | 19.715 ng/ml |

Target Compounds

-----


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB082219\  
Data File : FB022075.D  
Signal(s) : FID2B.CH  
Acq On : 22 Aug 2019 13:23  
Operator : DD/AJ  
Sample : K4087-02  
Misc : 5.02/5.00ml DI WATER  
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e  
Quant Time: Aug 23 02:10:51 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB082019.M  
Quant Title :  
QLast Update : Wed Aug 21 07:59:08 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

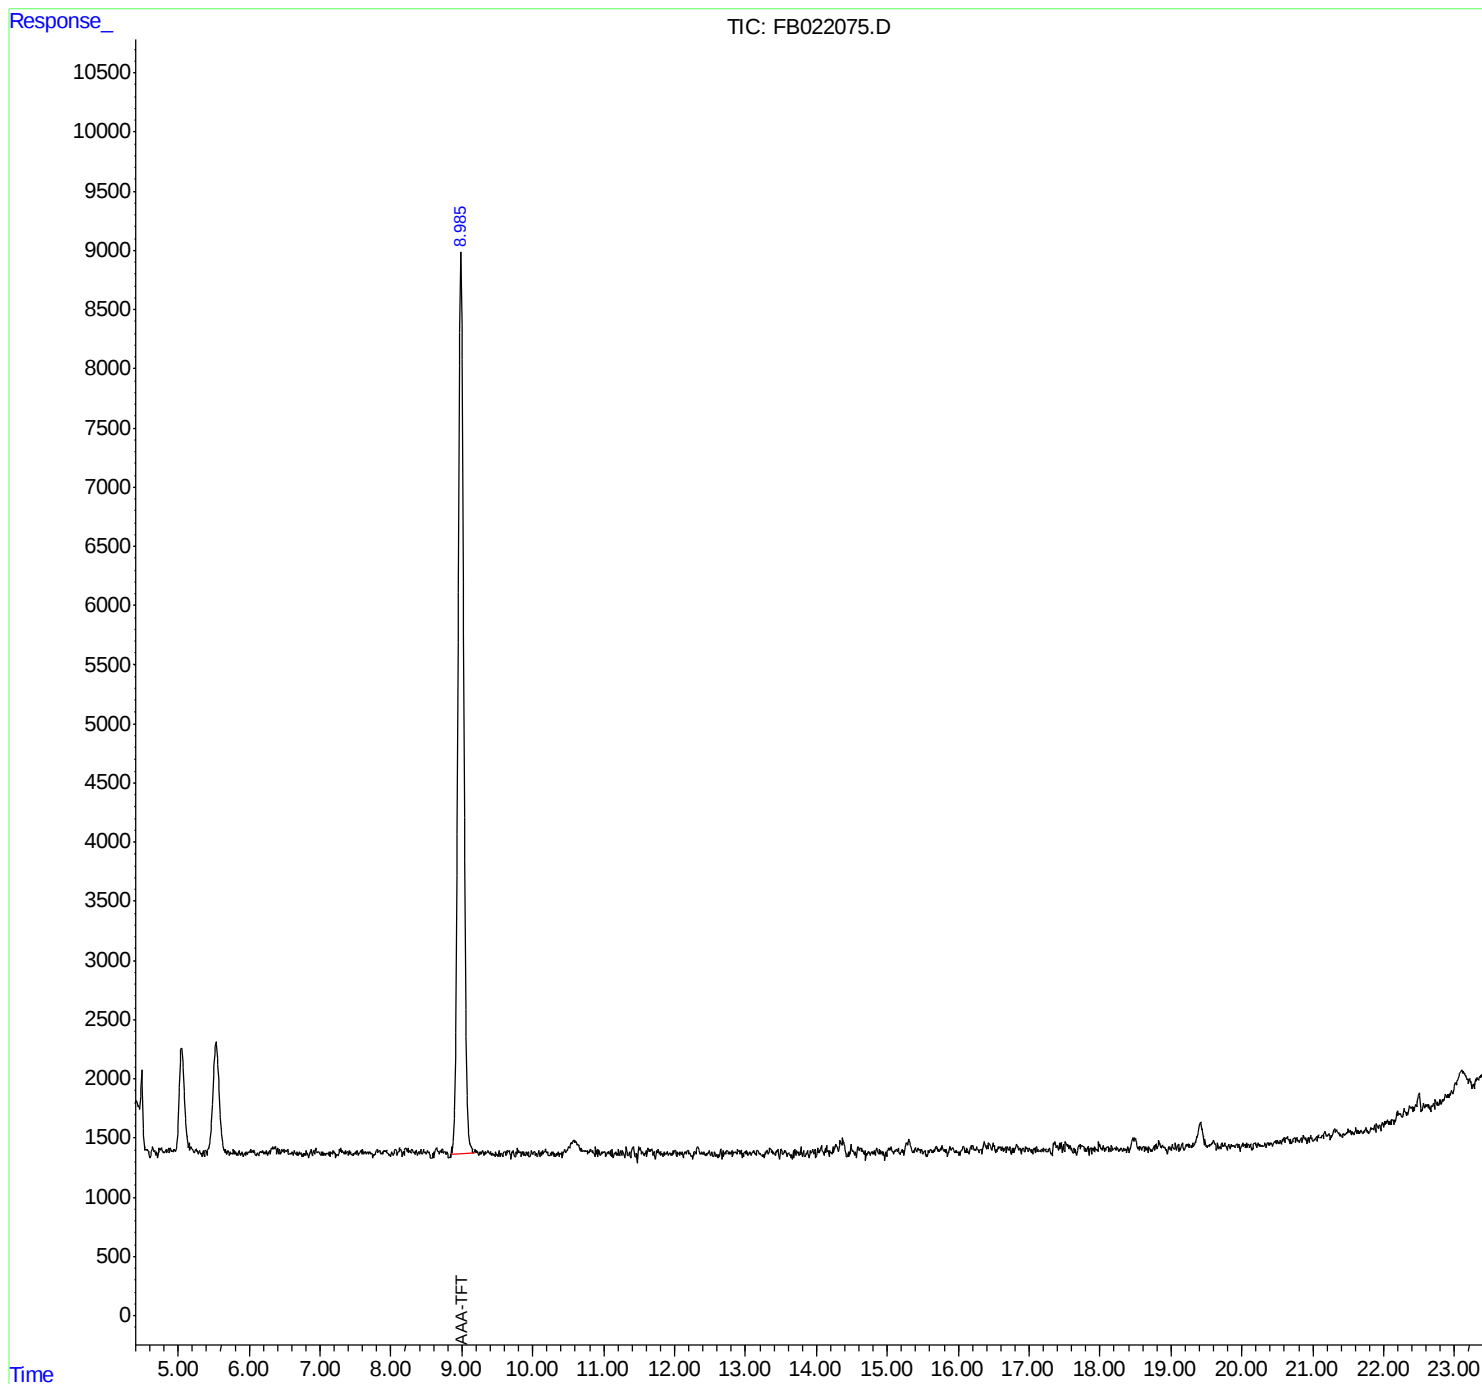

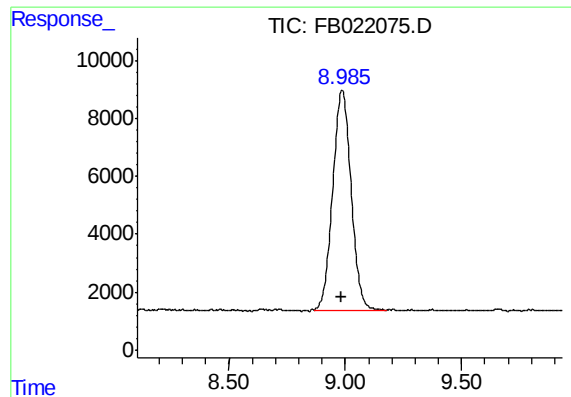

#5 AAA-TFT

R.T.: 8.986 min  
Delta R.T.: 0.004 min  
Response: 418747  
Conc: 19.71 ng/ml