

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082219\
 Data File : FB022077.D
 Signal(s) : FID2B.CH
 Acq On : 22 Aug 2019 14:26
 Operator : DD/AJ
 Sample : K4401-01MSD
 Misc : 5.03/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Aug 23 02:11:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
 Quant Title :
 QLast Update : Wed Aug 21 07:59:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.988	384247	18.091 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.859	881043	22.014 ng/ml
2) t	2,2,4-Trimethylpentane	7.608	714550	17.741 ng/ml
3) t	n-Heptane	7.947	236477	6.191 ng/ml
4) t	Benzene	8.083	400713	8.926 ng/ml
6) t	Toluene	10.829	808835	26.310 ng/ml
7) t	Ethylbenzene	13.274	183153	8.975 ng/ml
8) t	m-Xylene	13.407	381538	18.116 ng/ml
9) t	O-Xylene	14.137	406453	18.174 ng/ml
10) t	1,2,4-Trimethylbenzene	16.416	439203	17.126 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB082219\
Data File : FB022077.D
Signal(s) : FID2B.CH
Acq On : 22 Aug 2019 14:26
Operator : DD/AJ
Sample : K4401-01MSD
Misc : 5.03/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Aug 23 02:11:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB082019.M
Quant Title :
QLast Update : Wed Aug 21 07:59:08 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

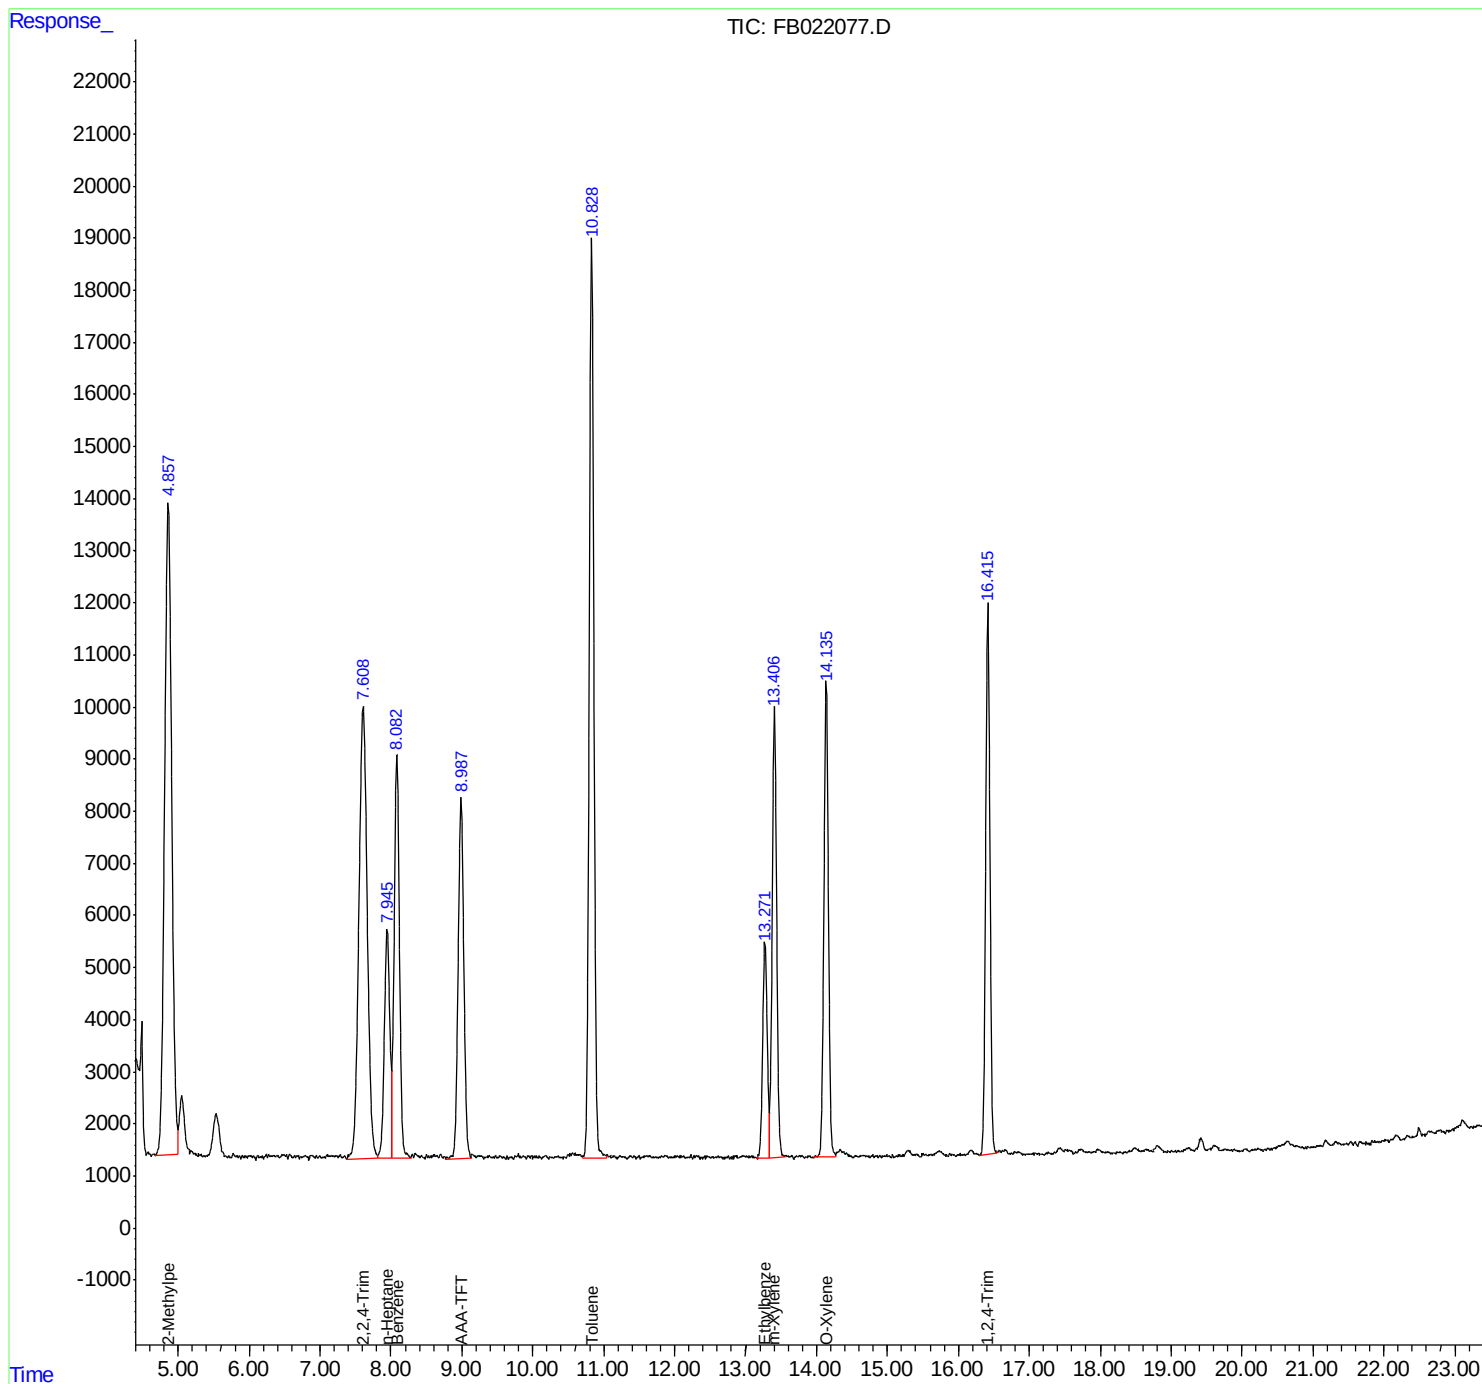

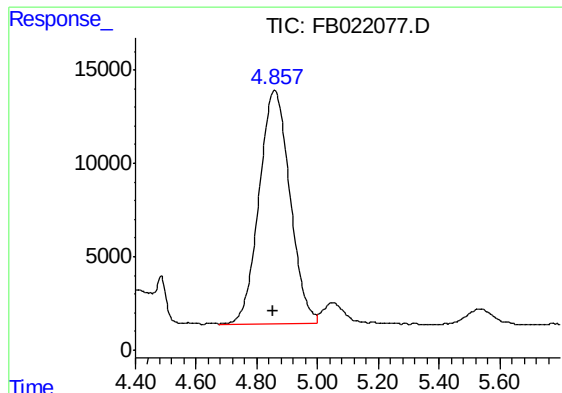


#1 2-Methylpentane

R.T.: 4.859 min
Delta R.T.: 0.007 min
Response: 881043
Conc: 22.01 ng/ml

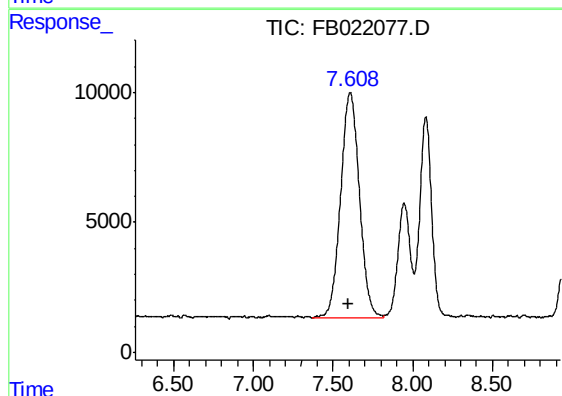


#2 2,2,4-Trimethylpentane

R.T.: 7.608 min
Delta R.T.: 0.008 min
Response: 714550
Conc: 17.74 ng/ml

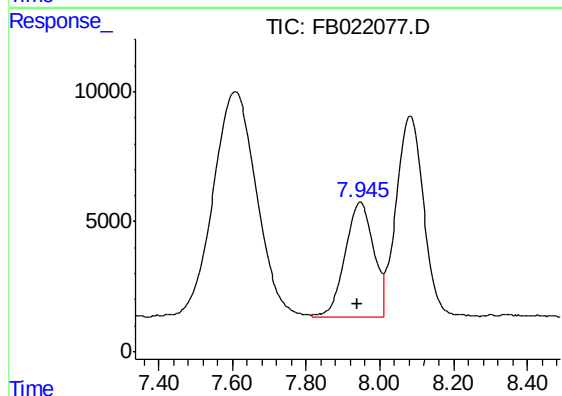


#3 n-Heptane

R.T.: 7.947 min
Delta R.T.: 0.005 min
Response: 236477
Conc: 6.19 ng/ml

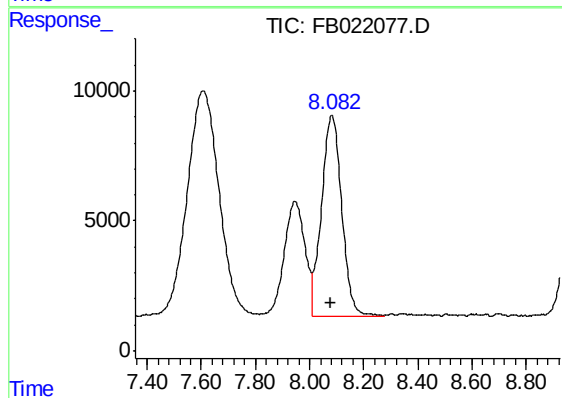


#4 Benzene

R.T.: 8.083 min
Delta R.T.: 0.006 min
Response: 400713
Conc: 8.93 ng/ml

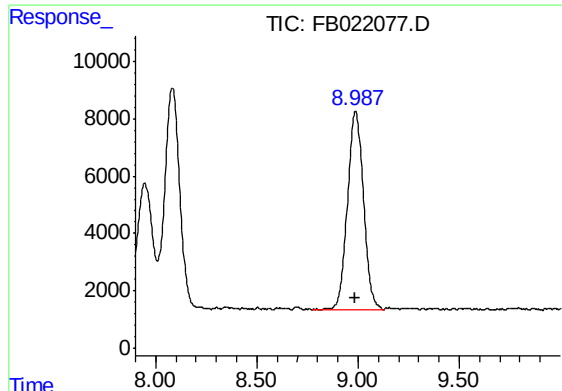


#5 AAA-TFT

R.T.: 8.988 min
Delta R.T.: 0.006 min
Response: 384247
Conc: 18.09 ng/ml

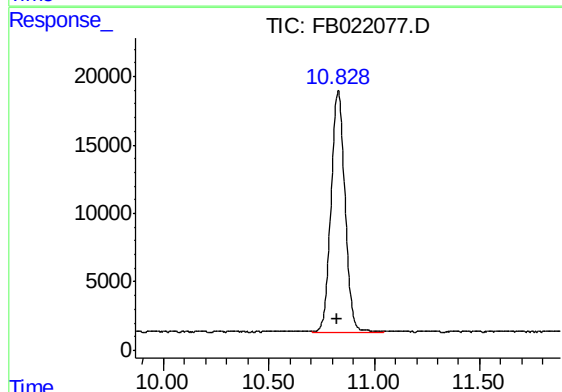


#6 Toluene

R.T.: 10.829 min
Delta R.T.: 0.006 min
Response: 808835
Conc: 26.31 ng/ml

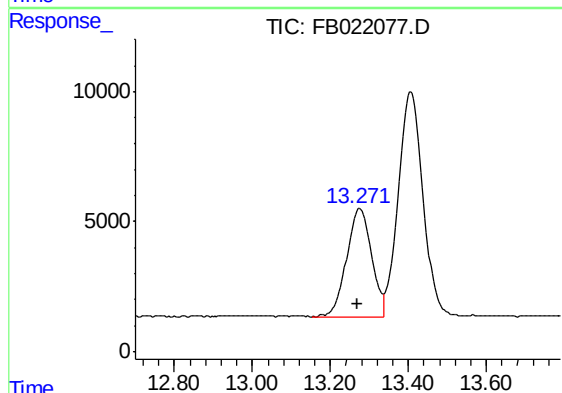


#7 Ethylbenzene

R.T.: 13.274 min
Delta R.T.: 0.005 min
Response: 183153
Conc: 8.98 ng/ml

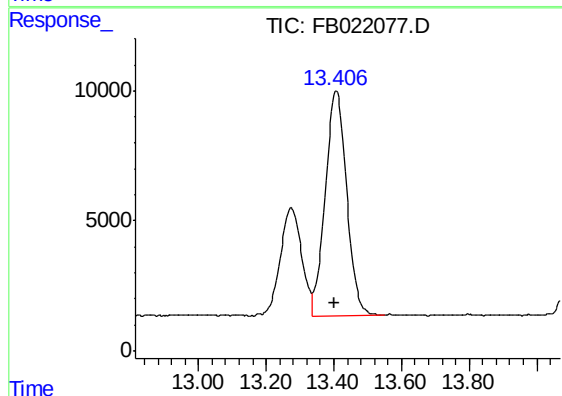


#8 m-Xylene

R.T.: 13.407 min
Delta R.T.: 0.006 min
Response: 381538
Conc: 18.12 ng/ml

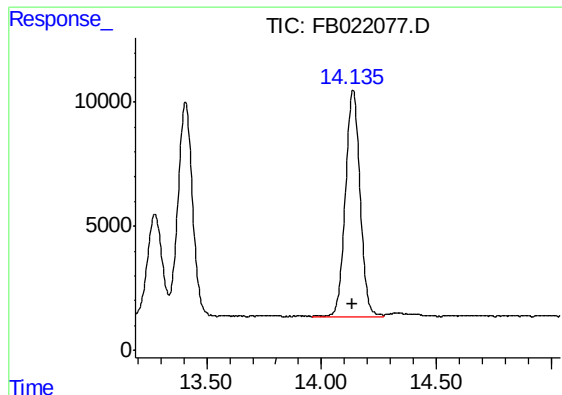

#9 O-Xylene

R.T.: 14.137 min
Delta R.T.: 0.005 min
Response: 406453
Conc: 18.17 ng/ml

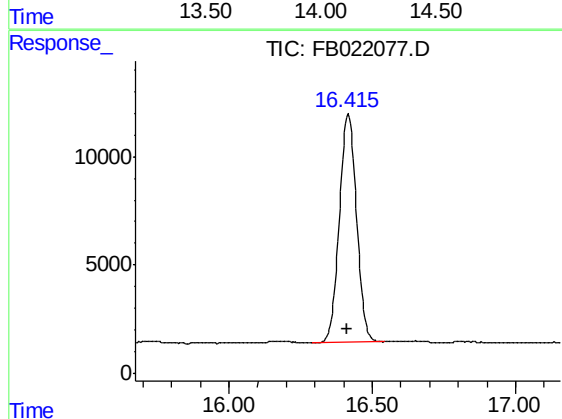

#10 1,2,4-Trimethylbenzene

R.T.: 16.416 min
Delta R.T.: 0.005 min
Response: 439203
Conc: 17.13 ng/ml