

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031721\
 Data File : FB025538.D
 Signal(s) : FID2B.CH
 Acq On : 17 Mar 2021 16:12
 Operator : DD/AJ
 Sample : M1687-01
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 AUD-1052-1053

Manual Integrations
 APPROVED

Ankita
 3/22/2021 10:49:42 AM

Integration File: Calibration.e
 Quant Time: Mar 18 01:53:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031621.M
 Quant Title :
 QLast Update : Wed Mar 17 08:44:23 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.871	10578855	505.368 ng/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB031721\
Data File : FB025538.D
Signal(s) : FID2B.CH
Acq On : 17 Mar 2021 16:12
Operator : DD/AJ
Sample : M1687-01
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 16 Sample Multiplier: 1


Instrument :
FID_B
ClientSampleId :
AUD-1052-1053


Manual Integrations
APPROVED

Ankita
3/22/2021 10:49:42 AM

Integration File: Calibration.e
Quant Time: Mar 18 01:53:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB031621.M
Quant Title :
QLast Update : Wed Mar 17 08:44:23 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

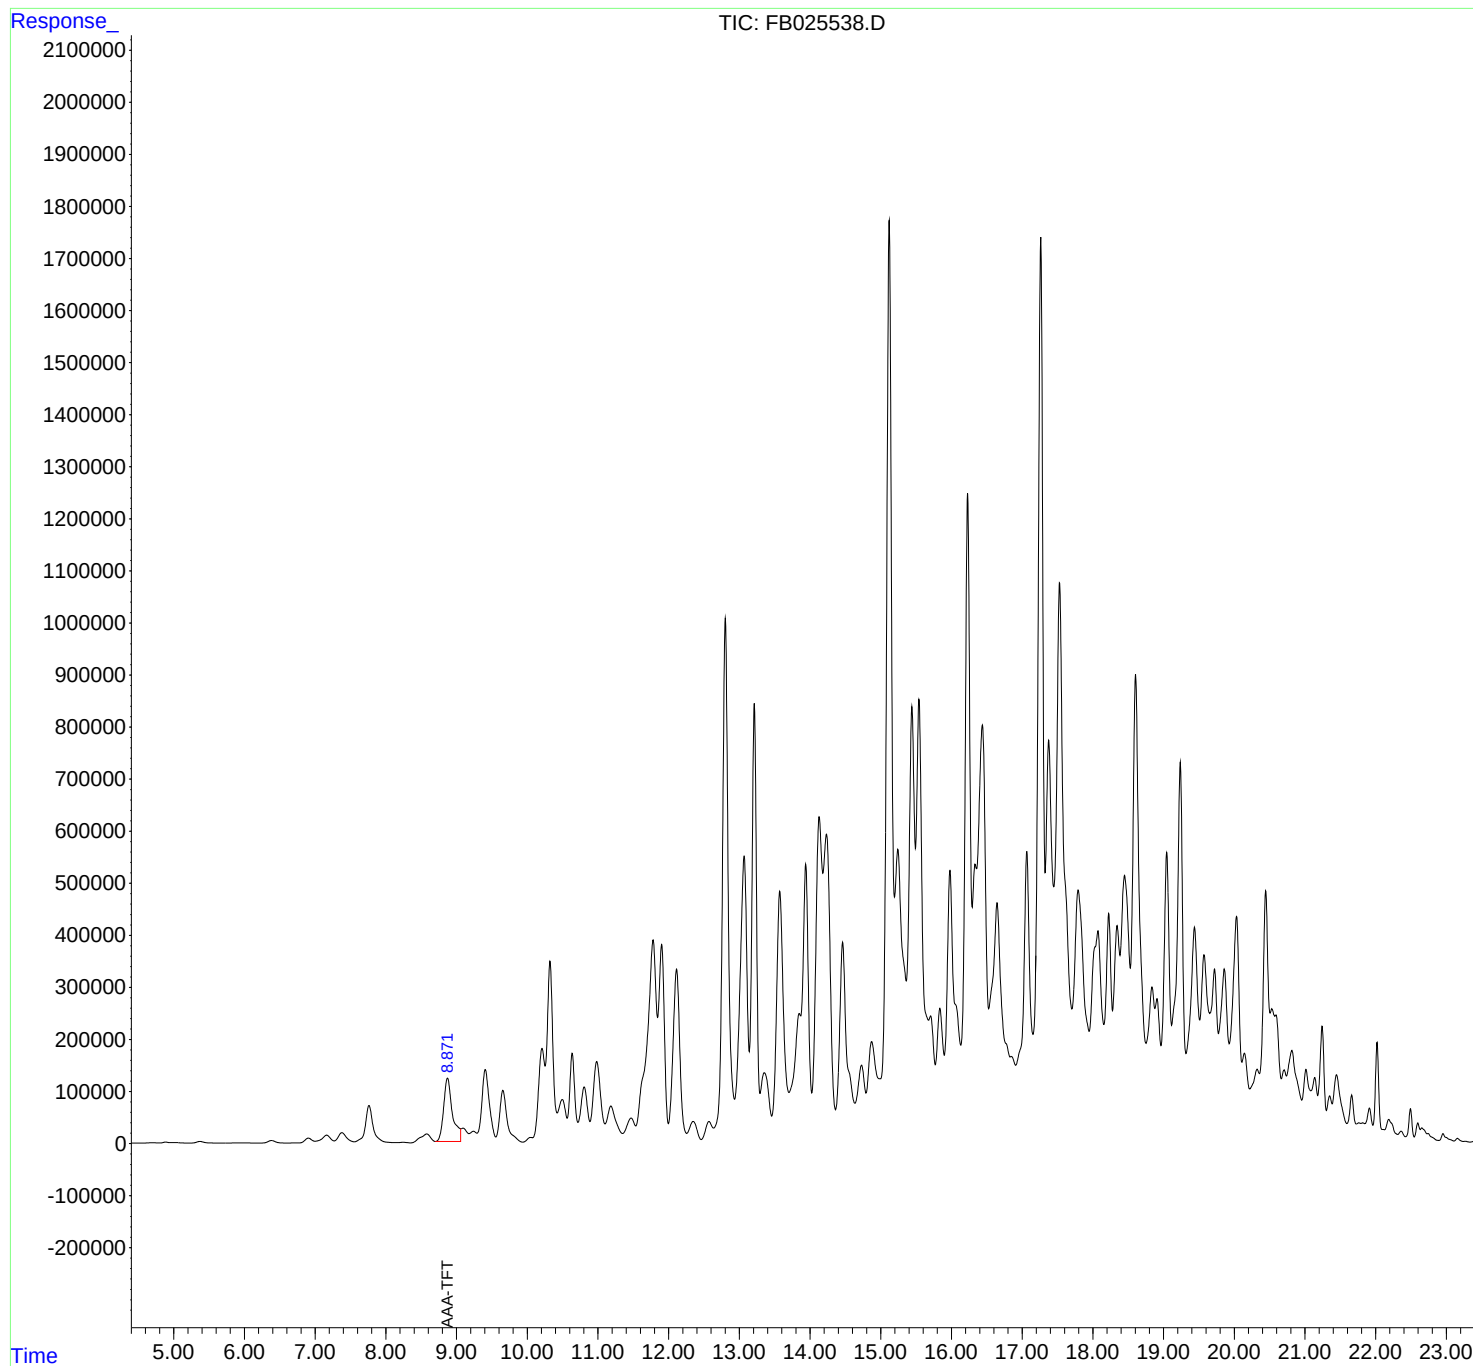

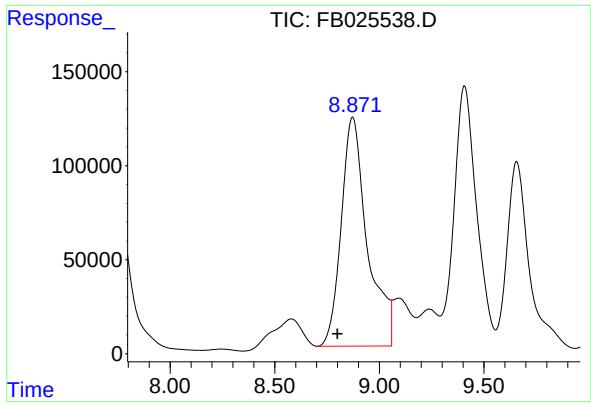

#5 AAA-TFT

R.T.: 8.871 min

Delta R.T.: 0.071 min

Response: 10578855

Conc: 505.37 ng/ml m

Instrument :
FID_B
ClientSampleId :
AUD-1052-1053

Manual Integrations
APPROVED

Ankita
3/22/2021 10:49:42 AM